
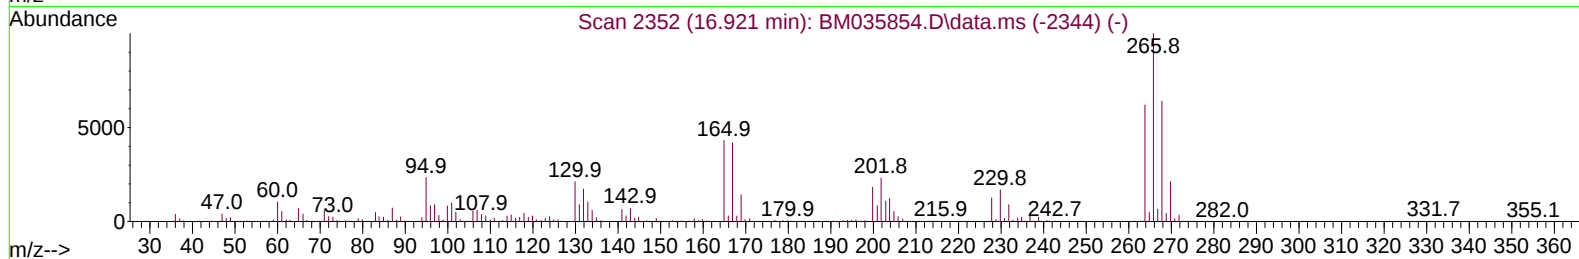
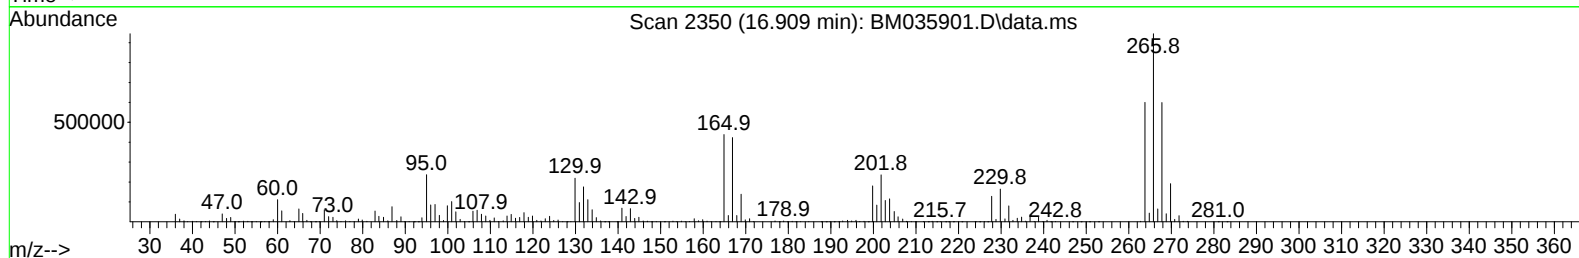


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072222\
Data File : BM035901.D
Acq On : 22 Jul 2022 10:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 14:34:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 22 14:25:12 2022
Response via : Initial Calibration

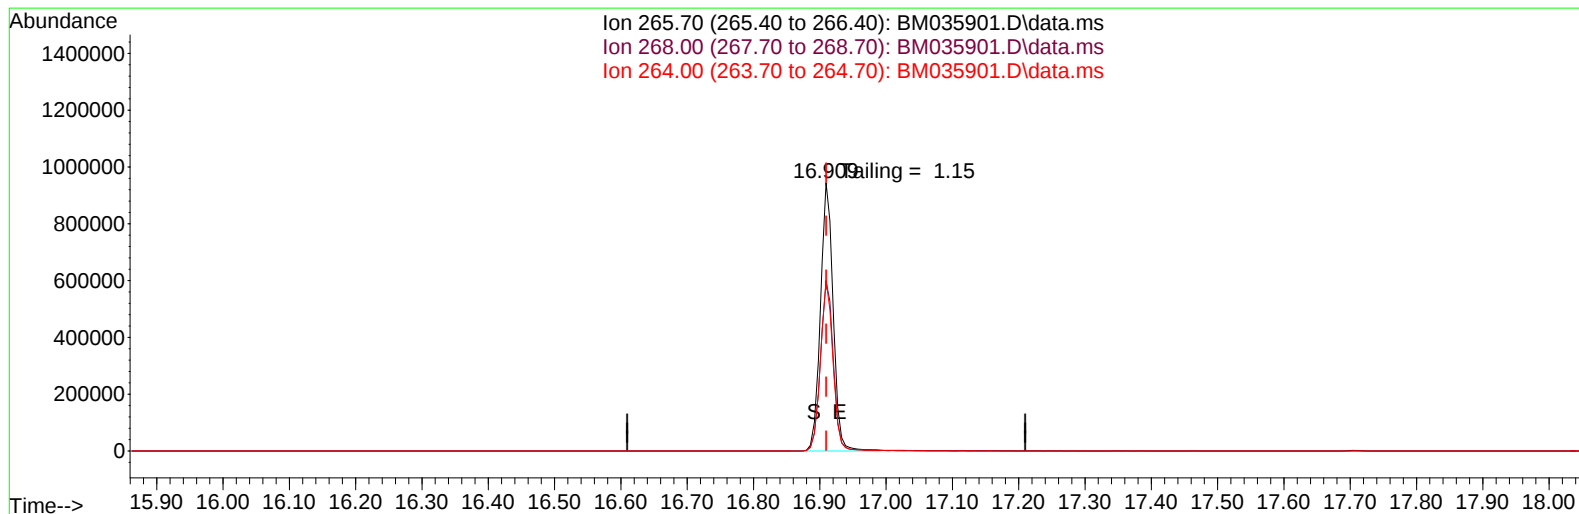

TIC: BM035901.D\data.ms

(70) Pentachlorophenol (C)




16.909min (-0.000) 970845.89 ng

response 1269911

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.39
264.00	63.30	63.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072222\
 Data File : BM035901.D
 Acq On : 22 Jul 2022 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 14:34:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 22 14:25:12 2022
 Response via : Initial Calibration

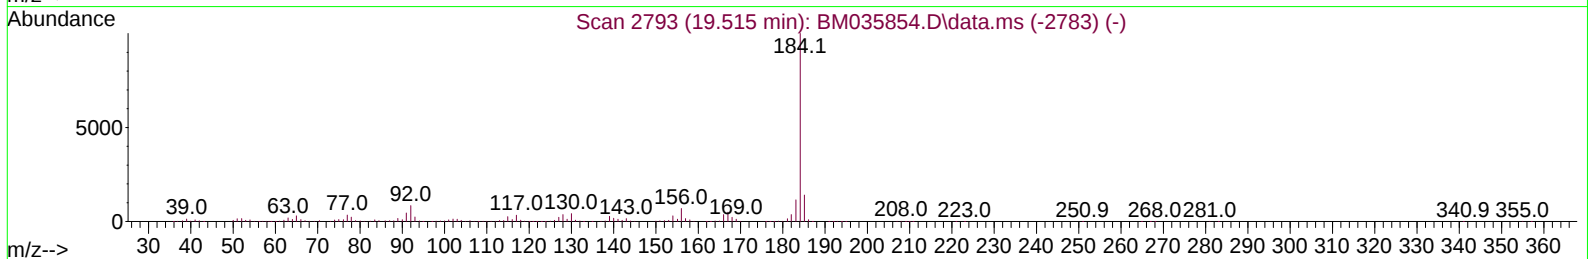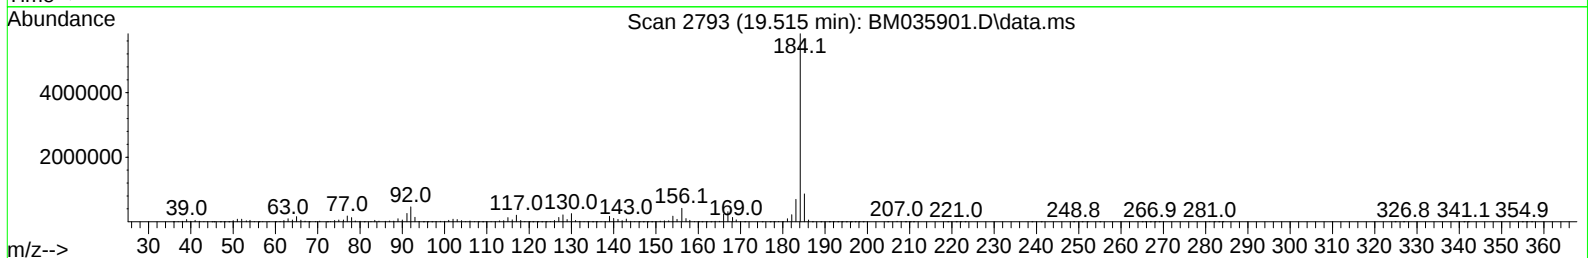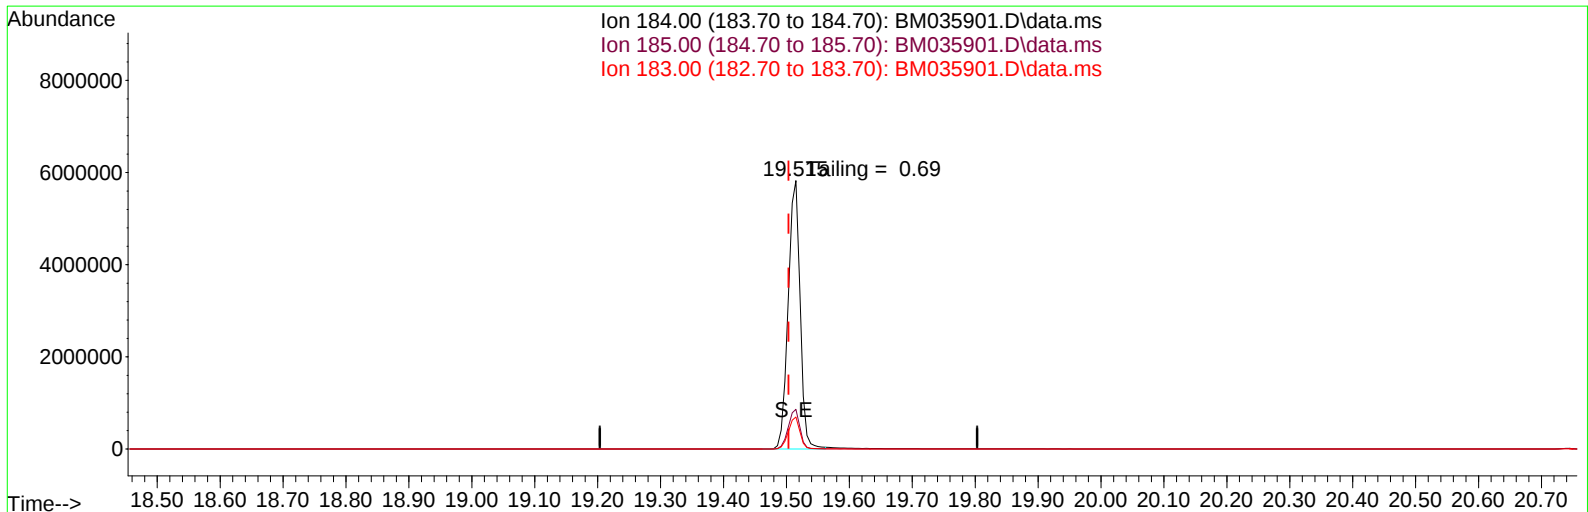

TIC: BM035901.D\data.ms

(77) Benzidine**19.515min (+ 0.012) 359721.20 ng****response 7869299**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.81
183.00	11.90	11.92
0.00	0.00	0.00