

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072222\
 Data File : BM035903.D
 Acq On : 22 Jul 2022 12:47
 Operator : CG/JU
 Sample : PB146339BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB146339BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.451	395	402	417	rBV	6371893	8892527	68.26%	12.696%
2	7.057	667	675	689	rBV	5701261	8717448	66.91%	12.446%
3	7.887	809	816	824	rBV	1166159	1790910	13.75%	2.557%
4	9.057	1007	1015	1024	rBV	3498408	5528290	42.43%	7.893%
5	10.692	1285	1293	1302	rBV	1489796	2414408	18.53%	3.447%
6	13.157	1704	1712	1720	rBV	8002652	11563135	88.75%	16.508%
7	14.521	1937	1944	1951	rBV	1905638	2703558	20.75%	3.860%
8	16.004	2189	2196	2216	rBV	5074603	7067882	54.25%	10.091%
9	17.262	2403	2410	2418	rBV	1944158	2731136	20.96%	3.899%
10	19.886	2850	2856	2869	rVB	10859885	13028196	100.00%	18.600%
11	21.433	3115	3119	3128	rBV	2193134	2749553	21.10%	3.925%
12	23.803	3516	3522	3532	rVB2	1452347	2857067	21.93%	4.079%




Sum of corrected areas: 70044110

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072222\
Data File : BM035903.D
Acq On : 22 Jul 2022 12:47
Operator : CG/JU
Sample : PB146339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

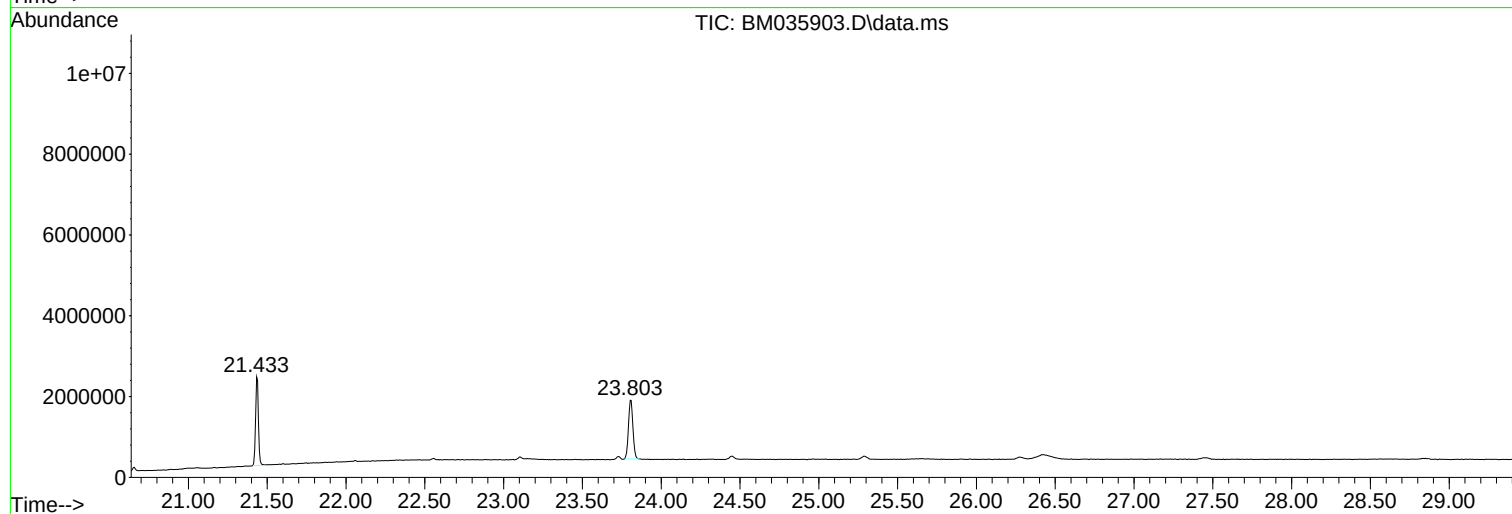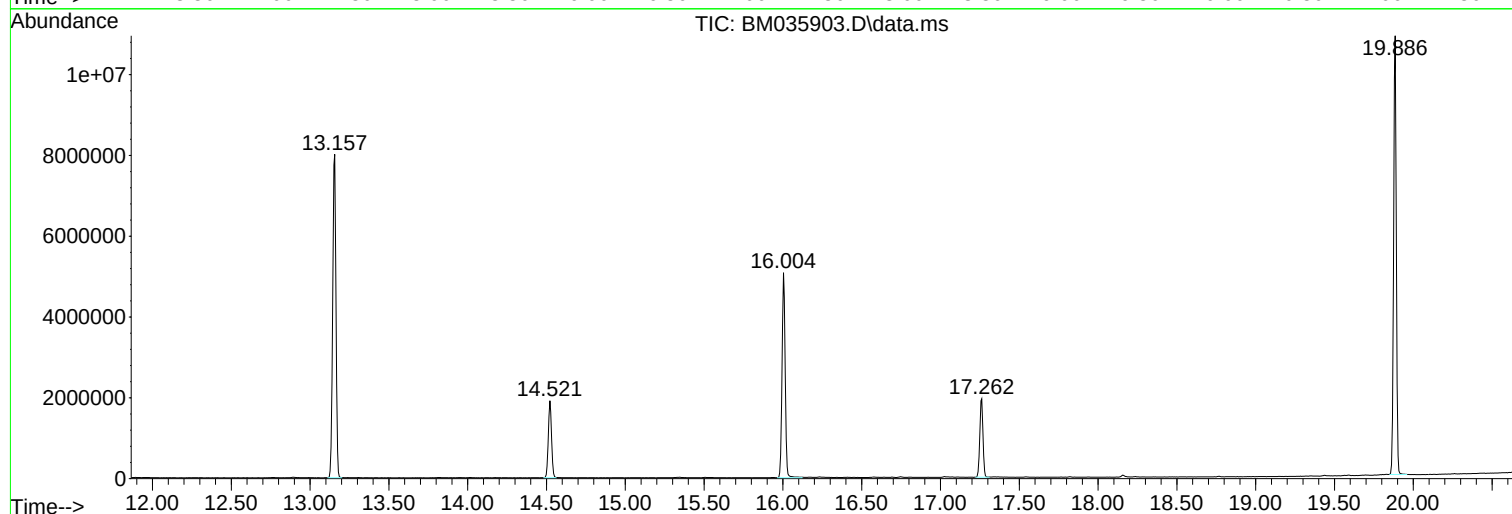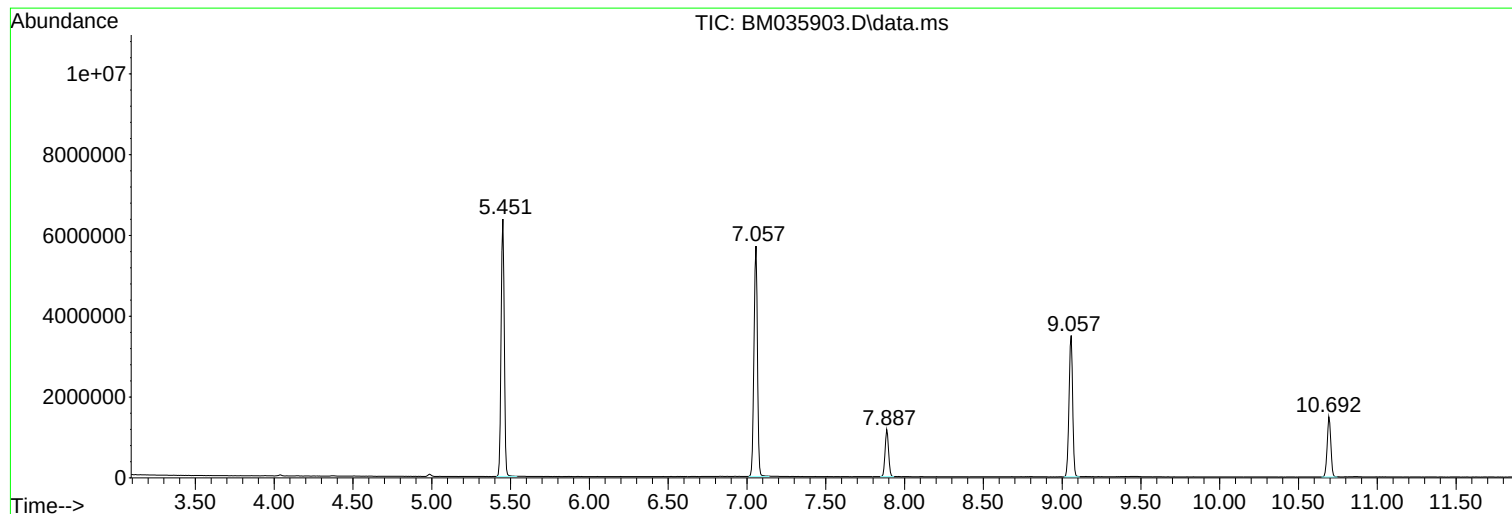

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072222\
Data File : BM035903.D
Acq On : 22 Jul 2022 12:47
Operator : CG/JU
Sample : PB146339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072222\
Data File : BM035903.D
Acq On : 22 Jul 2022 12:47
Operator : CG/JU
Sample : PB146339BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB146339BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------