

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072222\
 Data File : BM035906.D
 Acq On : 22 Jul 2022 15:01
 Operator : CG/JU
 Sample : N3786-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0718-WC-TP-WC3EA

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035906.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.981	317	322	334	rVB	49387	84465	1.62%	0.221%
2	5.445	395	401	411	rBV	1858257	2626492	50.28%	6.865%
3	7.051	667	674	685	rBV	1754391	2668144	51.08%	6.974%
4	7.887	809	816	825	rBV	1329159	2016546	38.60%	5.271%
5	9.051	1005	1014	1025	rBV	1345093	2174130	41.62%	5.683%
6	10.692	1284	1293	1303	rBV	1686724	2766917	52.97%	7.232%
7	13.151	1704	1711	1720	rBV	3231140	4607584	88.20%	12.043%
8	13.427	1754	1758	1764	rBV4	34619	58490	1.12%	0.153%
9	14.521	1937	1944	1951	rBV	2263908	3188595	61.04%	8.334%
10	16.004	2190	2196	2208	rBV	1533407	2120164	40.59%	5.542%
11	17.262	2403	2410	2416	rBV	2349199	3334314	63.83%	8.715%
12	17.939	2520	2525	2529	rBV	41243	53457	1.02%	0.140%
13	18.162	2557	2563	2572	rBV	209554	354111	6.78%	0.926%
14	19.439	2776	2780	2785	rBV	70919	106937	2.05%	0.280%
15	19.886	2850	2856	2867	rBV	4254647	5223903	100.00%	13.654%
16	20.656	2984	2987	2993	rBV	98316	109453	2.10%	0.286%
17	21.156	3069	3072	3082	rBV	188790	294245	5.63%	0.769%
18	21.439	3115	3120	3131	rBV	2600293	3301912	63.21%	8.630%
19	23.809	3516	3523	3534	rVB2	1635976	3169702	60.68%	8.285%




Sum of corrected areas: 38259561

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072222\
Data File : BM035906.D
Acq On : 22 Jul 2022 15:01
Operator : CG/JU
Sample : N3786-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-WC3EA

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

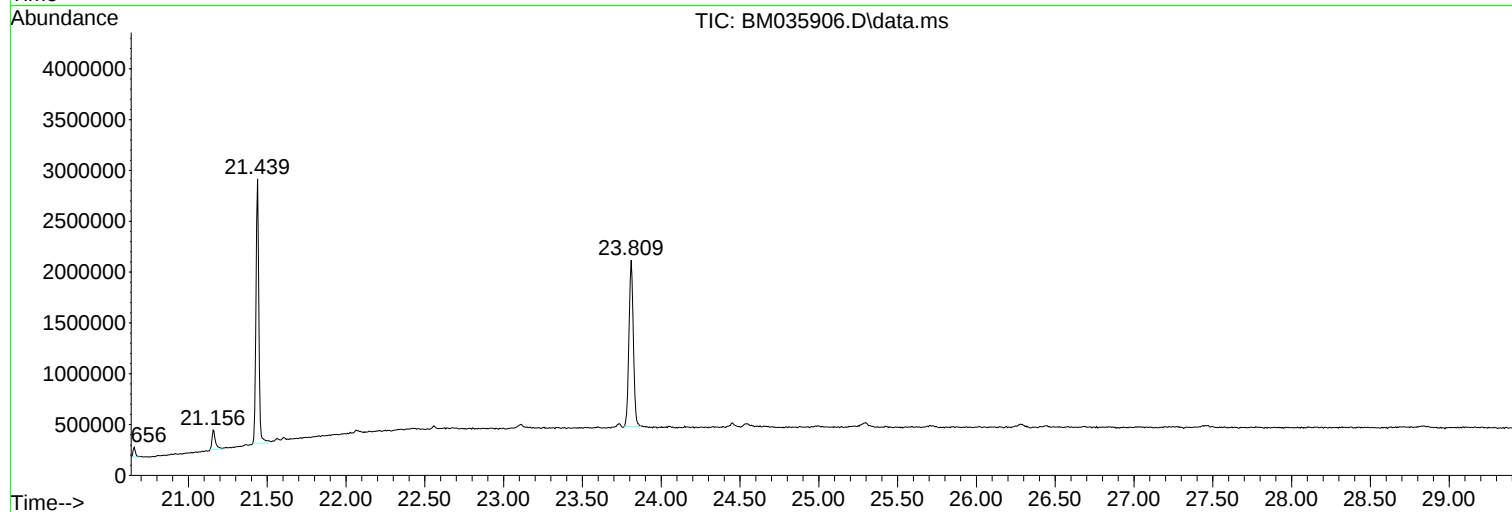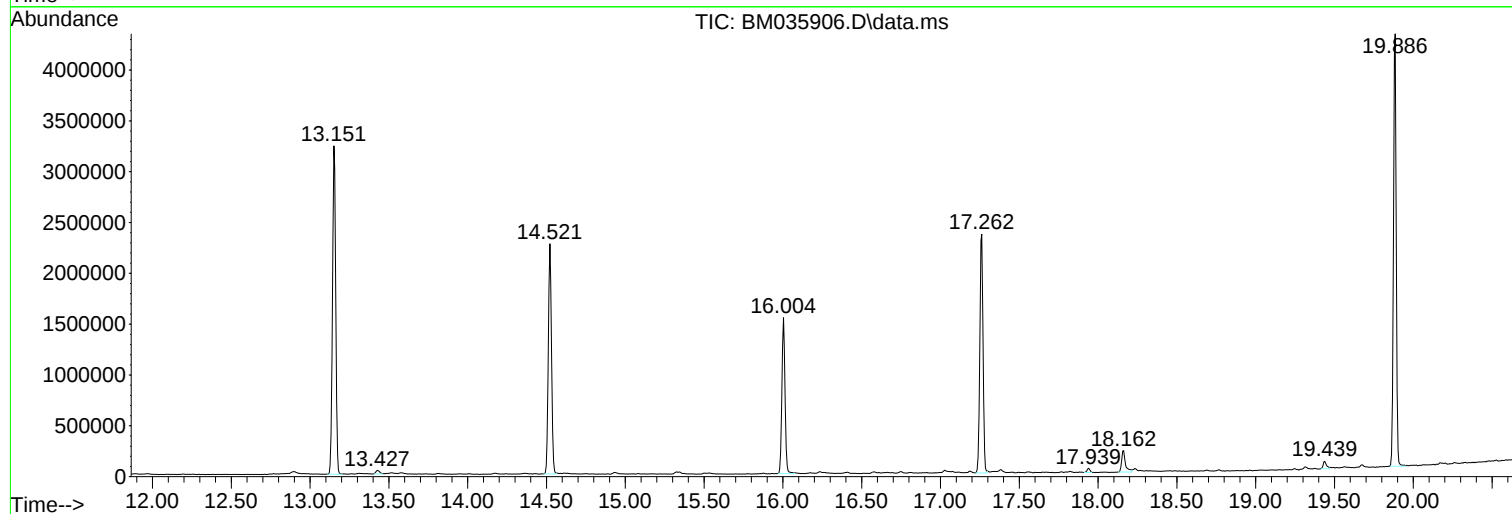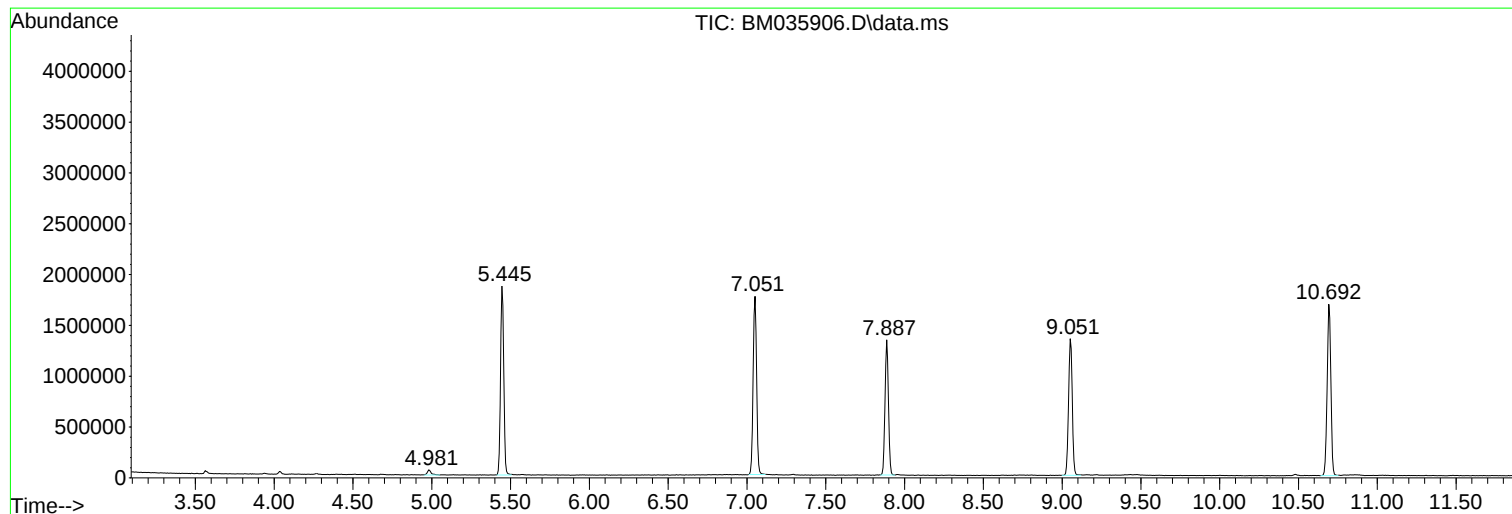

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072222\
Data File : BM035906.D
Acq On : 22 Jul 2022 15:01
Operator : CG/JU
Sample : N3786-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-WC3EA

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072222\
Data File : BM035906.D
Acq On : 22 Jul 2022 15:01
Operator : CG/JU
Sample : N3786-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0718-WC-TP-WC3EA

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------