
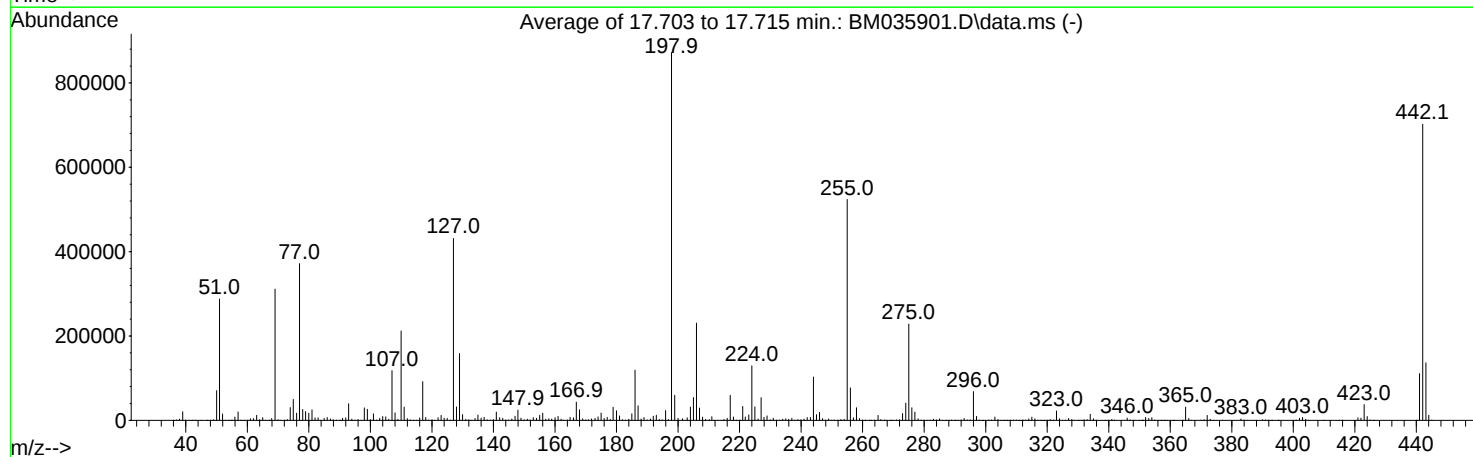


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072222\
 Data File : BM035901.D
 Acq On : 22 Jul 2022 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 22 14:25:12 2022

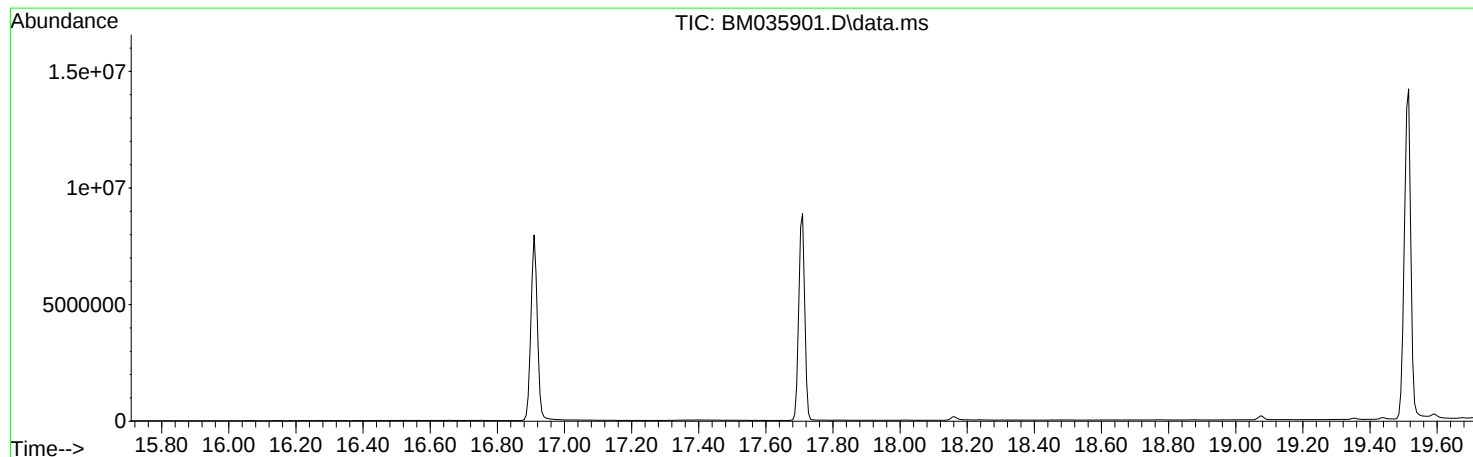

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	287970	PASS
68	69	0.00	2	1.3	4046	PASS
69	198	0.00	100	35.7	311218	PASS
70	69	0.00	2	0.5	1530	PASS
127	198	10	80	49.5	431339	PASS
197	198	0.00	2	0.2	1886	PASS
198	198	100	100	100.0	872107	PASS
199	198	5	9	6.8	59504	PASS
275	198	10	60	26.2	228224	PASS
365	198	1	100	3.6	31336	PASS
441	198	0.01	100	12.7	110685	PASS
442	442	50	100	100.0	701952	PASS
443	442	15	24	19.5	136677	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/22/2022	BNA_M	<u>BM035901.D</u>
Compound Name	Response	Retention Time
DDT	3602115	20.73
DDD	28784	20.29
DDE	3017	19.79
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31801	3633916	0.88

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072222\
 Data File : BM035901.D
 Acq On : 22 Jul 2022 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 22 14:34:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 22 14:25:12 2022
 Response via : Initial Calibration

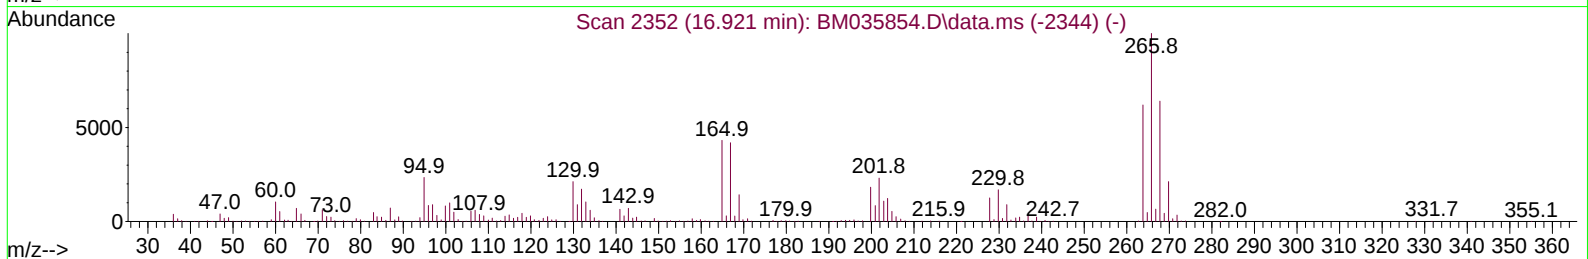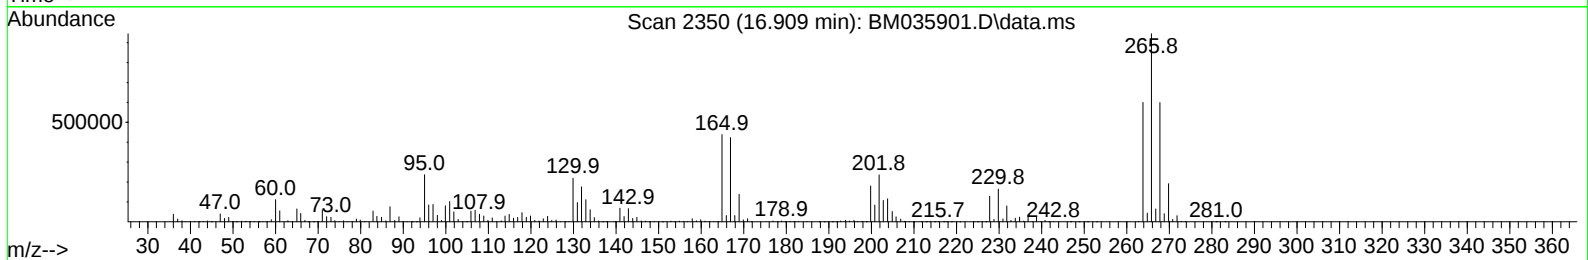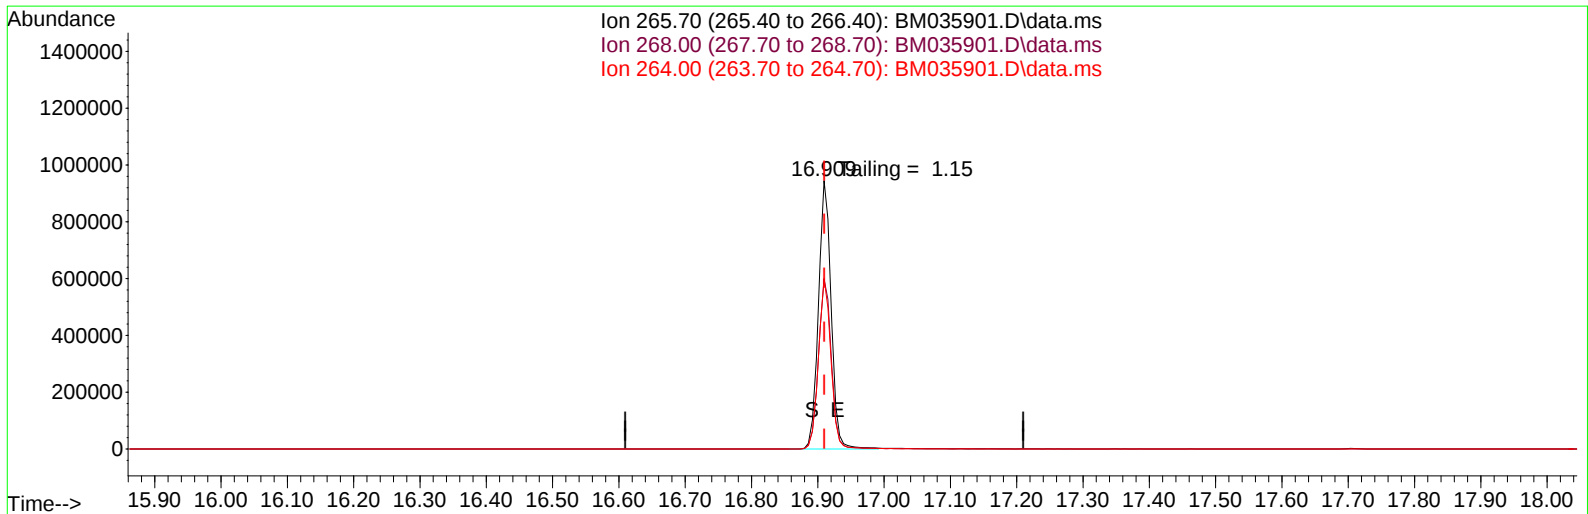

TIC: BM035901.D\data.ms

(70) Pentachlorophenol (C)

16.909min (-0.000) 970845.89 ng




response 1269911

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.39
264.00	63.30	63.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072222\
 Data File : BM035901.D
 Acq On : 22 Jul 2022 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 22 14:34:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 22 14:25:12 2022
 Response via : Initial Calibration

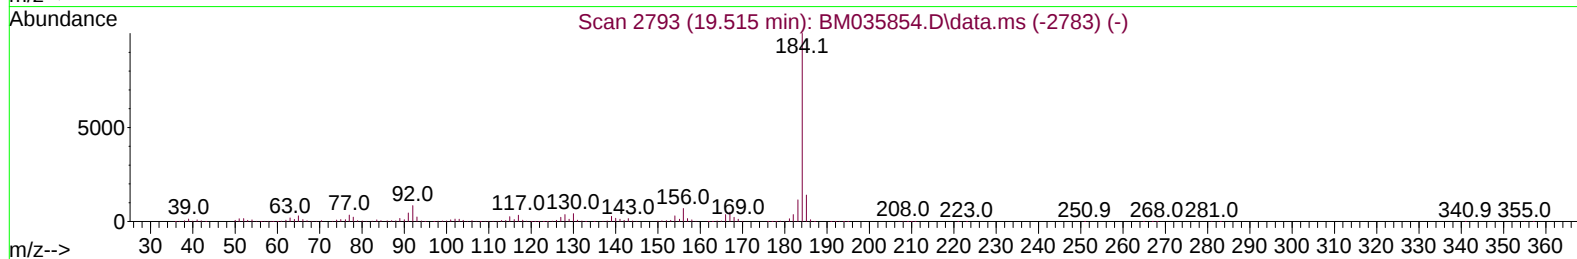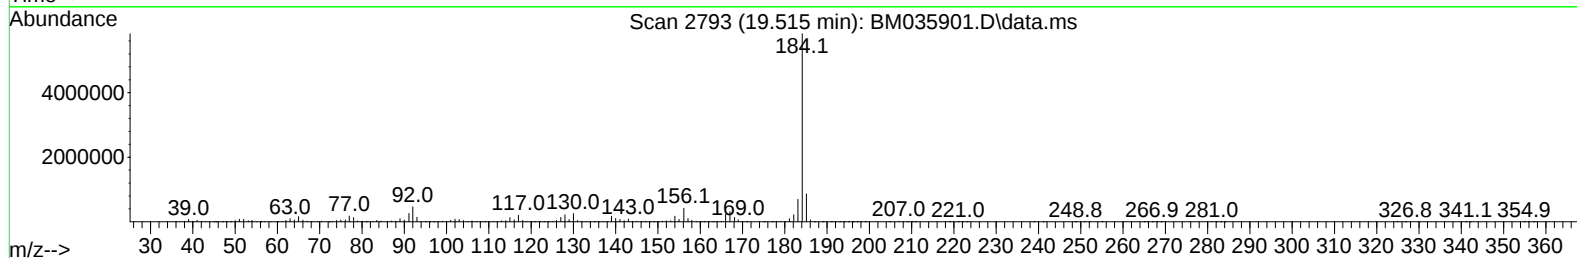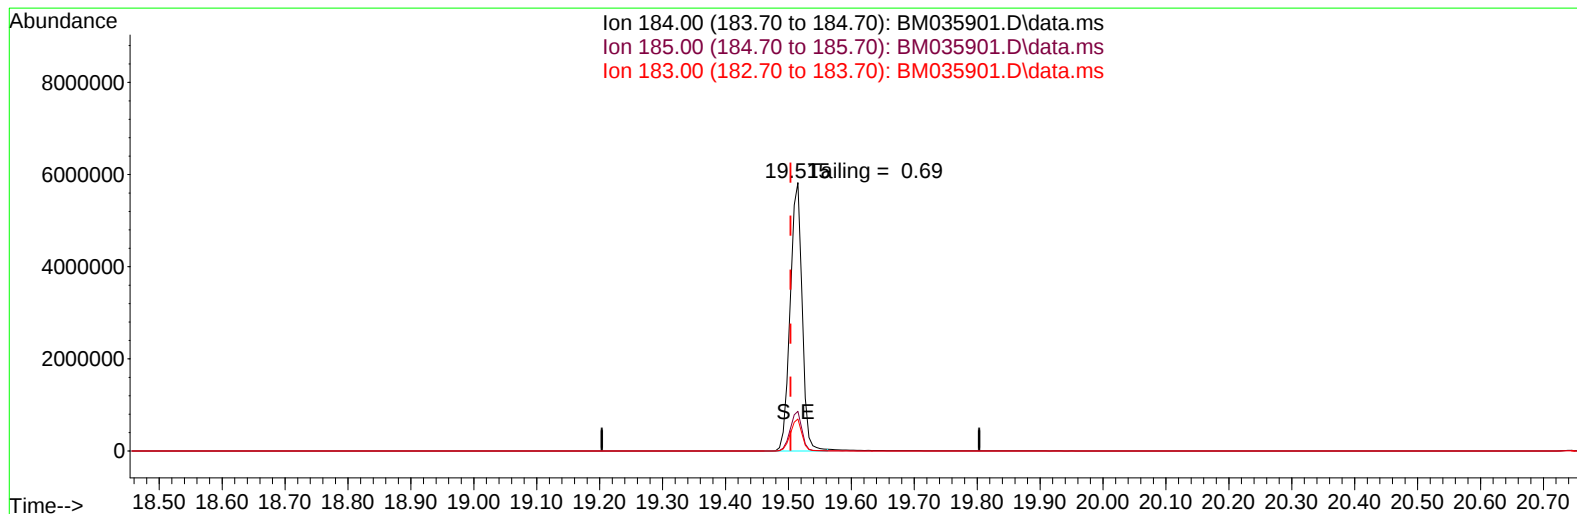

TIC: BM035901.D\data.ms

(77) Benzidine

19.515min (+ 0.012) 359721.20 ng

response 7869299

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.81
183.00	11.90	11.92
0.00	0.00	0.00