
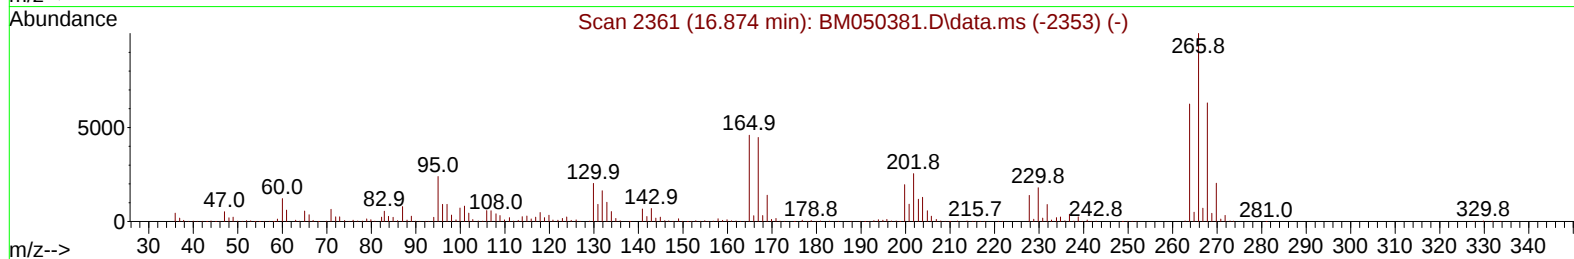
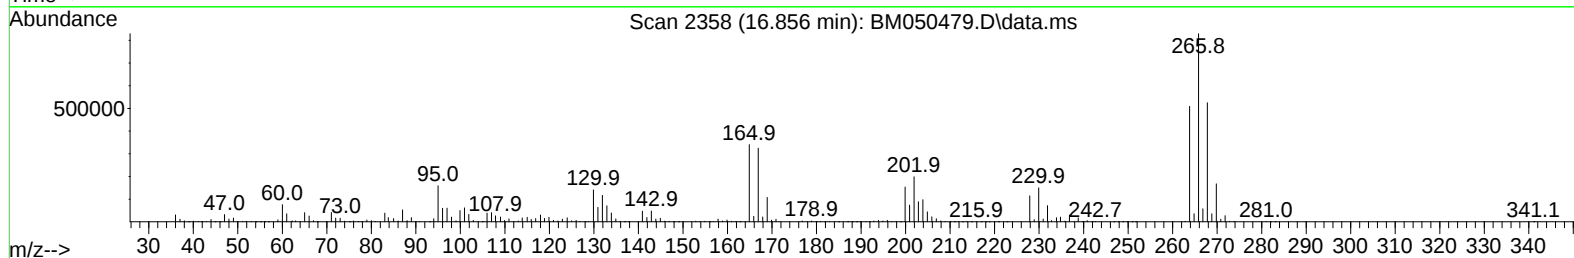


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072225\
Data File : BM050479.D
Acq On : 22 Jul 2025 08:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 10:43:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 16:20:15 2025
Response via : Initial Calibration

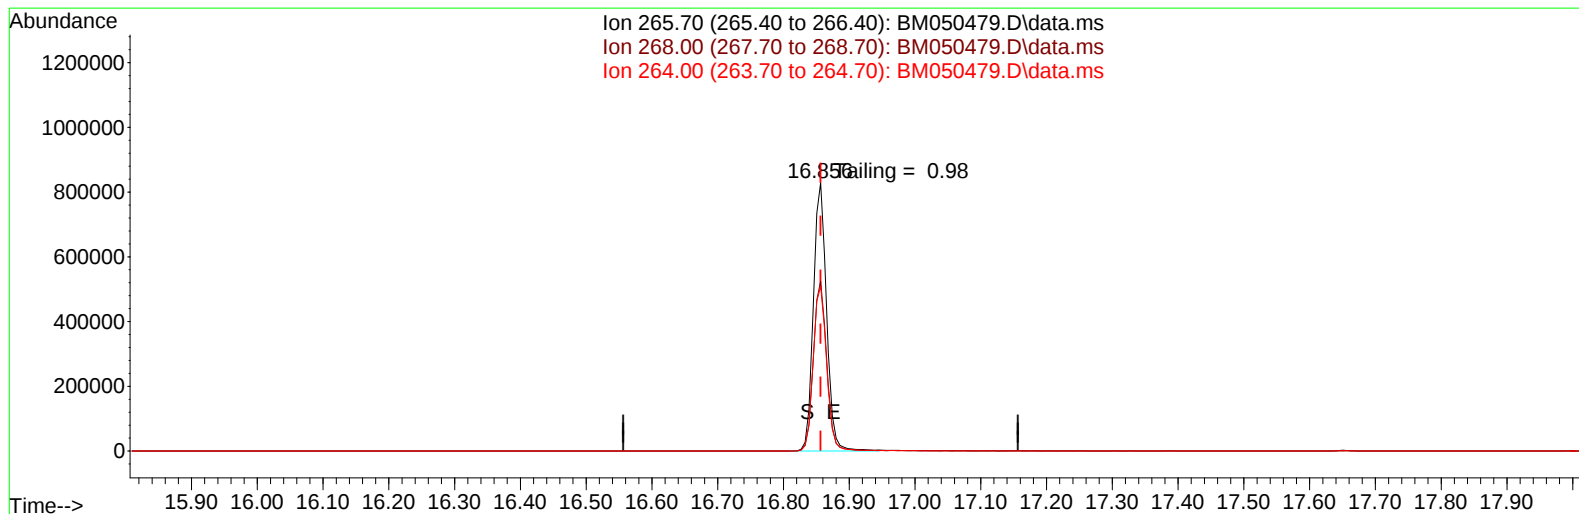

TIC: BM050479.D\data.ms

(70) Pentachlorophenol (C)




16.856min (-0.000) 0.00 ng

response 1159267

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.34
264.00	62.40	61.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072225\
Data File : BM050479.D
Acq On : 22 Jul 2025 08:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 10:43:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 16:20:15 2025
Response via : Initial Calibration

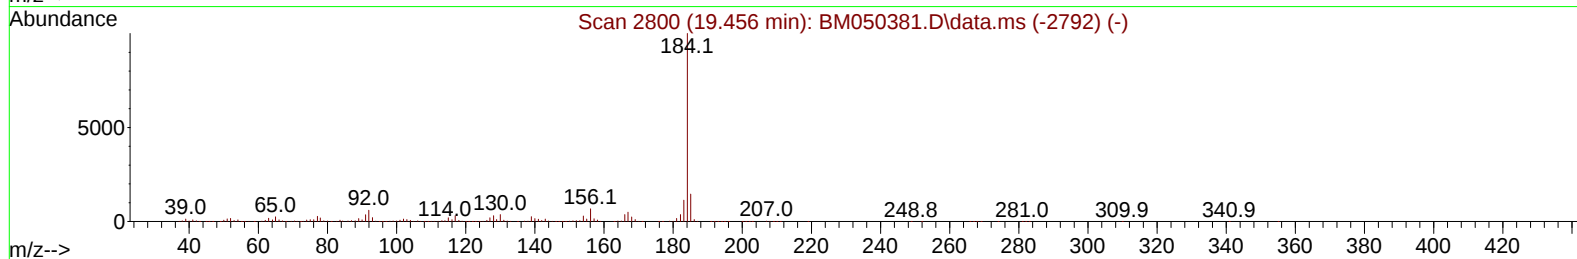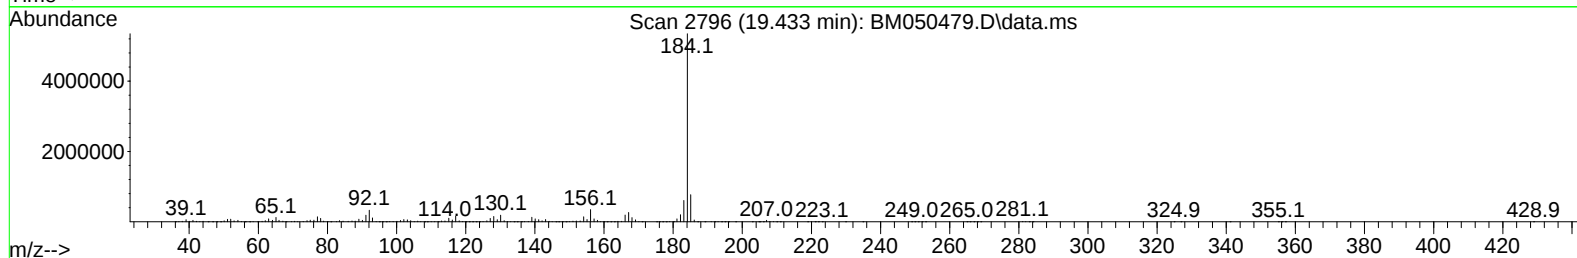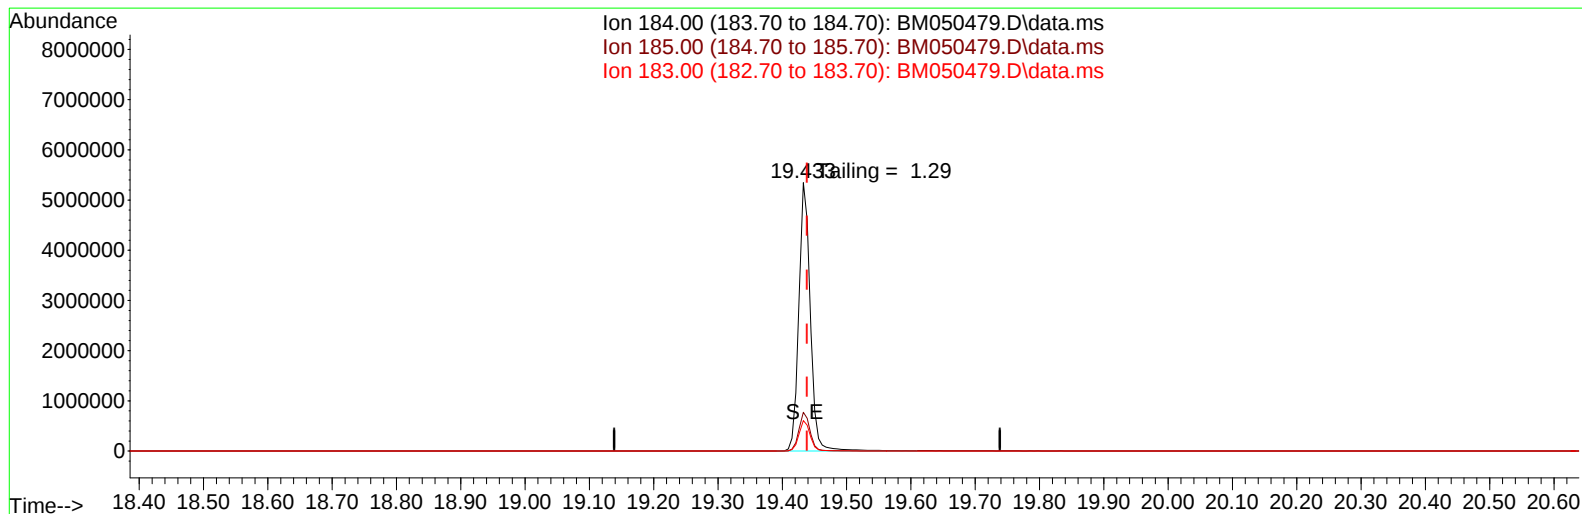

TIC: BM050479.D\data.ms

(77) Benzidine**19.433min (-0.006) 4337618.57 ng****response 6638220**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.43
183.00	11.30	11.32
0.00	0.00	0.00