

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072225\
 Data File : BM050484.D
 Acq On : 22 Jul 2025 13:32
 Operator : RC/JU
 Sample : Q2638-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OU4-TS-36-071725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM050484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	343	347	374	rVB2	911377	3452410	3.71%	0.284%
2	5.475	415	423	484	rVB	12630857	46704434	50.21%	3.845%
3	7.046	679	690	722	rBV	19560947	48478064	52.12%	3.991%
4	7.863	821	829	852	rBV	8175862	22322806	24.00%	1.838%
5	9.016	1009	1025	1042	rBV	15359133	34206878	36.77%	2.816%
6	10.651	1294	1303	1321	rBV	15278473	30538304	32.83%	2.514%
7	12.151	1550	1558	1570	rVB2	381437	1170842	1.26%	0.096%
8	13.104	1712	1720	1730	rVB2	48548720	78994385	84.92%	6.503%
9	13.922	1852	1859	1864	rBV2	761787	1708960	1.84%	0.141%
10	14.192	1899	1905	1916	rBV	2883692	5190964	5.58%	0.427%
11	14.322	1922	1927	1934	rVB3	705511	1593101	1.71%	0.131%
12	14.475	1945	1953	1960	rBV	27157992	41383794	44.49%	3.407%
13	14.886	2016	2023	2029	rBV4	415750	931154	1.00%	0.077%
14	15.339	2095	2100	2104	rBV	1110932	1647554	1.77%	0.136%
15	15.427	2107	2115	2118	rBV4	1104650	2791581	3.00%	0.230%
16	15.539	2131	2134	2142	rVB	774028	1302002	1.40%	0.107%
17	15.727	2162	2166	2174	rVB3	517401	955915	1.03%	0.079%
18	15.827	2178	2183	2191	rVB	5944748	8696307	9.35%	0.716%
19	15.963	2198	2206	2212	rBV	40357528	62788931	67.50%	5.169%
20	16.186	2240	2244	2247	rBV2	820602	1406532	1.51%	0.116%
21	16.416	2280	2283	2287	rVB	1261647	1514305	1.63%	0.125%
22	16.616	2314	2317	2321	rVB	1258944	1546939	1.66%	0.127%
23	16.786	2343	2346	2350	rVB	785006	946528	1.02%	0.078%
24	17.210	2412	2418	2422	rBV2	32703512	47440039	51.00%	3.906%
25	17.251	2422	2425	2431	rVV	4332926	6716093	7.22%	0.553%
26	17.304	2431	2434	2436	rVV	1118912	1356822	1.46%	0.112%
27	17.339	2436	2440	2444	rVB	2742002	3762578	4.04%	0.310%
28	17.386	2444	2448	2454	rBV4	808067	1708690	1.84%	0.141%
29	17.580	2478	2481	2484	rBV	852391	1069263	1.15%	0.088%
30	17.874	2529	2531	2537	rVB3	1192571	1643567	1.77%	0.135%
31	18.121	2559	2573	2580	rBV2	25491103	46108428	49.57%	3.796%
32	18.210	2584	2588	2593	rVB	1667286	2521763	2.71%	0.208%
33	18.268	2594	2598	2603	rBV2	2679544	5391639	5.80%	0.444%
34	18.680	2666	2668	2675	rVB3	643765	949651	1.02%	0.078%
35	18.827	2690	2693	2697	rVB3	1013675	1187381	1.28%	0.098%
36	18.992	2717	2721	2726	rBV2	3197579	4730275	5.09%	0.389%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072225\
Data File : BM050484.D
Acq On : 22 Jul 2025 13:32
Operator : RC/JU
Sample : Q2638-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-36-071725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	19.127	2740	2744	2749	rBV3	2995592	5206562	5.60%	0.429%
38	19.257	2760	2766	2772	rBV	16633564	25815354	27.75%	2.125%
39	19.315	2773	2776	2780	rVV3	4096827	5711886	6.14%	0.470%
40	19.386	2784	2788	2796	rVB2	12028331	18966580	20.39%	1.561%
41	19.521	2808	2811	2817	rVB	2537240	3911764	4.21%	0.322%
42	19.621	2819	2828	2836	rVV	15308009	26056715	28.01%	2.145%
43	19.698	2837	2841	2846	rVB3	1880165	2998624	3.22%	0.247%
44	19.786	2853	2856	2857	rBV2	1455999	1584344	1.70%	0.130%
45	19.827	2857	2863	2868	rVV2	58686228	93018246	100.00%	7.658%
46	19.939	2878	2882	2892	rBV4	2806951	6894347	7.41%	0.568%
47	20.109	2908	2911	2915	rVB	5358834	6903019	7.42%	0.568%
48	20.209	2925	2928	2933	rVB	2335677	2912993	3.13%	0.240%
49	20.268	2934	2938	2942	rVB2	3794092	5033296	5.41%	0.414%
50	20.409	2958	2962	2966	rBV	4417677	5968074	6.42%	0.491%
51	20.457	2966	2970	2983	rVB2	5387731	10932080	11.75%	0.900%
52	20.609	2993	2996	3002	rVB	2836340	4014535	4.32%	0.331%
53	21.074	3073	3075	3077	rBV2	1637863	1665579	1.79%	0.137%
54	21.109	3077	3081	3090	rVB3	13150566	18229417	19.60%	1.501%
55	21.439	3129	3137	3142	rBV4	40205992	86855002	93.37%	7.151%
56	21.480	3142	3144	3156	rVB	13414684	18840656	20.25%	1.551%
57	22.127	3251	3254	3260	rVB2	4349865	6592206	7.09%	0.543%
58	22.221	3262	3270	3276	rVV3	9047384	22053346	23.71%	1.816%
59	22.386	3294	3298	3302	rVB	2796770	4066481	4.37%	0.335%
60	23.515	3483	3490	3496	rBV	7083474	21342972	22.94%	1.757%
61	23.627	3503	3509	3515	rBV	16609568	31587025	33.96%	2.601%
62	24.192	3600	3605	3618	rVB2	4954287	17162837	18.45%	1.413%
63	24.327	3621	3628	3642	rVB	7935753	21384293	22.99%	1.761%
64	24.486	3645	3655	3663	rBV2	23164545	63194295	67.94%	5.203%
65	25.297	3786	3793	3807	rVB	8267232	24015881	25.82%	1.977%
66	25.580	3831	3841	3850	rBV	12739715	38030741	40.89%	3.131%
67	25.686	3853	3859	3866	rBV2	2975320	7723723	8.30%	0.636%
68	26.221	3943	3950	3966	rVB2	7912720	28366853	30.50%	2.335%
69	29.503	4495	4508	4516	rBV3	9556892	43007054	46.24%	3.541%
70	31.485	4837	4845	4846	rBV	4697152	9742566	10.47%	0.802%




Sum of corrected areas: 1214648225

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072225\
Data File : BM050484.D
Acq On : 22 Jul 2025 13:32
Operator : RC/JU
Sample : Q2638-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-36-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

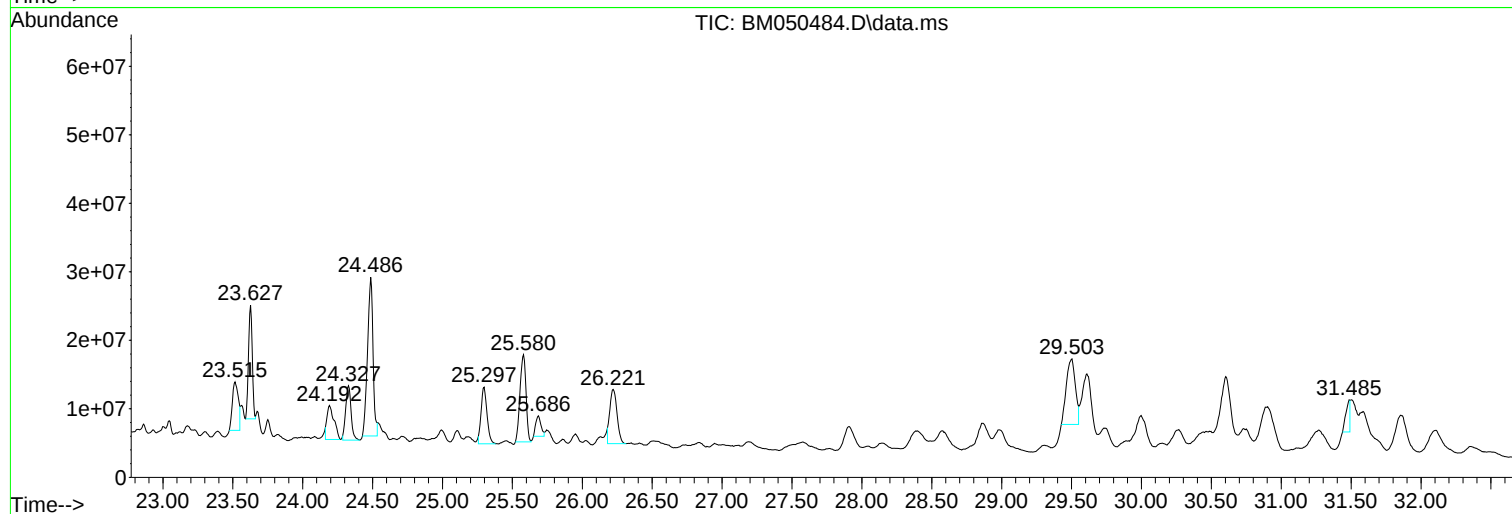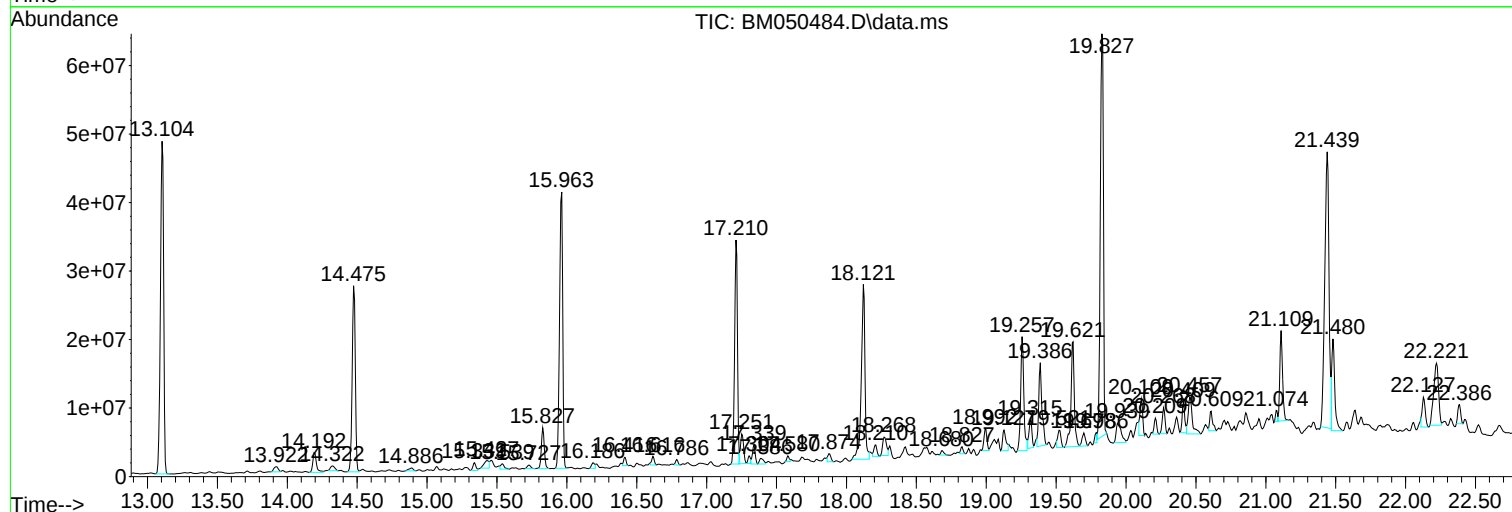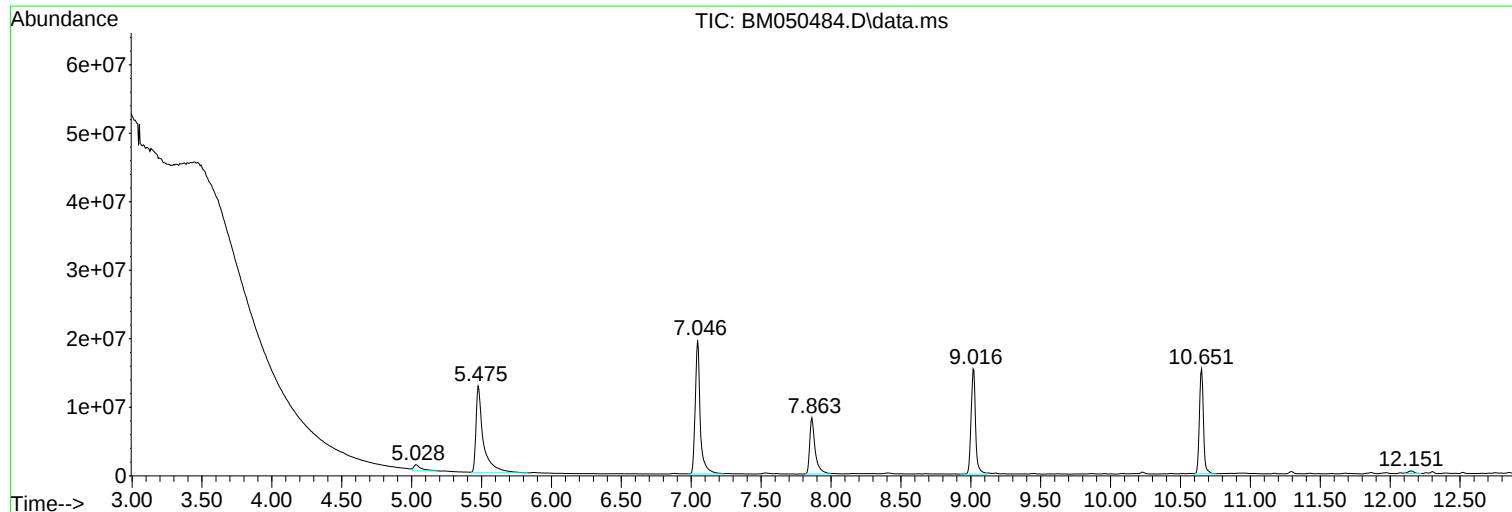

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072225\
Data File : BM050484.D
Acq On : 22 Jul 2025 13:32
Operator : RC/JU
Sample : Q2638-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-36-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072225\
Data File : BM050484.D
Acq On : 22 Jul 2025 13:32
Operator : RC/JU
Sample : Q2638-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OU4-TS-36-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------