


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072225\
Data File : BM050479.D
Acq On : 22 Jul 2025 08:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 17 16:20:15 2025

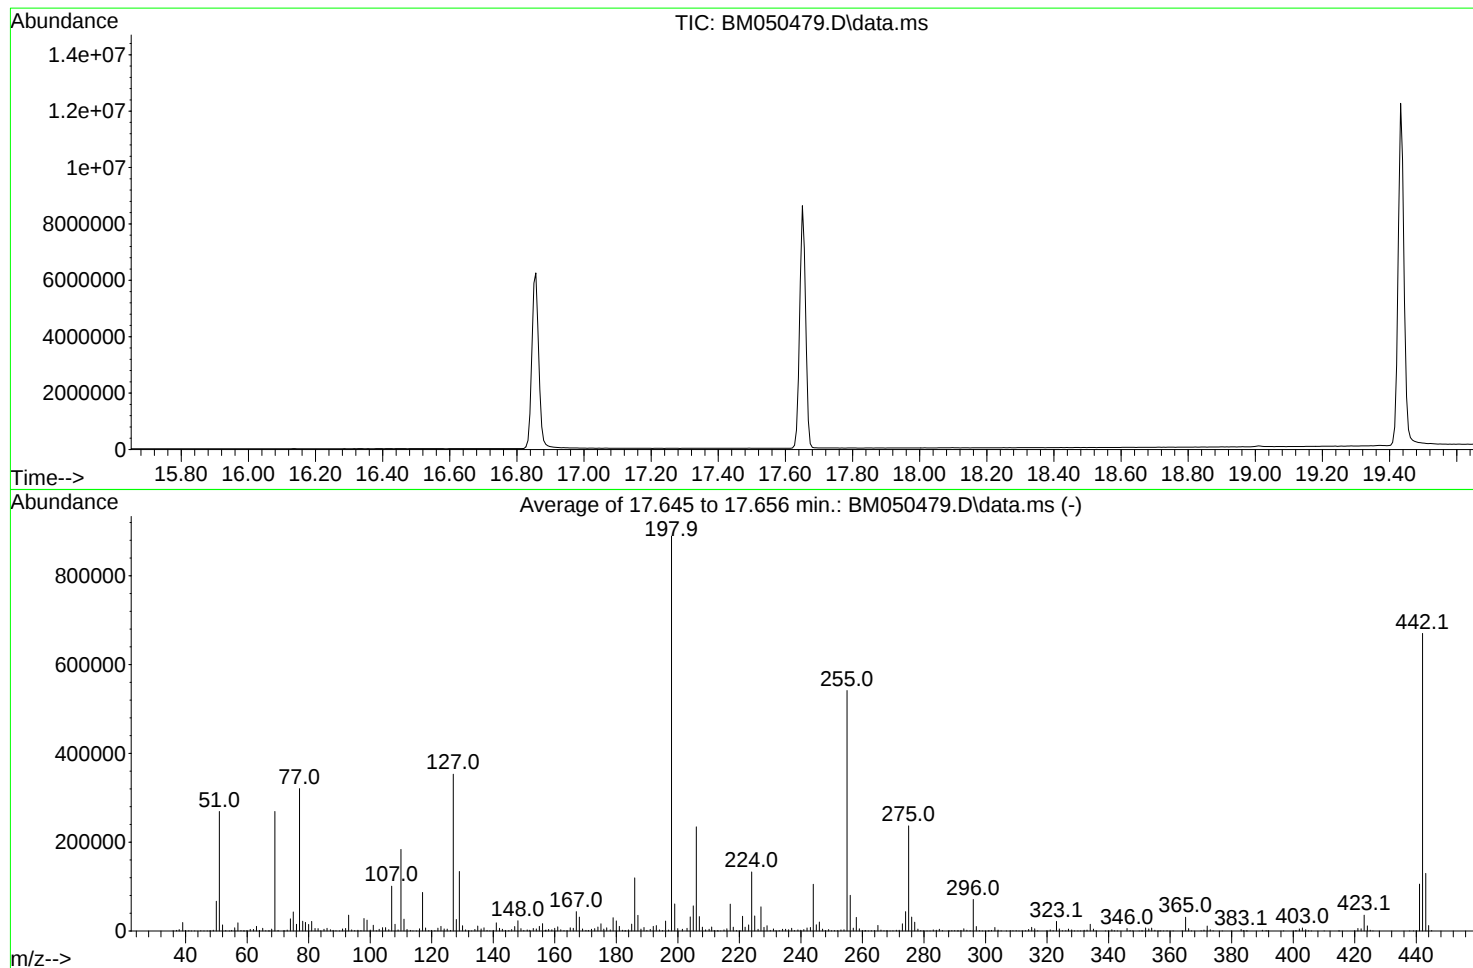




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.6	4240	PASS
69	69	100	100	100.0	269077	PASS
70	69	0.00	2	0.5	1452	PASS
197	198	0.00	2	0.2	1868	PASS
198	198	100	100	100.0	889323	PASS
199	198	5	9	6.8	60907	PASS
365	198	1	100	3.5	30741	PASS
441	443	0.01	150	81.5	105600	PASS
442	442	100	100	100.0	670059	PASS
443	442	15	24	19.3	129531	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072225\
Data File : BM050479.D
Acq On : 22 Jul 2025 08:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 22 10:43:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 16:20:15 2025
Response via : Initial Calibration

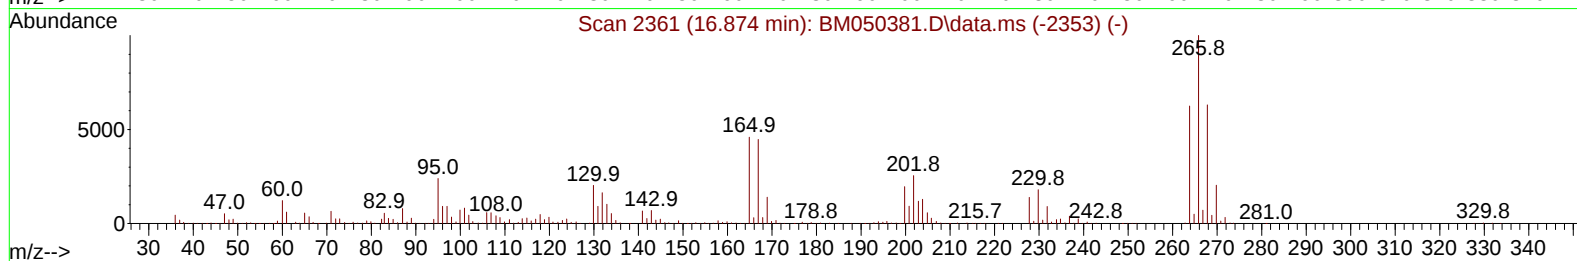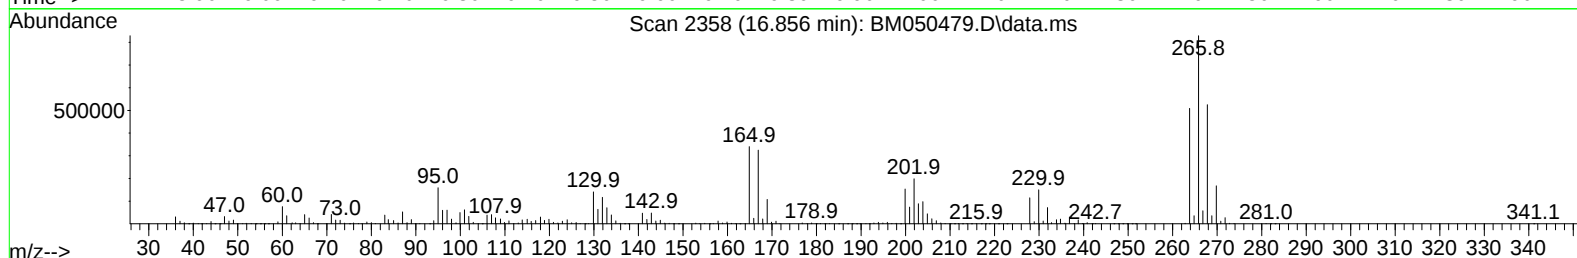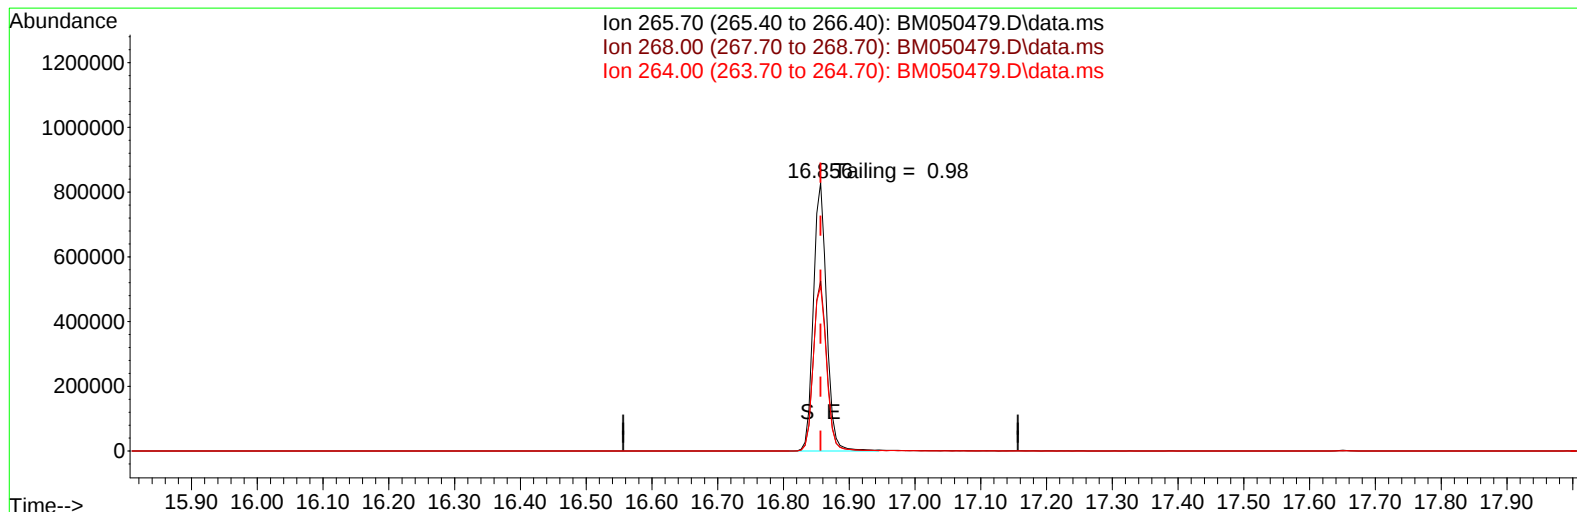

TIC: BM050479.D\data.ms

(70) Pentachlorophenol (C)

16.856min (-0.000) 0.00 ng




response 1159267

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.34
264.00	62.40	61.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072225\
Data File : BM050479.D
Acq On : 22 Jul 2025 08:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 22 10:43:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 16:20:15 2025
Response via : Initial Calibration

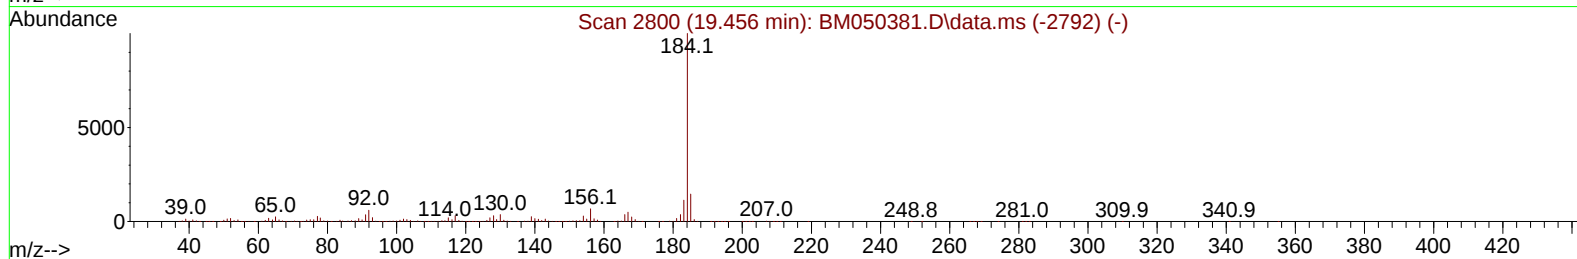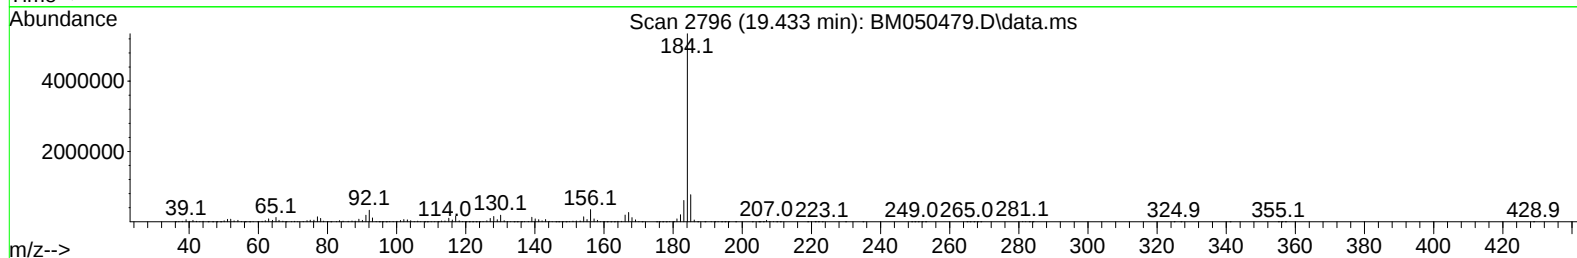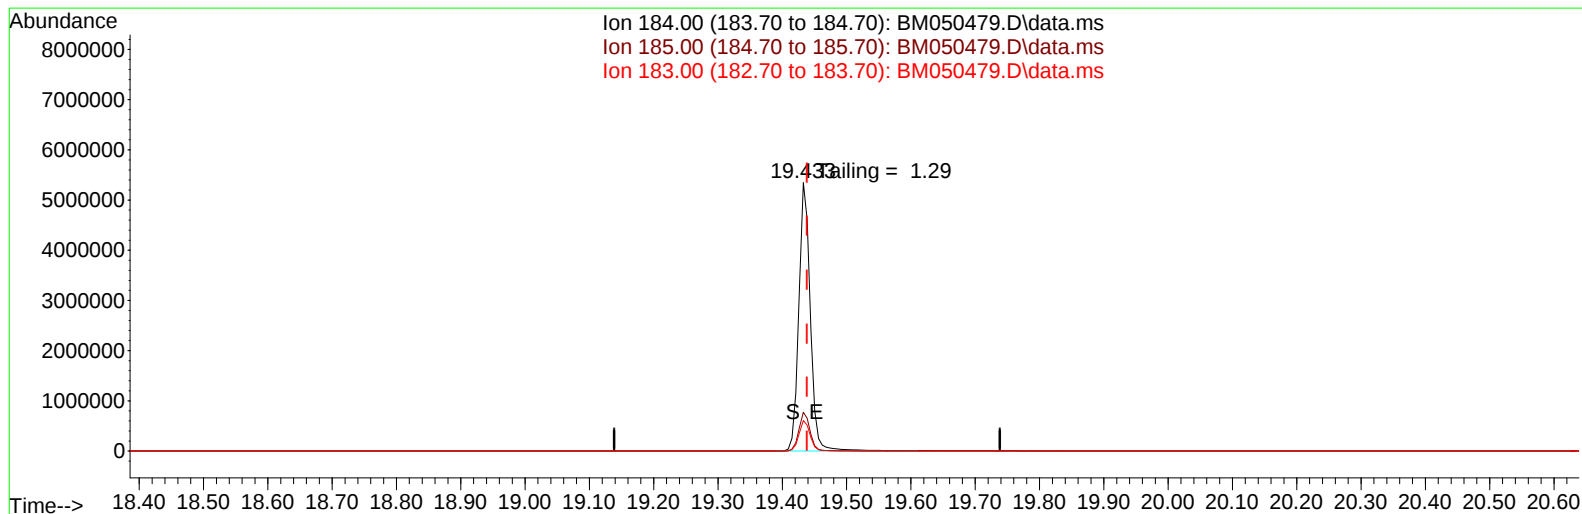

TIC: BM050479.D\data.ms

(77) Benzidine

19.433min (-0.006) 4337618.57 ng

response 6638220

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.43
183.00	11.30	11.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/22/2025	BNA_M	<u>BM050479.D</u>
Compound Name	Response	Retention Time
DDT	3179260	20.668
DDD	40849	20.286
DDE	5511	19.727
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
46360	3225620	1.44

Instrument :
BNA_M
ClientSampleId :
DFTPP