

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072315\
 Data File : BM002015.D
 Acq On : 23 Jul 2015 14:20
 Operator : TP/UM
 Sample : G3000-02
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C02MORE

Quant Time: Jul 24 01:31:56 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 24 01:29:30 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	77439	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	309615	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	182282	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	412092	20.00	ng/ul	0.00
77) Chrysene-d12	21.23	240	479506	20.00	ng/ul	0.00
85) Perylene-d12	23.44	264	478826	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.09	96	7586	4.79	ng/uL	0.00
5) Phenol-d5	6.79	99	177515	28.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	96027	27.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	152186	30.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	141360	27.22	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	71233	30.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	82676	32.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	149939	28.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	94329	17.69	ng/ul	0.04
43) Dimethylphthalate-d6	13.69	166	409808	27.87	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	518967	29.35	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	68446	27.49	ng/ul	0.00
57) Fluorene-d10	15.27	176	355511	28.30	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	45131	16.91	ng/ul	0.00
70) Anthracene-d10	17.12	188	522388	27.00	ng/ul	0.00
78) Pyrene-d10	19.43	212	576195	26.31	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.30	264	561252	23.18	ng/ul	0.00


Target Compounds				Qvalue		
2) 1,4-Dioxane	2.82	88	3150	1.89	ng/uL#	1
16) 4-Methylphenol	8.40	108	10119	1.86	ng/ul	93
44) Dimethylphthalate	13.73	163	107364	7.18	ng/ul	98
69) Phenanthrene	17.07	178	119809	5.37	ng/ul	100
71) Anthracene	17.07	178	120425	5.23	ng/ul	99
76) Fluoranthene	19.09	202	195636	7.50	ng/ul	97
79) Pyrene	19.46	202	208171	7.26	ng/ul	97
82) Benzo(a)anthracene	21.22	228	107406	3.76	ng/ul	95
83) Bis(2-ethylhexyl)phthalate	21.14	149	28218	1.76	ng/ul	98
84) Chrysene	21.26	228	125169	4.68	ng/ul	97
87) Benzo(b)fluoranthene	22.78	252	141490	4.82	ng/ul#	85
88) Benzo(k)fluoranthene	22.78	252	84416	2.99	ng/ul#	86
90) Benzo(a)pyrene	23.35	252	91573	3.32	ng/ul#	92
91) Indeno(1,2,3-cd)pyrene	25.66	276	60173	2.08	ng/ul	97
93) Benzo(g,h,i)perylene	26.35	276	60503	2.54	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072315\
Data File : BM002015.D
Acq On : 23 Jul 2015 14:20
Operator : TP/UM
Sample : G3000-02
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C02M0RE

Quant Time: Jul 24 01:31:56 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 01:29:30 2015
Response via : Initial Calibration

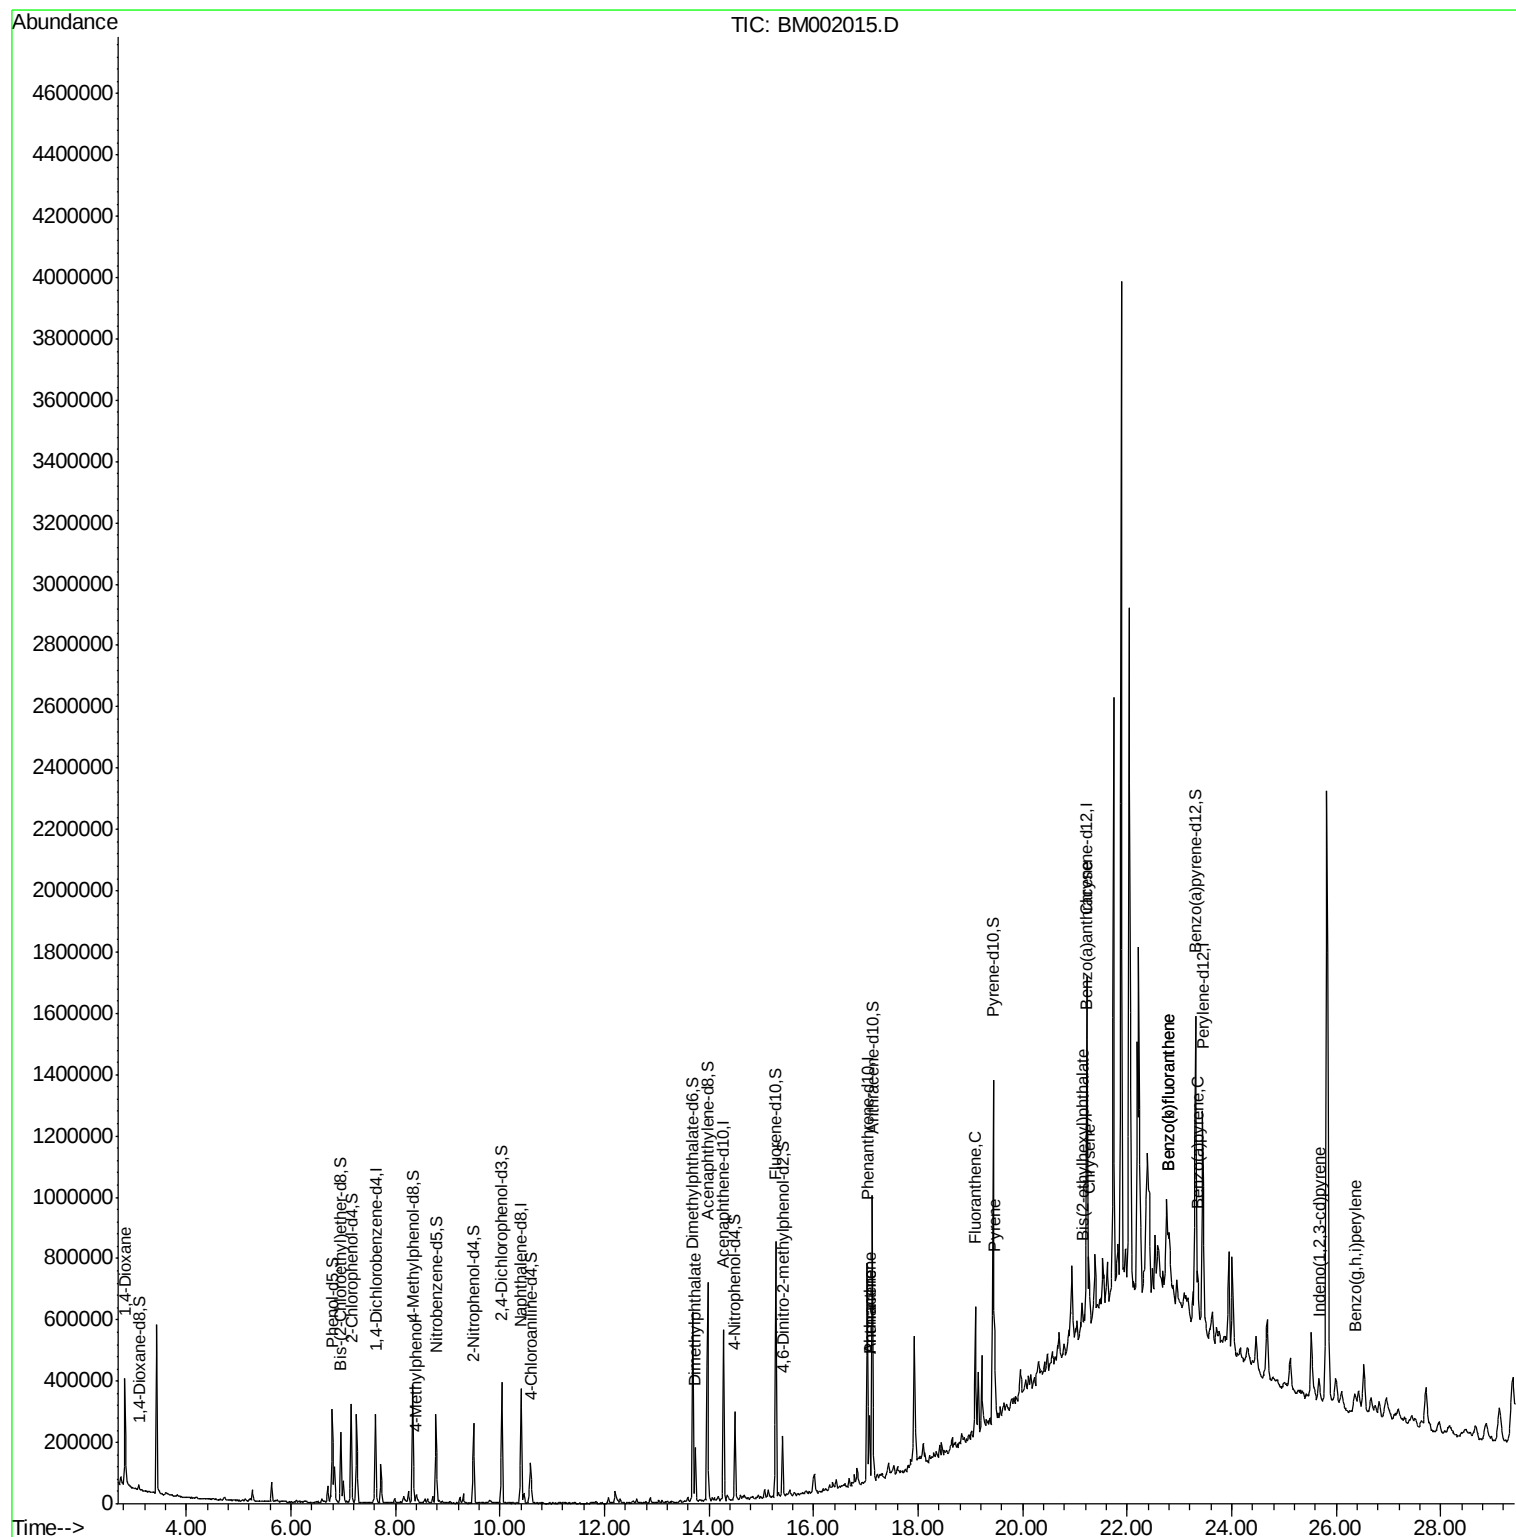

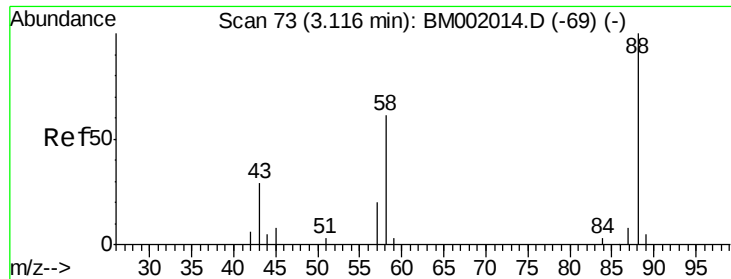

#2

1,4-Dioxane

Concen: 1.89 ng/uL

RT: 2.82 min Scan# 23

Delta R.T. -0.29 min

Lab File: BM002015.D

Acq: 23 Jul 2015 14:20

Instrument :

BNA_M

ClientSampleId :

C02M0RE


Tgt Ion: 88 Resp: 3150

Ion Ratio Lower Upper

88 100

43 1791.1 25.2 37.8#




58 24.7 55.6 83.4#

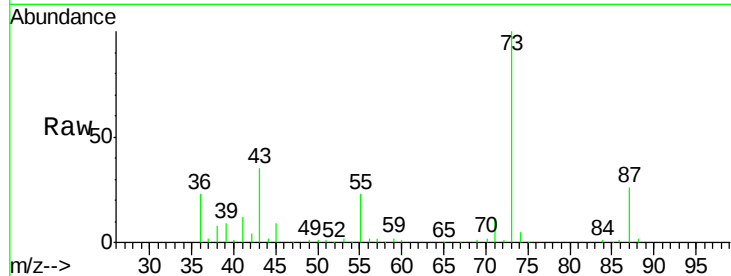

Abundance Ion 88.00 (87.70 to 88.70): BM002014.D (-69) (-)

Ion 43.00 (42.70 to 43.70): BM002014.D (-69) (-)

Ion 58.00 (57.70 to 58.70): BM002014.D (-69) (-)

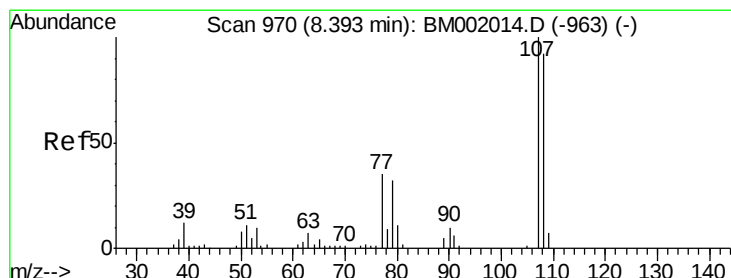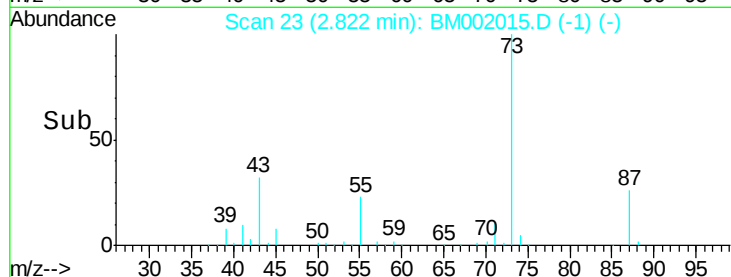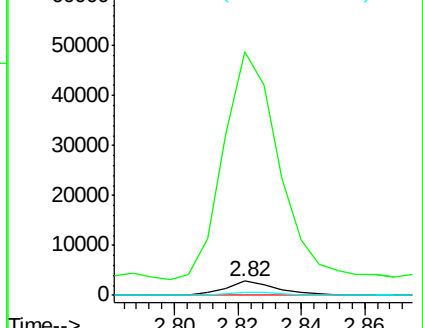

#16

4-Methylphenol

Concen: 1.86 ng/uL

RT: 8.40 min Scan# 971

Delta R.T. 0.01 min

Lab File: BM002015.D


Acq: 23 Jul 2015 14:20

Tgt Ion: 108 Resp: 10119

Ion Ratio Lower Upper



108 100


107 105.6 90.6 136.0

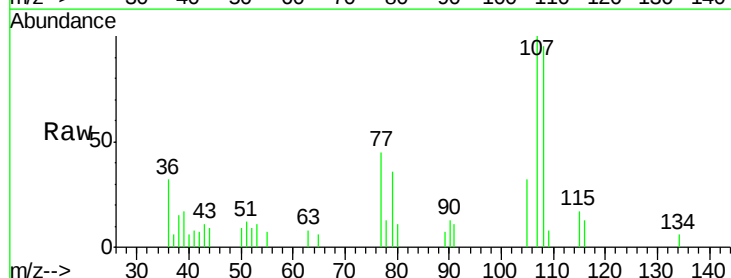

Abundance Ion 108.00 (107.70 to 108.70): BM002014.D (-963) (-)

Ion 107.00 (106.70 to 107.70): BM002014.D (-963) (-)



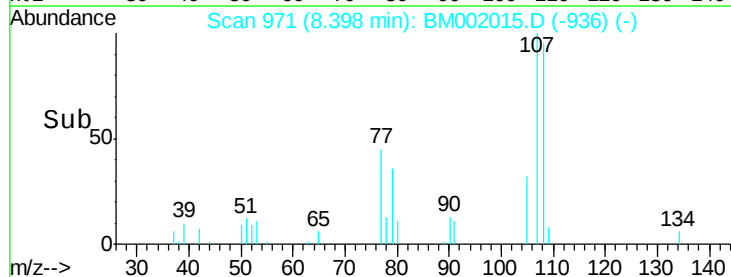
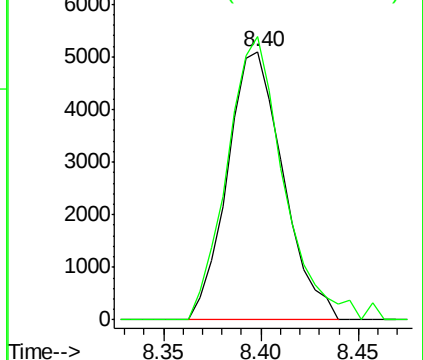


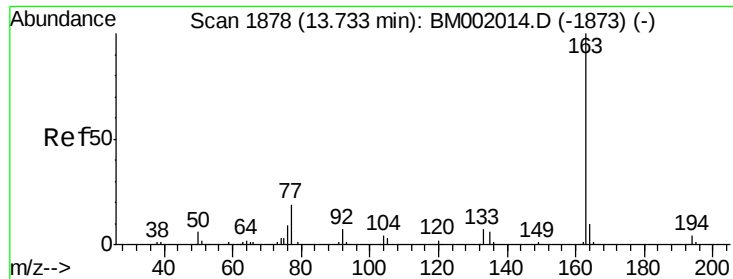

#44
Dimethylphthalate
Concen: 7.18 ng/ul
RT: 13.73 min Scan# 1878
Delta R.T. -0.00 min
Lab File: BM002015.D
Acq: 23 Jul 2015 14:20




Instrument :
BNA_M
ClientSampled :
C02MORE


Tgt Ion:163 Resp: 107364
Ion Ratio Lower Upper
163 100
194 4.0 3.5 5.3
164 9.4 8.2 12.4

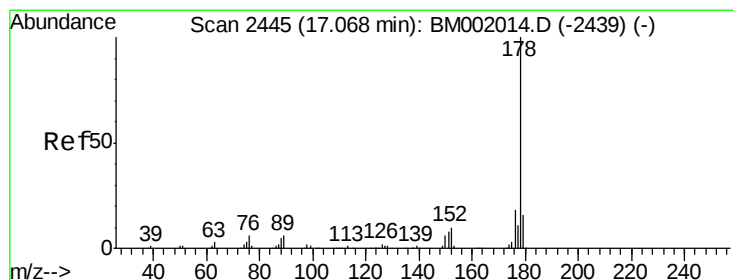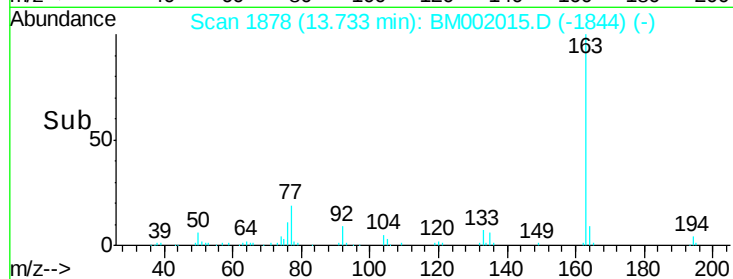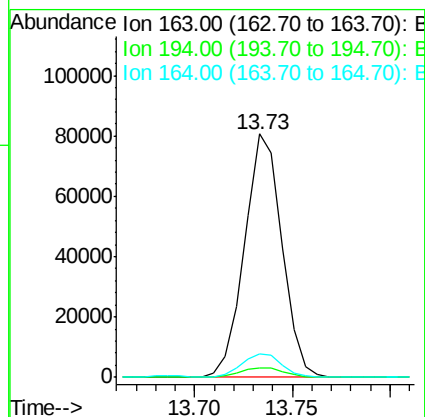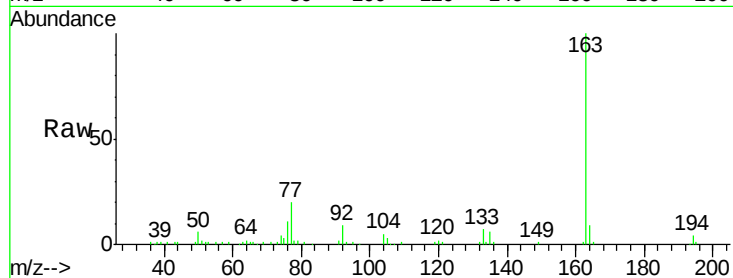

#69
Phenanthrene
Concen: 5.37 ng/ul
RT: 17.07 min Scan# 2445
Delta R.T. -0.00 min
Lab File: BM002015.D
Acq: 23 Jul 2015 14:20

Tgt Ion:178 Resp: 119809
Ion Ratio Lower Upper
178 100
179 14.9 12.1 18.1
176 18.4 14.6 21.8


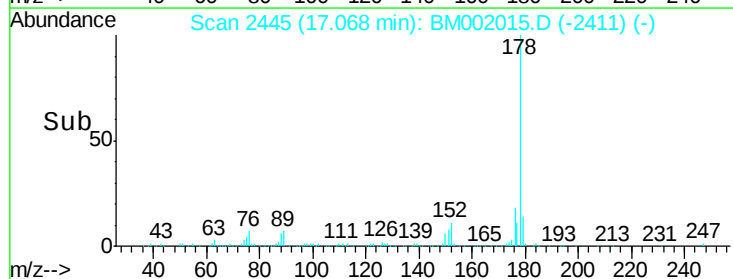
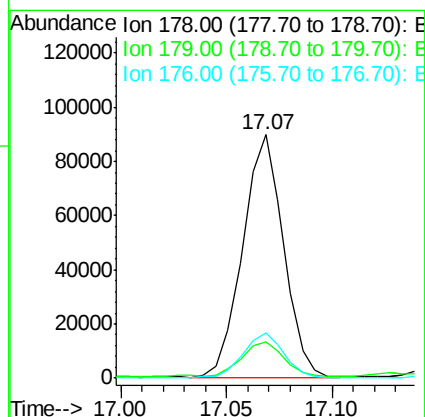
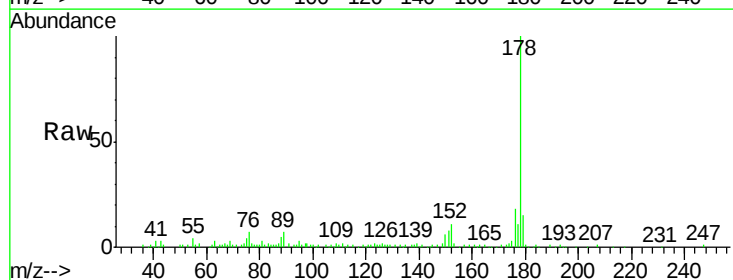


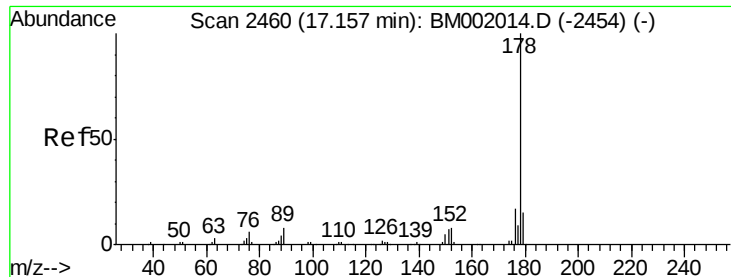

#71
 Anthracene
 Concen: 5.23 ng/ul
 RT: 17.07 min Scan# 2445
 Delta R.T. -0.09 min
 Lab File: BM002015.D
 Acq: 23 Jul 2015 14:20




Instrument :
 BNA_M
 ClientSampleId :
 C02MORE


Tgt Ion:178 Resp: 120425
 Ion Ratio Lower Upper
 178 100
 179 14.9 12.4 18.6
 176 18.4 14.3 21.5

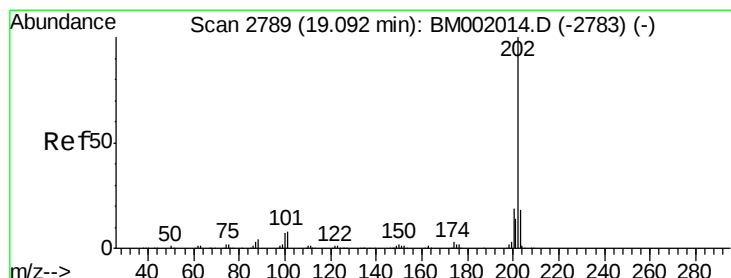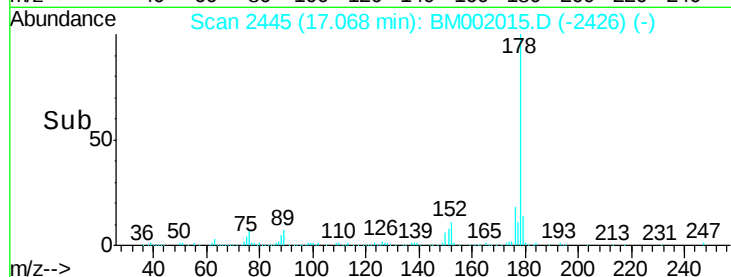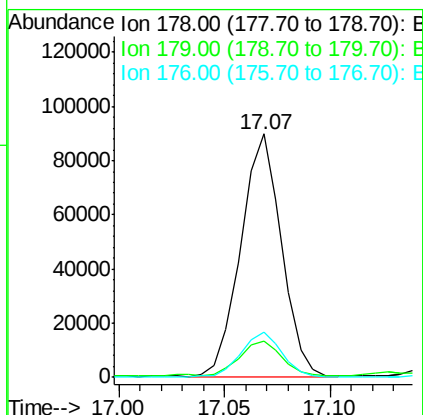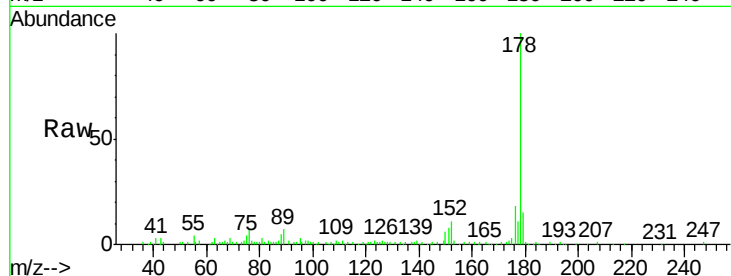

#76
 Fluoranthene
 Concen: 7.50 ng/ul
 RT: 19.09 min Scan# 2789
 Delta R.T. -0.00 min
 Lab File: BM002015.D
 Acq: 23 Jul 2015 14:20

Tgt Ion:202 Resp: 195636
 Ion Ratio Lower Upper
 202 100
 101 9.1 6.3 9.5
 100 6.8 5.0 7.4

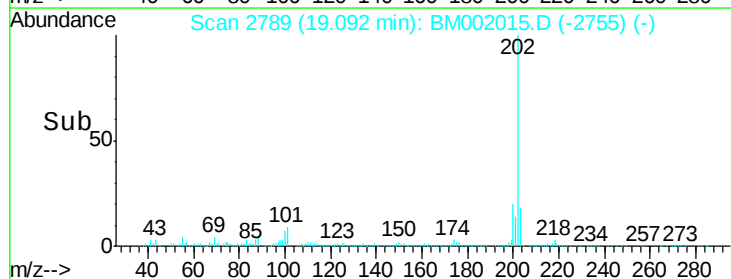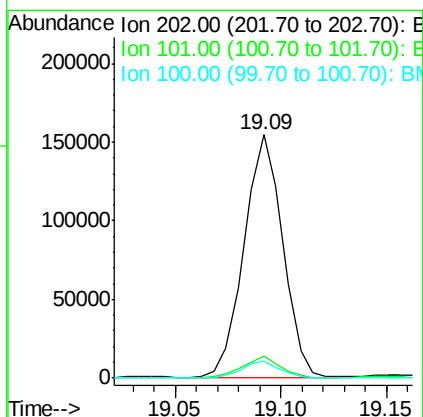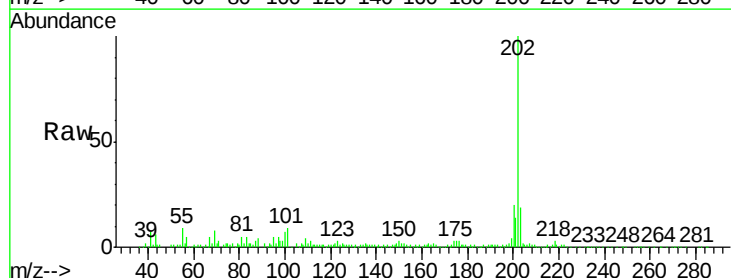

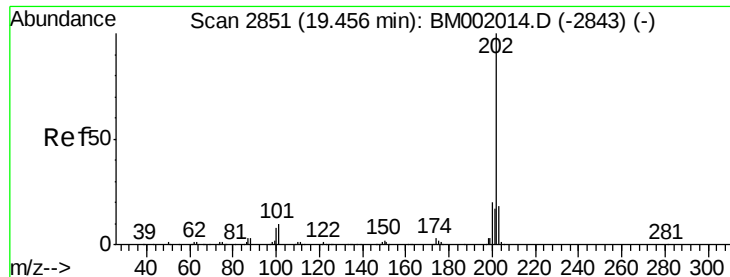

#79

Pyrene

Concen: 7.26 ng/ul

RT: 19.46 min Scan# 2851

Delta R.T. -0.00 min

Lab File: BM002015.D

Acq: 23 Jul 2015 14:20

Instrument :

BNA_M

ClientSampleId :

C02M0RE


Tgt Ion:202 Resp: 208171

Ion Ratio Lower Upper

202 100

101 10.5 7.3 10.9




100 8.3 6.2 9.4

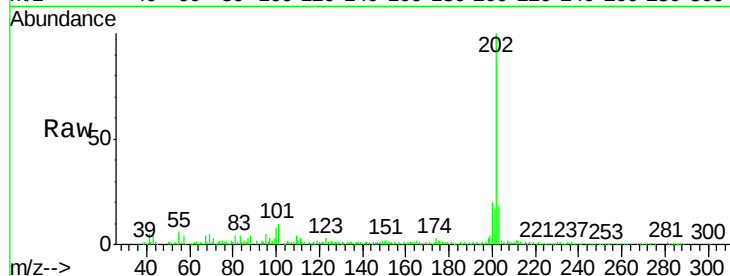

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

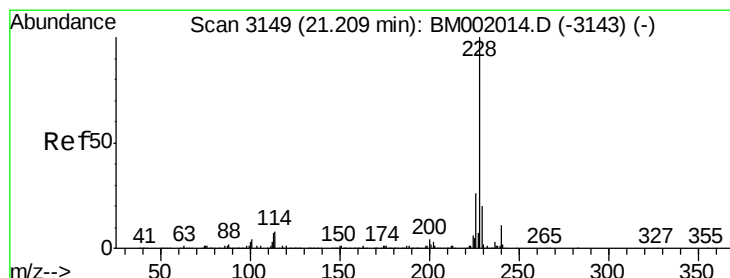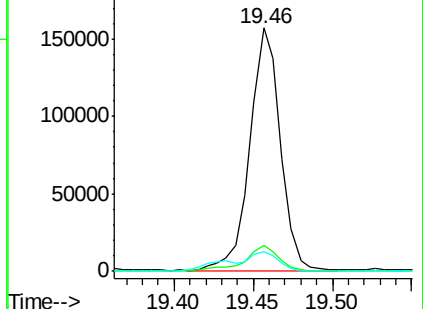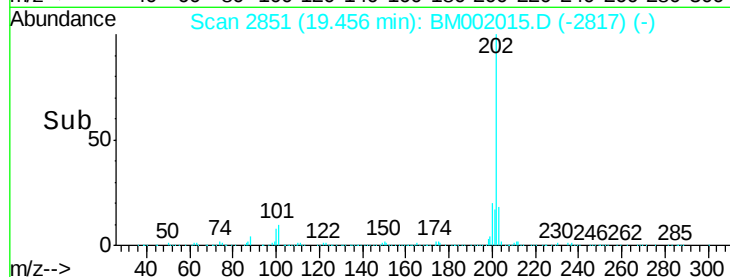

#82

Benzo(a)anthracene

Concen: 3.76 ng/ul

RT: 21.22 min Scan# 3150

Delta R.T. 0.01 min

Lab File: BM002015.D

Acq: 23 Jul 2015 14:20


Tgt Ion:228 Resp: 107406

Ion Ratio Lower Upper

228 100

229 22.3 15.4 23.2



226 28.3 20.7 31.1

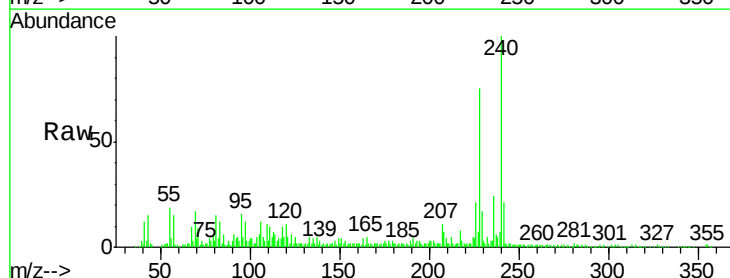


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E



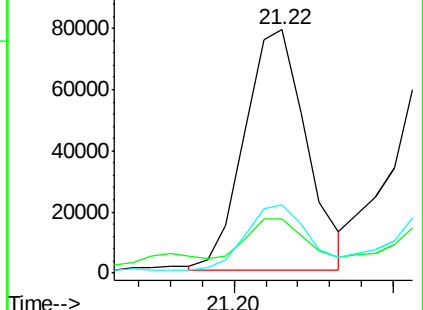
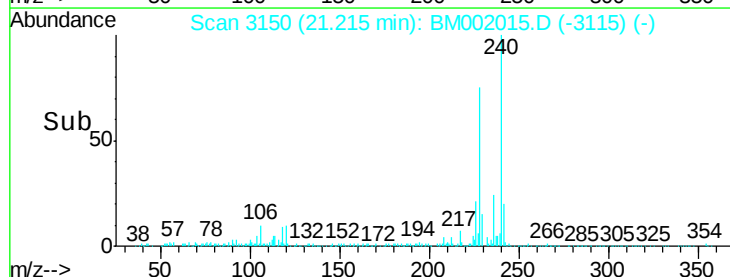


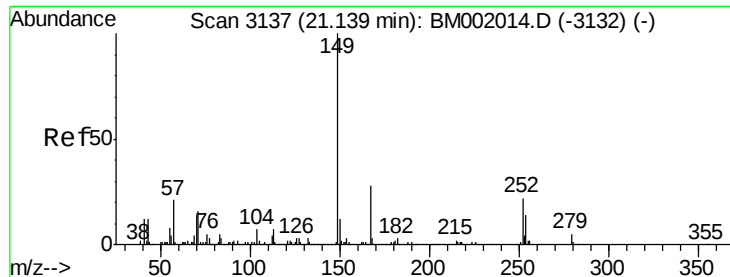

#83
Bis(2-ethylhexyl)phthalate
Concen: 1.76 ng/ul
RT: 21.14 min Scan# 3138
Delta R.T. 0.01 min
Lab File: BM002015.D
Acq: 23 Jul 2015 14:20




Instrument :
BNA_M
ClientSampleId :
C02MORE


Tgt Ion:149 Resp: 28218
Ion Ratio Lower Upper
149 100
167 28.1 23.2 34.8
279 6.7 4.5 6.7

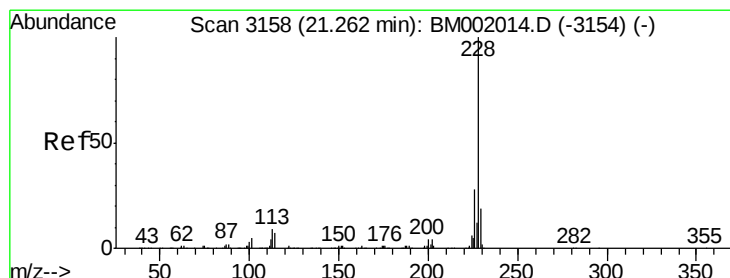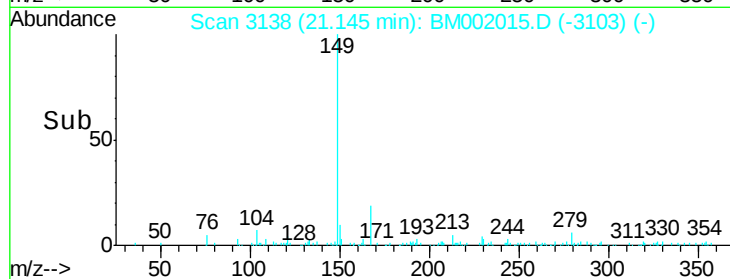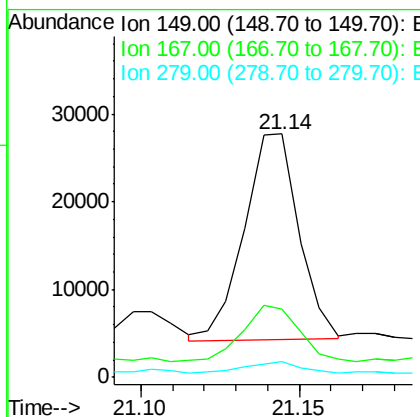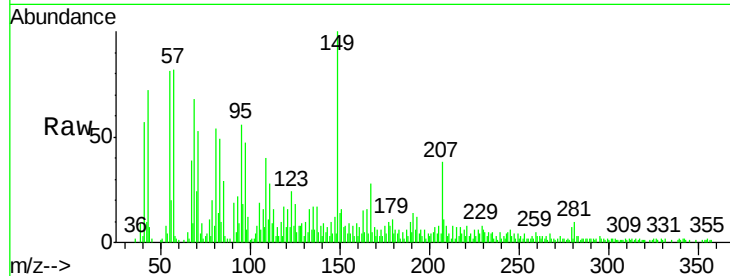

#84
Chrysene
Concen: 4.68 ng/ul
RT: 21.26 min Scan# 3158
Delta R.T. -0.00 min
Lab File: BM002015.D
Acq: 23 Jul 2015 14:20

Tgt Ion:228 Resp: 125169
Ion Ratio Lower Upper
228 100
226 28.0 23.0 34.4
229 22.0 15.6 23.4

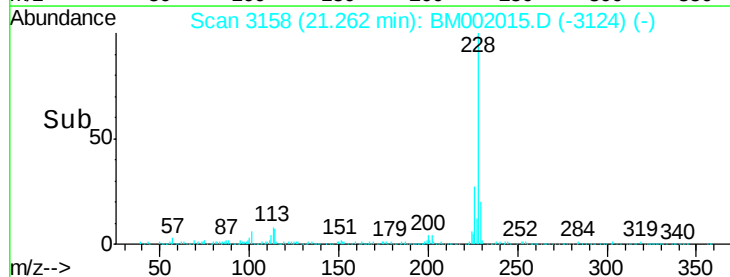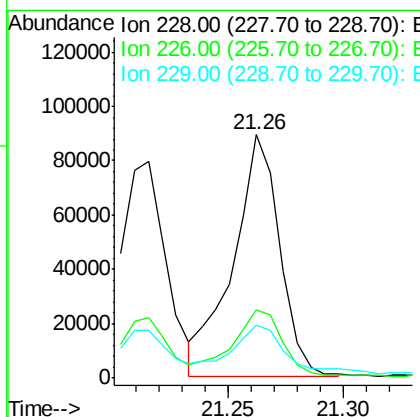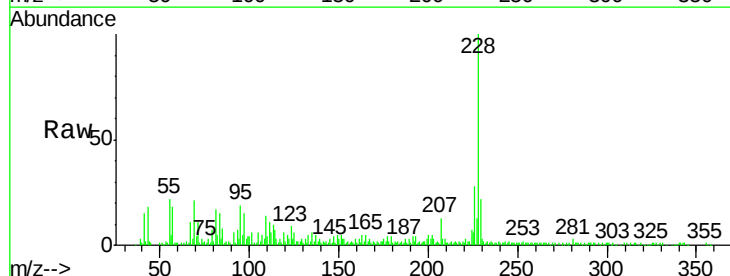


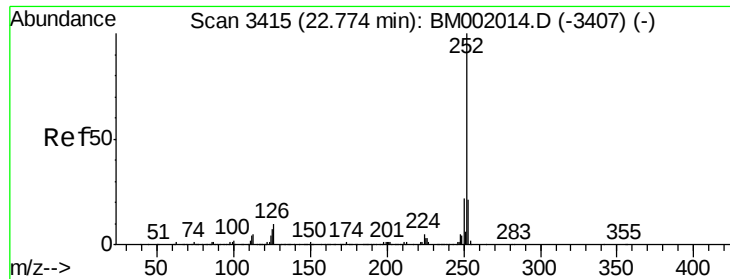




#87
Benzo(b)fluoranthene
Concen: 4.82 ng/ul
RT: 22.78 min Scan# 3416
Delta R.T. 0.01 min
Lab File: BM002015.D
Acq: 23 Jul 2015 14:20

Instrument :
BNA_M
ClientSampleId :
C02MORE

Tgt Ion:252 Resp: 141490
Ion Ratio Lower Upper
252 100
253 26.2 17.2 25.8#
125 16.9 5.3 7.9#

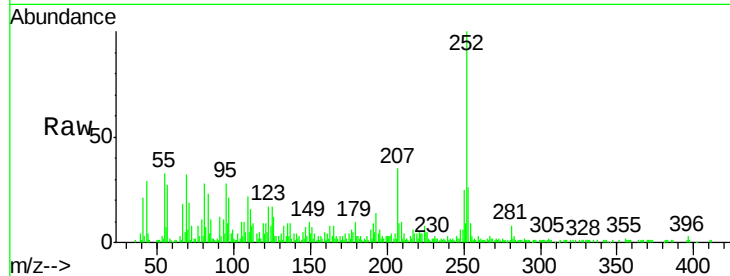


Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

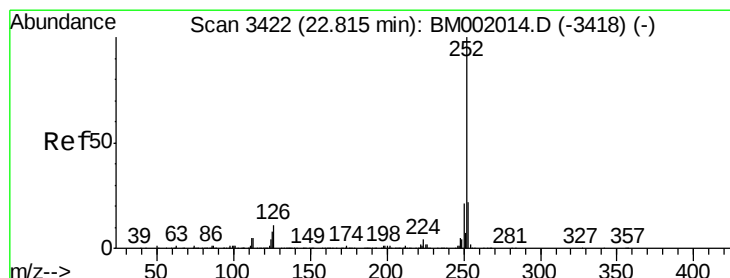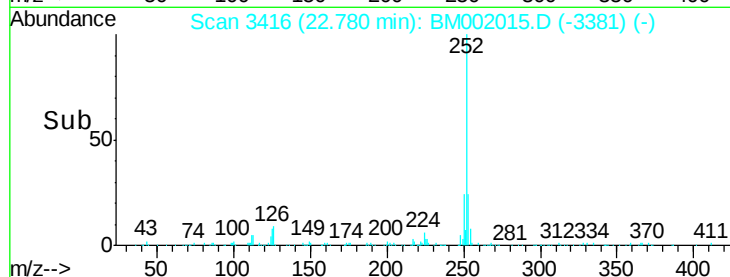
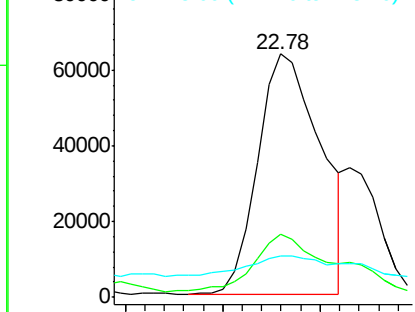



#88
Benzo(k)fluoranthene
Concen: 2.99 ng/ul
RT: 22.78 min Scan# 3416
Delta R.T. -0.04 min
Lab File: BM002015.D
Acq: 23 Jul 2015 14:20

Tgt Ion:252 Resp: 84416
Ion Ratio Lower Upper
252 100
253 26.2 17.4 26.2#
125 16.9 5.1 7.7#

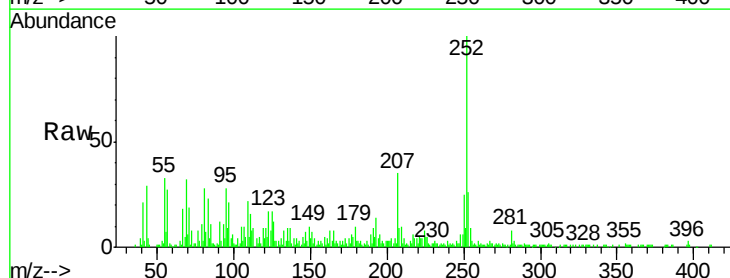

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

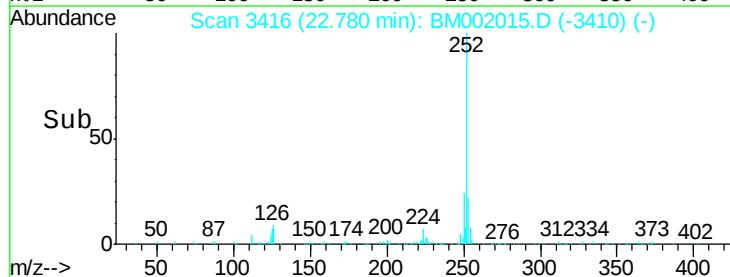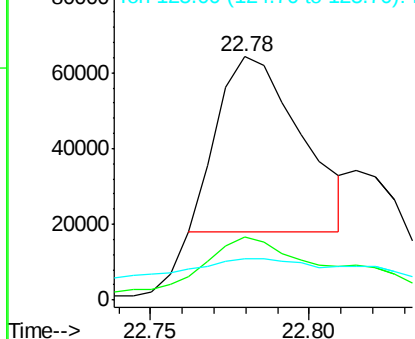

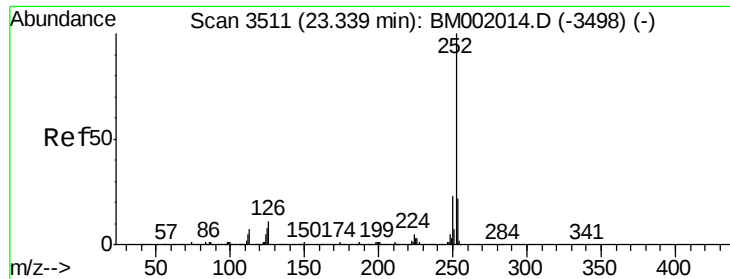

#90

Benzo(a)pyrene

Concen: 3.32 ng/ul

RT: 23.35 min Scan# 3513

Delta R.T. 0.01 min

Lab File: BM002015.D

Acq: 23 Jul 2015 14:20

Instrument :

BNA_M

ClientSampleId :

C02MORE


Tgt Ion:252 Resp: 91573

Ion Ratio Lower Upper

252 100

253 22.3 17.6 26.4




125 17.9 6.0 9.0#

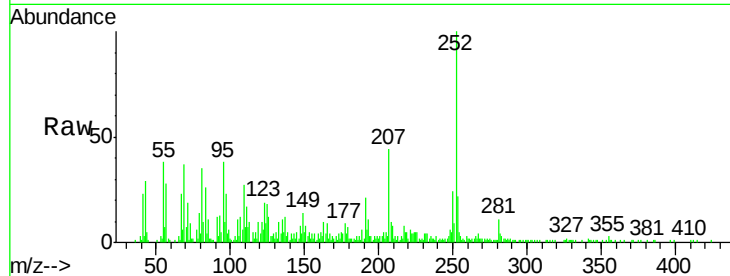

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

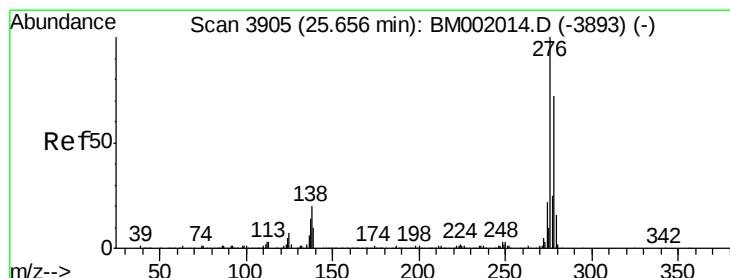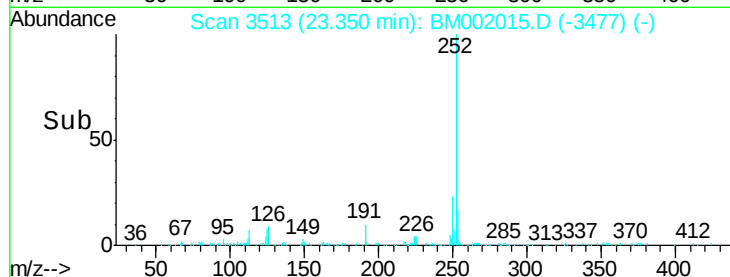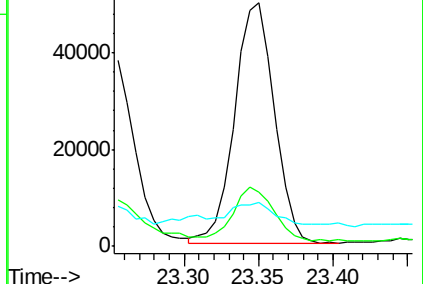

#91

Indeno(1,2,3-cd)pyrene

Concen: 2.08 ng/ul

RT: 25.66 min Scan# 3906

Delta R.T. 0.01 min

Lab File: BM002015.D

Acq: 23 Jul 2015 14:20


Tgt Ion:276 Resp: 60173

Ion Ratio Lower Upper

276 100

138 20.6 15.2 22.8



277 26.2 20.1 30.1

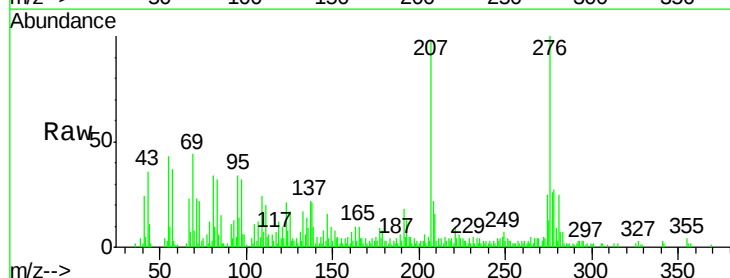


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

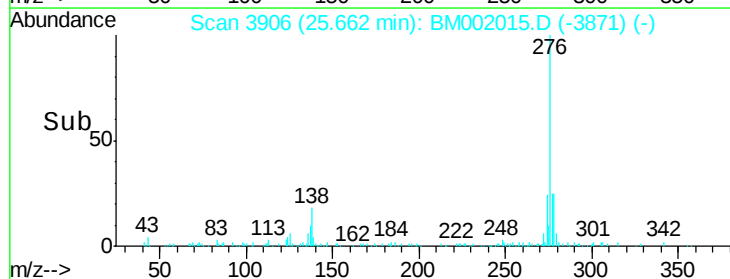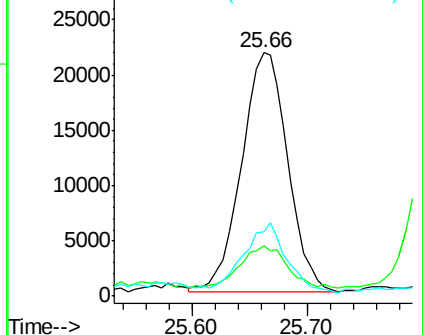

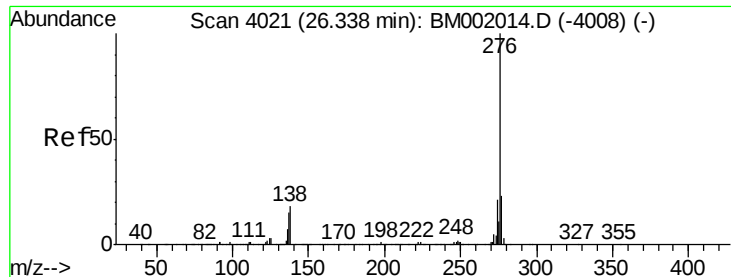

#93

Benzo(g,h,i)perylene

Concen: 2.54 ng/ul

RT: 26.35 min Scan# 4023

Delta R.T. 0.01 min

Lab File: BM002015.D


Acq: 23 Jul 2015 14:20

Instrument :

BNA_M

ClientSampleId :

C02M0RE

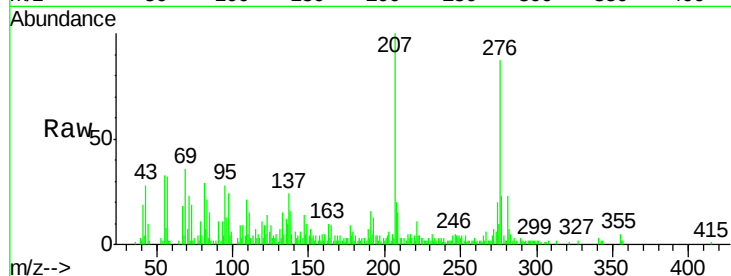


Tgt Ion: 276 Resp: 60503

Ion Ratio Lower Upper

276 100

138 18.6 12.7 19.1

277 26.0 18.6 28.0

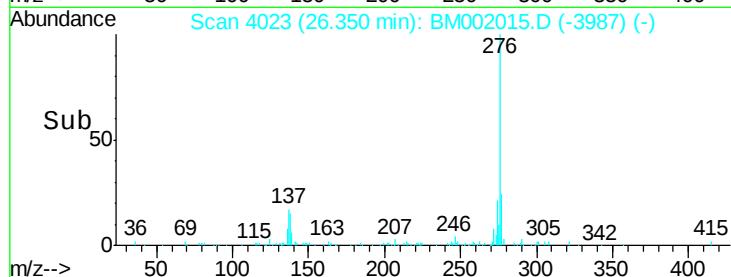

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

