

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072315\
Data File : BM002015.D
Acq On : 23 Jul 2015 14:20
Operator : TP/UM
Sample : G3000-02RE
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jul 24 12:47:47 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 01:29:30 2015
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
C02M0RE

Manual Integrations
APPROVED
apatel
7/24/2015 4:48:45 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	77439	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	309615	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	182282	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	412092	20.00	ng/ul	0.00
77) Chrysene-d12	21.23	240	479506	20.00	ng/ul	0.00
85) Perylene-d12	23.44	264	478826	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.09	96	7586	4.79	ng/uL	0.00
5) Phenol-d5	6.79	99	177515	28.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	96027	27.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	152186	30.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	141360	27.22	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	71233	30.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	82676	32.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	149939	28.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	94329	17.69	ng/ul	0.04
43) Dimethylphthalate-d6	13.69	166	409808	27.87	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	518967	29.35	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	68446	27.49	ng/ul	0.00
57) Fluorene-d10	15.27	176	355511	28.30	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	45131	16.91	ng/ul	0.00
70) Anthracene-d10	17.12	188	522388	27.00	ng/ul	0.00
78) Pyrene-d10	19.43	212	576195	26.31	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.30	264	561252	23.18	ng/ul	0.00

Target Compounds					Qvalue
16) 4-Methylphenol	8.40	108	10119	1.86 ng/ul	93
44) Dimethylphthalate	13.73	163	107364	7.18 ng/ul	98
69) Phenanthrene	17.07	178	119809	5.37 ng/ul	100
76) Fluoranthene	19.09	202	195636	7.50 ng/ul	97
79) Pyrene	19.46	202	208171	7.26 ng/ul	97
82) Benzo(a)anthracene	21.22	228	107406	3.76 ng/ul	95
83) Bis(2-ethylhexyl)phthalate	21.14	149	28218	1.76 ng/ul	98
84) Chrysene	21.26	228	125169	4.68 ng/ul	97
87) Benzo(b)fluoranthene	22.78	252	141490	4.82 ng/ul#	85
88) Benzo(k)fluoranthene	22.81	252	43523m	1.54 ng/ul	
90) Benzo(a)pyrene	23.35	252	91573	3.32 ng/ul#	92
91) Indeno(1,2,3-cd)pyrene	25.66	276	60173	2.08 ng/ul	97
93) Benzo(g,h,i)perylene	26.35	276	60503	2.54 ng/ul	94

T.P
07/23/2015

(#) = qualifier out of range (m) - manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072315\
 Data File : BM002015.D
 Acq On : 23 Jul 2015 14:20
 Operator : TP/UM
 Sample : G3000-02RE




Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jul 24 04:12:28 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 24 01:29:30 2015
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 C02M0RE

Manual Integrations
 APPROVED

apatel
 7/24/2015 4:48:45 PM

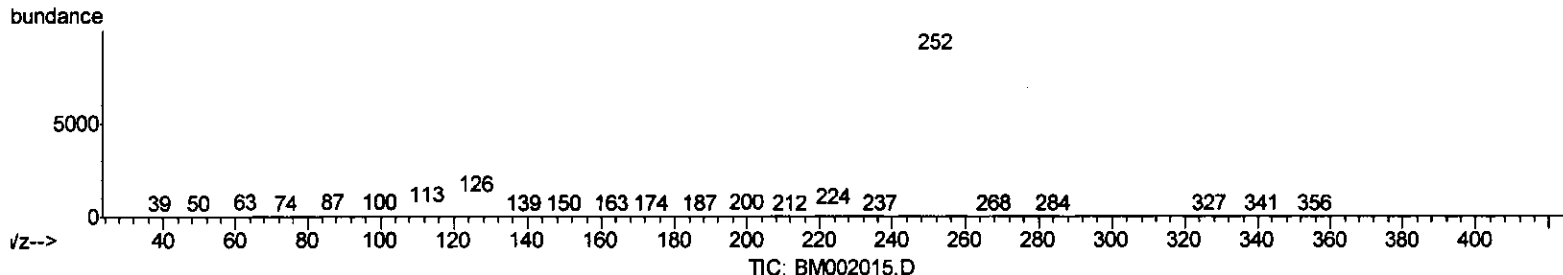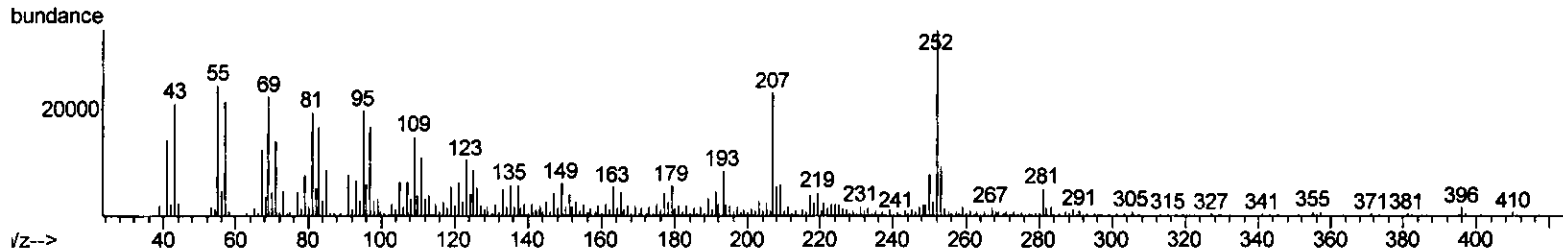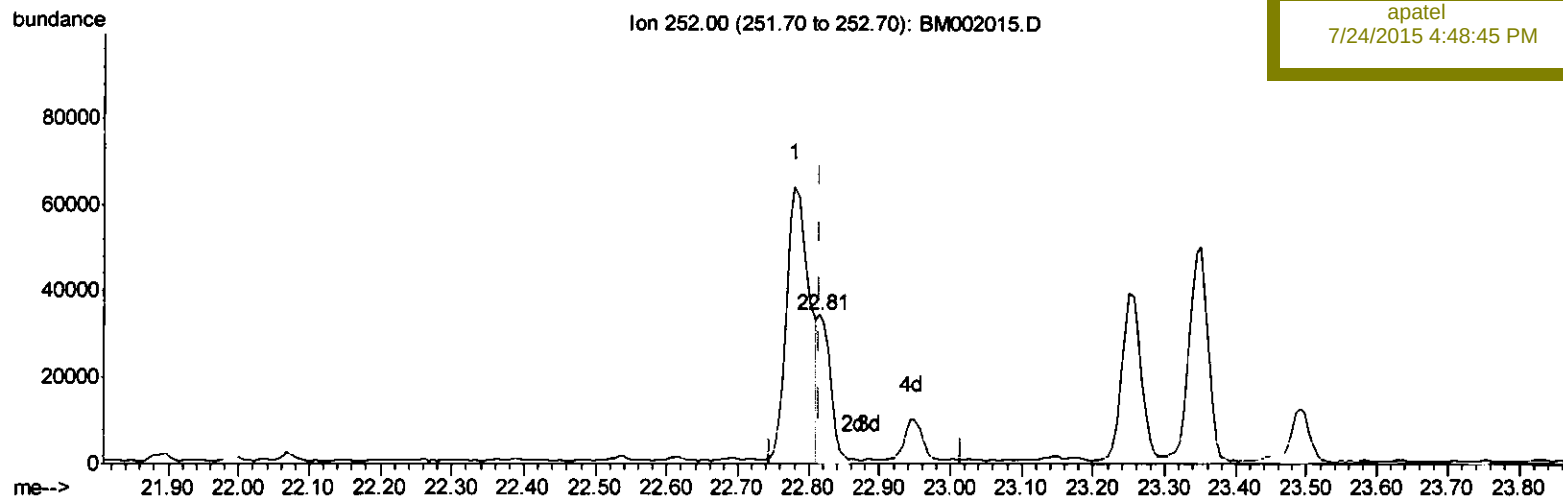

(88) Benzo(k)fluoranthene
 22.815min (-0.000) 1.54ng/ul m
 response 43523

Ion	Exp%	Act%
252.00	100	100
253.00	21.80	27.19#
125.00	6.40	25.54#
0.00	0.00	0.00

T.P
07/23/2015

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072315\
Data File : BM002015.D
Acq On : 23 Jul 2015 14:20
Operator : TP/UM
Sample : G3000-02RE


Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jul 24 01:36:18 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 01:29:30 2015
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
C02M0RE

Manual Integrations
APPROVED

apatel
7/24/2015 4:48:45 PM

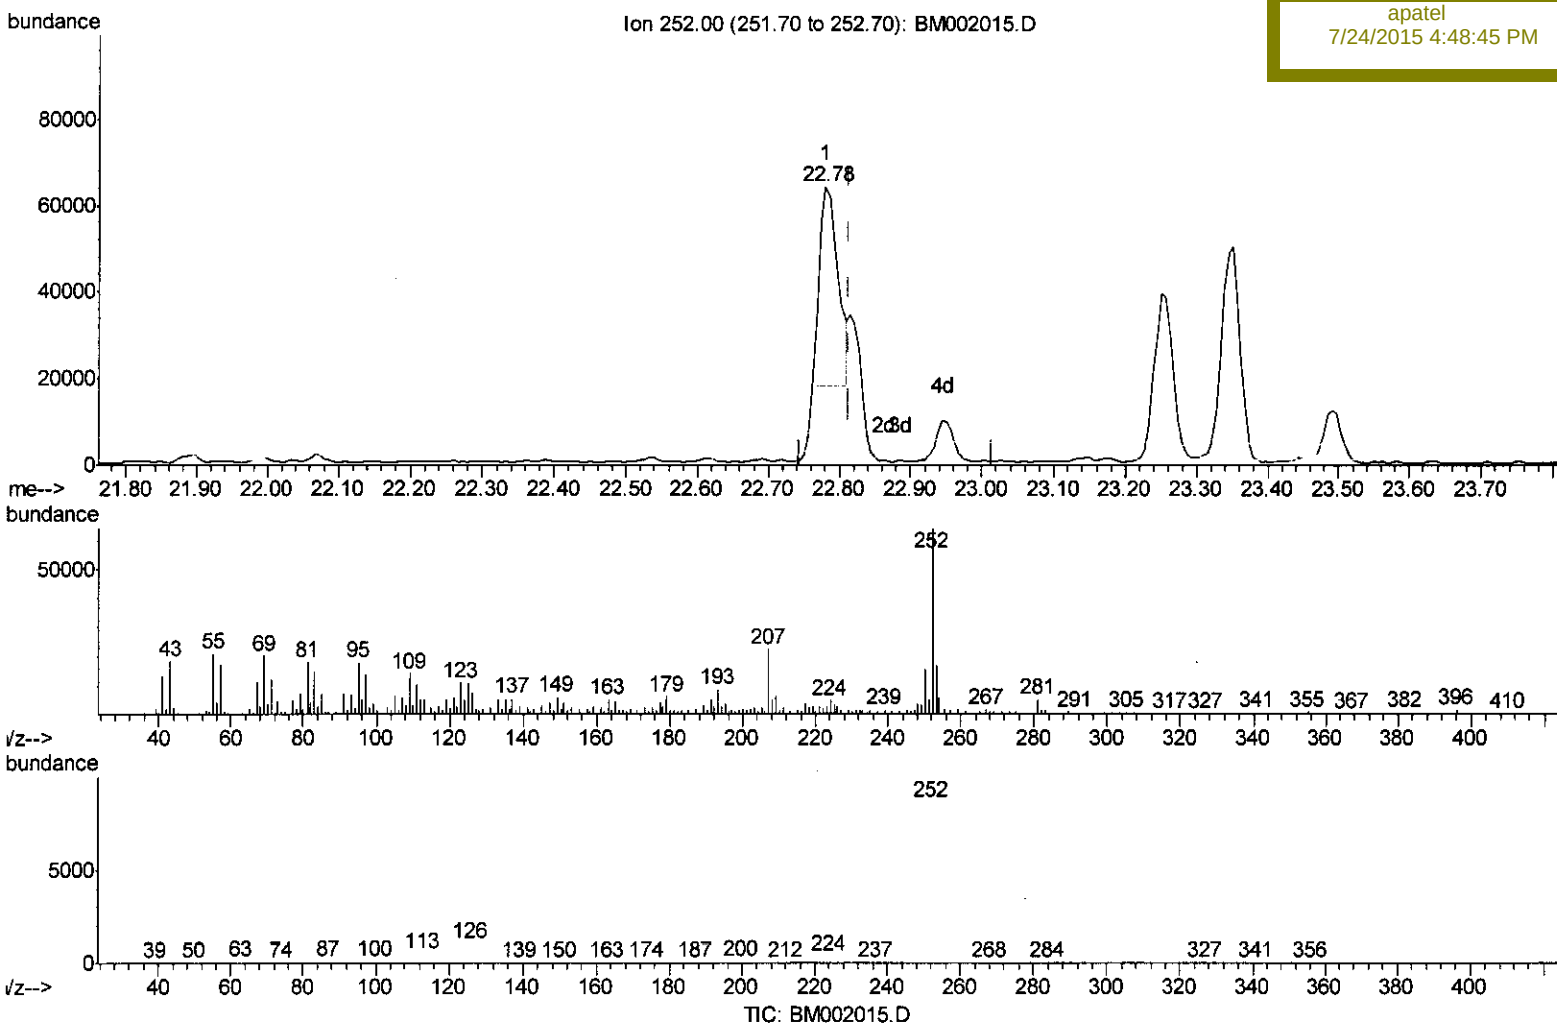

(88) Benzo(k)fluoranthene

22.780min (-0.035) 2.99ng/ul

response 84416

Ion	Exp%	Act%
252.00	100	100
253.00	21.80	26.19#
125.00	6.40	16.93#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072315\
Data File : BM002015.D
Acq On : 23 Jul 2015 14:20
Operator : TP/UM
Sample : G3000-02RE
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jul 24 12:47:47 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 01:29:30 2015
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
C02M0RE

Manual Integrations
APPROVED

apatel
7/24/2015 4:48:45 PM

