

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072315\
 Data File : BM002021.D
 Acq On : 23 Jul 2015 17:59
 Operator : TP/UM
 Sample : G3000-13RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C02B9RE

Quant Time: Jul 24 02:01:54 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 24 01:29:30 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	126713	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	484102	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.27	164	259322	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.03	188	531881	20.00	ng/ul	0.00
77) Chrysene-d12	21.23	240	566058	20.00	ng/ul	0.00
85) Perylene-d12	23.44	264	590601	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.09	96	2205	0.85	ng/uL	0.00
5) Phenol-d5	6.79	99	52765	5.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	29761	5.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	45278	5.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	38722	4.56	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	20189	5.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	19098	4.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	44074	5.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	51244	6.15	ng/ul	0.00
43) Dimethylphthalate-d6	13.69	166	127303	6.09	ng/ul	0.00
46) Acenaphthylene-d8	13.97	160	137098	5.45	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	14729	4.16	ng/ul	0.00
57) Fluorene-d10	15.27	176	92471	5.17	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul	
70) Anthracene-d10	17.12	188	135672	5.43	ng/ul	0.00
78) Pyrene-d10	19.43	212	139830	5.41	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	131823	4.41	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.73	163	50174	2.36 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072315\
Data File : BM002021.D
Acq On : 23 Jul 2015 17:59
Operator : TP/UM
Sample : G3000-13RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C02B9RE

Quant Time: Jul 24 02:01:54 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM071315.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 01:29:30 2015
Response via : Initial Calibration

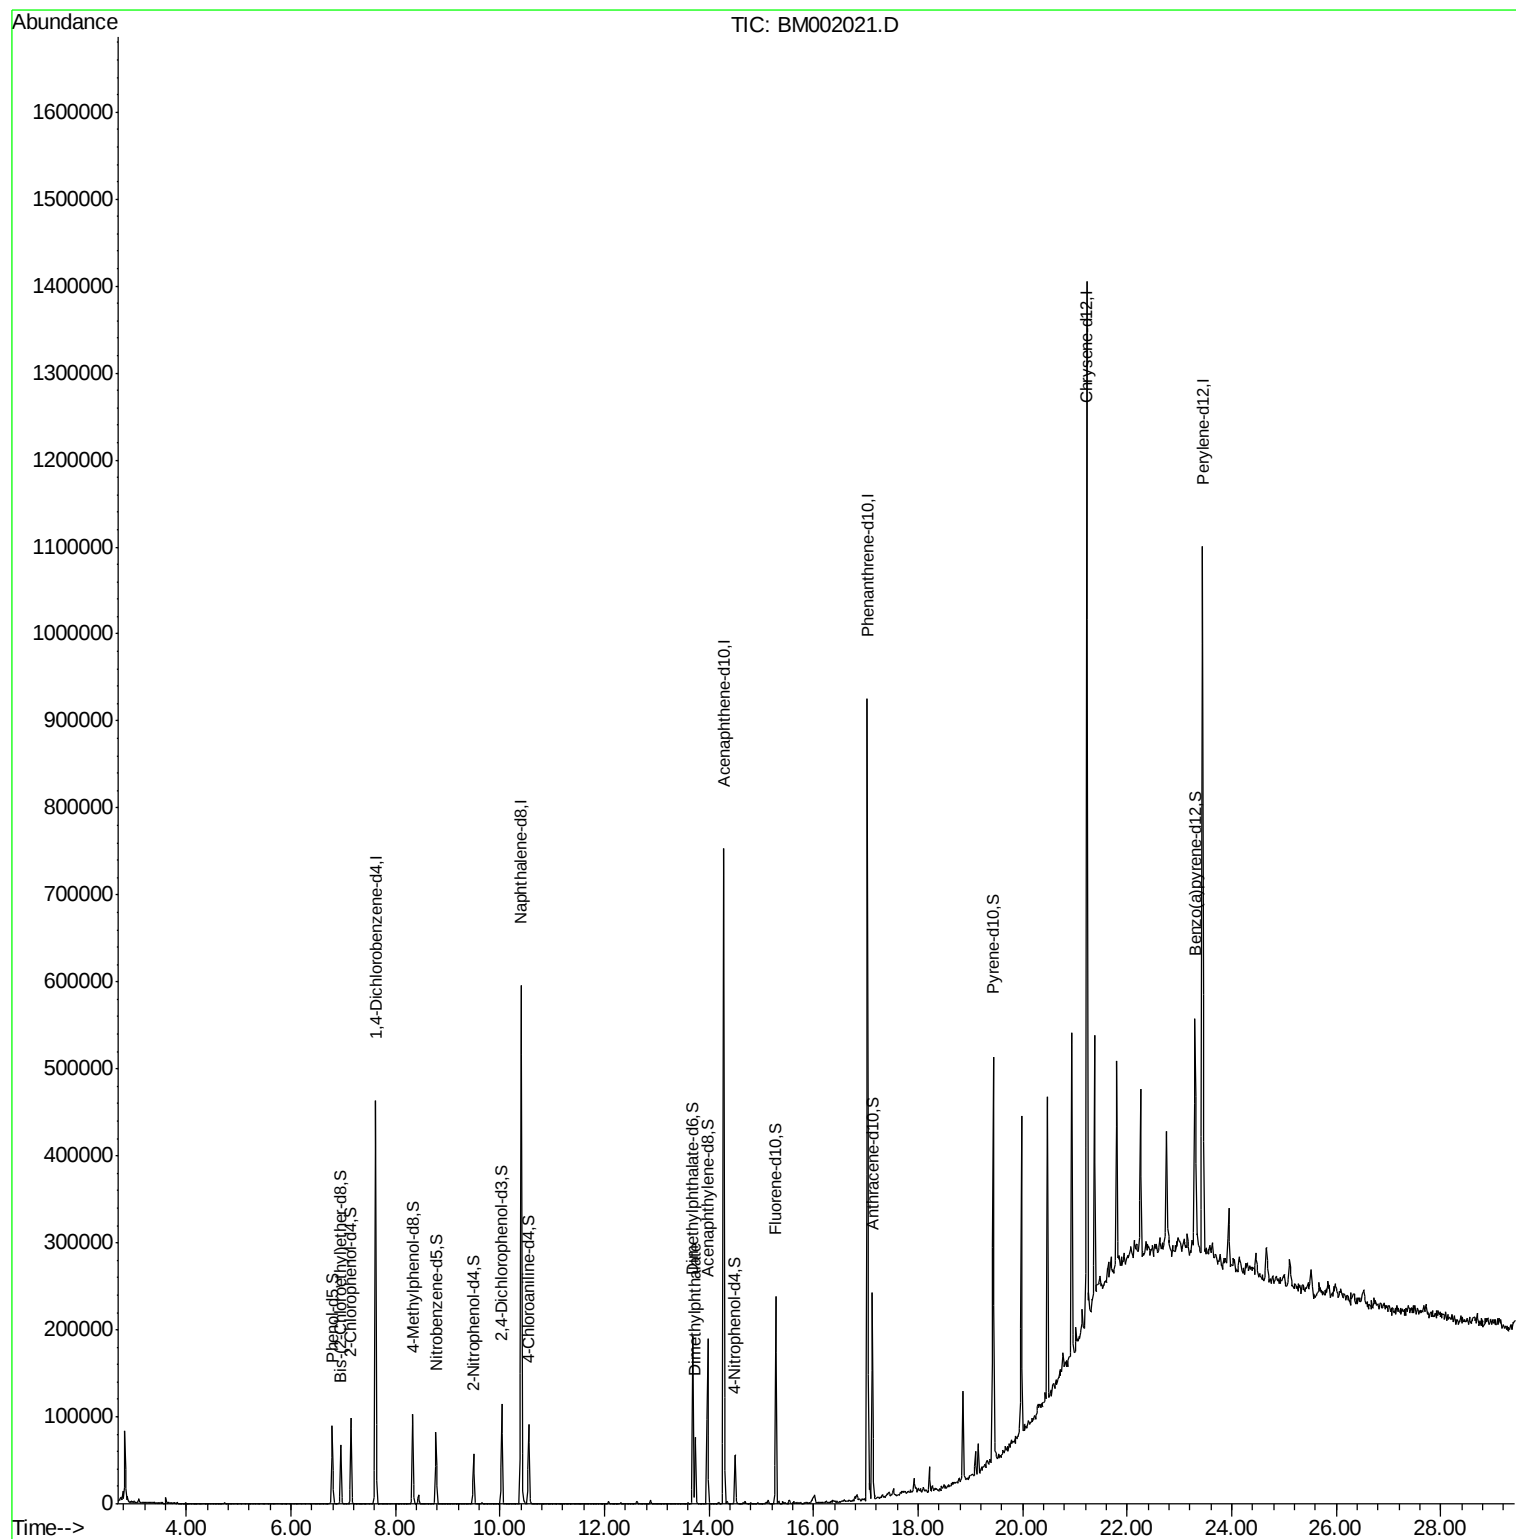


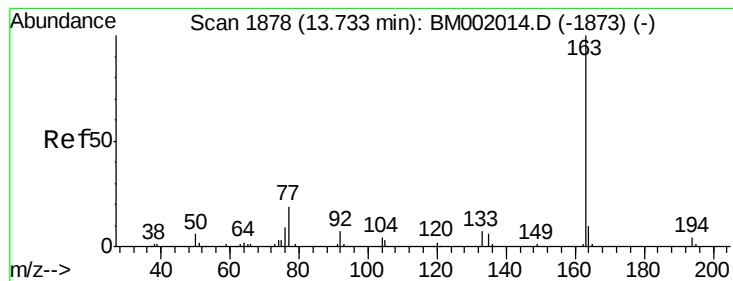

#44
 Dimethylphthalate
 Concen: 2.36 ng/ul
 RT: 13.73 min Scan# 1878
 Delta R.T. -0.00 min
 Lab File: BM002021.D
 Acq: 23 Jul 2015 17:59

Instrument :
 BNA_M
 ClientSampleId :
 C02B9RE

Tgt Ion:163 Resp: 50174
 Ion Ratio Lower Upper
 163 100
 194 4.4 3.5 5.3
 164 11.3 8.2 12.4

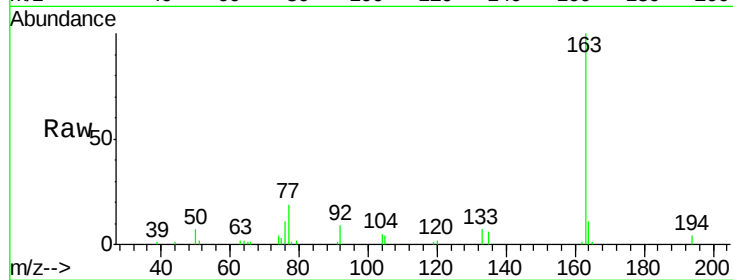

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

