


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072315\
 Data File : BM002013.D
 Acq On : 23 Jul 2015 11:57
 Operator : TP/UM
 Sample : DFTPP79
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP79

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042815.M
 Title : SVOA CALIBRATION
 Last Update : Tue Apr 28 06:36:34 2015

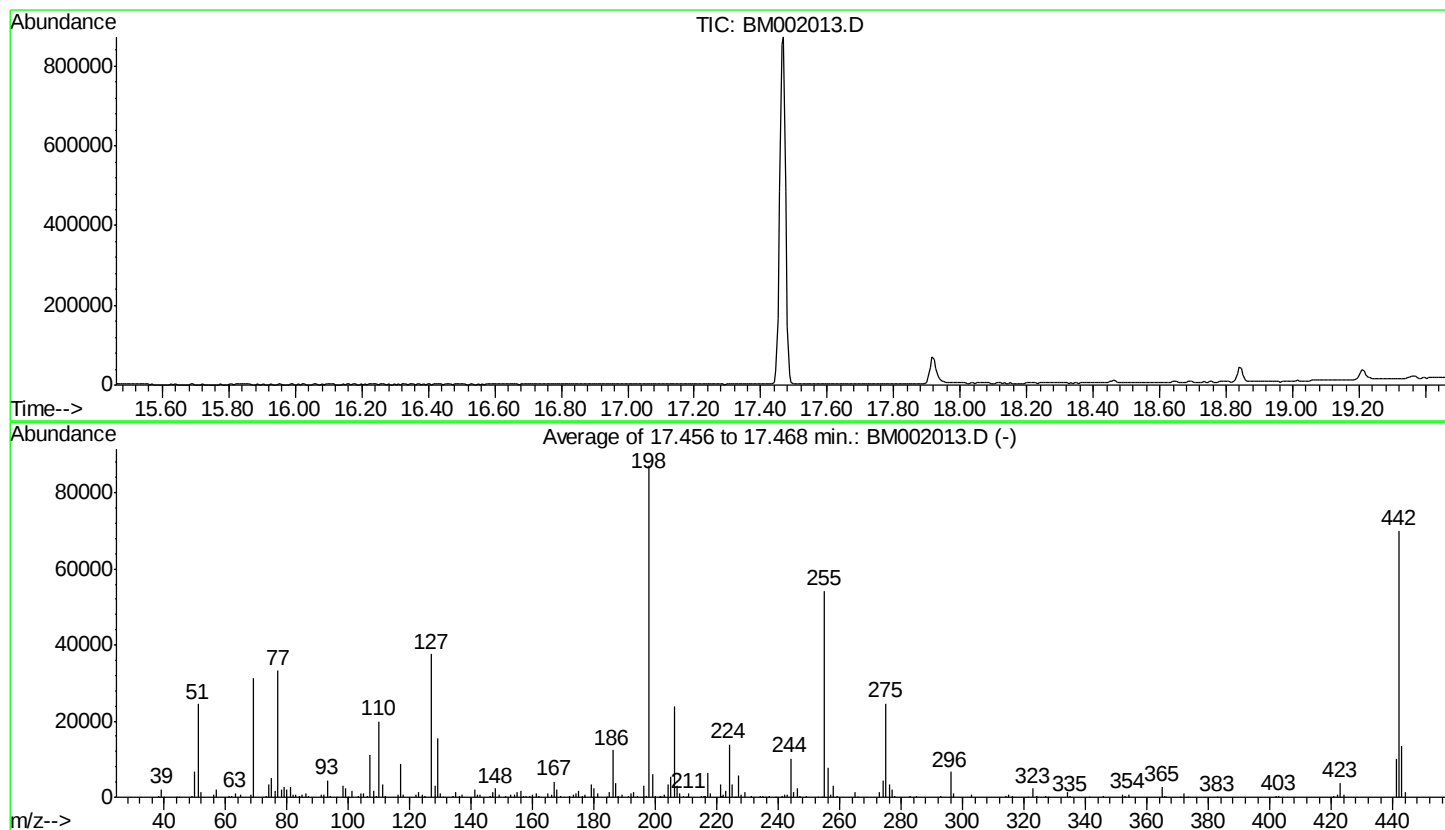

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	24464	PASS
68	69	0.00	2	1.9	607	PASS
69	198	0.00	100	35.8	31210	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	37605	PASS
197	198	0.00	2	0.5	401	PASS
198	198	100	100	100.0	87130	PASS
199	198	5	9	7.0	6116	PASS
275	198	10	60	28.2	24581	PASS
365	198	1	100	3.3	2855	PASS
441	443	0.01	100	73.2	9941	PASS
442	198	50	100	80.4	70034	PASS
443	442	15	24	19.4	13584	PASS

m/z	Abundance
39.10	1711.0
39.90	520.0
44.00	1186.0
48.90	300.0
50.00	5073.0
51.10	19352.0
52.00	1203.0
55.10	312.0
56.00	653.0
57.00	1487.0
61.00	363.0
62.00	407.0
63.00	879.0
65.00	496.0
68.00	565.0
69.00	24120.0
73.10	514.0
74.00	2747.0
75.00	4008.0
76.00	1187.0
77.10	25184.0
78.10	1777.0
79.00	1840.0
79.90	1485.0
81.00	1987.0
82.00	462.0
83.00	492.0
85.00	652.0
86.00	819.0
90.90	632.0
92.00	678.0
93.00	3352.0
98.00	2660.0
99.00	1910.0
101.00	1179.0
103.00	357.0
103.90	605.0
104.90	704.0
107.00	8196.0
108.00	1146.0
110.00	14351.0
111.00	2637.0
116.00	653.0
117.00	6384.0
117.90	555.0
121.90	559.0
122.90	872.0
124.00	363.0
125.00	418.0
127.00	27208.0
128.00	2182.0
129.00	11766.0
130.00	857.0
134.00	327.0
135.00	1003.0
137.00	481.0
141.00	1649.0
142.00	556.0
142.80	420.0
145.90	366.0
147.00	951.0
148.00	1783.0
149.00	467.0
153.00	475.0
154.00	404.0
155.00	786.0
156.00	1364.0
160.00	480.0
160.90	571.0
164.90	694.0
165.90	523.0
167.00	3053.0
168.00	1497.0
169.00	342.0
172.00	329.0
173.00	429.0
174.00	592.0
174.90	1140.0
175.90	318.0
176.80	422.0
177.10	395.0
179.00	2210.0
180.00	1626.0
181.00	890.0
184.90	914.0
186.00	8543.0
187.00	2382.0
189.00	424.0
191.00	411.0
192.00	801.0
192.90	853.0

Instrument :
BNA_M
ClientSampleId :
DFTPP79

196.00	2073.0
197.10	453.0
197.90	57664.0
199.00	4128.0
200.00	318.0
201.40	332.0
203.00	447.0
204.00	2156.0
205.00	3712.0
206.00	15914.0
207.00	2415.0
208.00	559.0
211.00	509.0
215.90	302.0
217.00	4489.0
218.00	573.0
220.90	2016.0
221.70	823.0
222.90	858.0
224.00	9087.0
225.00	2354.0
227.00	3930.0
227.90	447.0
229.00	830.0
231.10	339.0
234.90	342.0
242.00	450.0
242.90	539.0
244.00	6671.0
245.00	913.0
246.00	1659.0
246.90	334.0
255.00	33680.0
256.00	5245.0
257.00	412.0
258.00	2005.0
265.00	861.0
272.90	1011.0
274.00	2587.0
275.00	14472.0
276.00	1931.0
276.90	1280.0
296.00	4218.0
296.90	612.0
302.90	500.0
314.90	418.0
323.00	1355.0
334.00	648.0
354.10	563.0
365.00	1725.0
365.90	321.0
372.00	621.0
421.90	380.0
423.00	1992.0
424.00	561.0
441.10	4690.0
442.10	35856.0
443.00	7032.0
444.00	718.0

Instrument :
BNA_M
ClientSampleId :
DFTPP79

m/z	Abundance
38.00	427.0
39.00	2402.0
40.00	569.0
43.00	356.0
44.00	1143.0
45.00	316.0
49.00	321.0
50.00	8104.0
51.10	28640.0
52.00	1670.0
55.00	302.0
56.10	1065.0
57.00	2233.0
61.10	464.0
62.00	519.0
63.00	1436.0
65.00	733.0
68.00	629.0
69.00	36864.0
73.00	508.0
74.00	3924.0
75.00	5952.0
76.00	1936.0
77.10	39584.0
78.00	2228.0
79.00	3204.0
80.00	2132.0
81.00	2985.0
82.00	813.0
82.90	871.0
83.90	340.0
84.90	698.0
86.00	903.0
87.00	512.0
91.00	851.0
91.90	930.0
93.00	5224.0
93.90	441.0
98.00	3499.0
98.90	2922.0
100.00	309.0
101.00	1778.0
103.10	696.0
104.00	1216.0
105.00	954.0
106.00	424.0
107.00	13197.0
108.00	2024.0
109.00	603.0
110.00	23960.0
111.00	3626.0
111.90	406.0
116.00	749.0
117.00	10842.0
118.00	627.0
122.00	903.0
123.00	1665.0
123.90	614.0
124.90	606.0
127.00	44816.0
128.00	3351.0
129.00	17560.0
130.00	1547.0
130.90	336.0
133.90	622.0
135.00	1490.0
135.90	624.0
137.00	815.0
141.00	2446.0
142.00	968.0
142.90	698.0
146.00	647.0
147.00	1299.0
148.00	2781.0
149.00	670.0
151.20	368.0
152.90	860.0
154.00	644.0
155.00	1591.0
156.10	1784.0
157.10	343.0
158.00	481.0
159.00	464.0
160.00	1033.0
160.90	1114.0
161.90	365.0
165.00	1013.0
166.00	1059.0
167.00	4536.0
168.00	2177.0
168.90	459.0

Instrument :
BNA_M
ClientSampleId :
DFTPP79

171.90	583.0
173.00	583.0
174.00	1188.0
175.00	2228.0
176.00	459.0
176.90	835.0
178.90	3747.0
180.00	2222.0
181.00	1358.0
184.00	386.0
185.00	1854.0
186.00	14387.0
187.00	4210.0
188.00	328.0
188.90	1004.0
190.90	520.0
192.00	1322.0
193.00	1473.0
194.10	328.0
196.00	3220.0
197.10	752.0
198.00	102456.0
198.90	7086.0
199.90	504.0
201.10	349.0
201.60	331.0
203.00	789.0
204.00	3751.0
205.00	6225.0
206.00	28224.0
207.00	4323.0
208.00	1072.0
209.00	391.0
209.90	354.0
210.80	924.0
215.00	364.0
216.10	667.0
217.00	7077.0
217.90	969.0
221.00	4312.0
221.90	1100.0
223.00	1844.0
224.00	16187.0
225.00	3992.0
225.90	365.0
227.00	6849.0
228.00	884.0
229.00	1401.0
230.90	533.0
233.90	490.0
234.90	383.0
235.90	397.0
237.00	428.0
241.00	374.0
242.10	807.0
242.90	714.0
244.00	11275.0
245.10	1743.0
246.00	2578.0
246.90	383.0
249.00	392.0
254.10	384.0
255.00	61360.0
256.00	8664.0
257.00	872.0
258.00	3450.0
259.00	611.0
265.00	1638.0
273.00	1666.0
274.00	5161.0
275.00	28240.0
276.00	3805.0
277.00	2238.0
278.00	422.0
283.00	305.0
285.10	350.0
293.00	634.0
296.00	7208.0
297.00	1280.0
302.90	833.0
313.90	379.0
315.00	899.0
316.00	516.0
323.00	2891.0
324.00	508.0
326.90	506.0
327.90	366.0
334.00	1726.0
335.10	445.0
341.00	333.0
346.00	527.0
352.00	777.0
353.00	550.0
354.00	709.0
365.00	2945.0

Instrument :
BNA_M
ClientSampleId :
DFTPP79

365.90	583.0
372.00	901.0
402.00	350.0
403.00	723.0
420.90	436.0
421.90	600.0
423.10	4127.0
424.00	765.0
441.00	10928.0
442.10	76080.0
443.10	14737.0
443.90	1466.0

Instrument :
BNA_M
ClientSampleId :
DFTPP79

m/z	Abundance
38.00	336.0
39.00	2145.0
39.90	540.0
43.00	337.0
44.00	1529.0
49.00	337.0
50.10	6696.0
51.10	25400.0
52.00	1199.0
55.00	358.0
56.00	785.0
57.00	2341.0
61.00	317.0
62.00	412.0
63.00	1005.0
65.00	660.0
68.10	629.0
69.00	32648.0
73.10	489.0
74.10	3230.0
75.00	5235.0
76.00	1861.0
77.10	35064.0
78.10	2446.0
79.00	2746.0
80.00	2015.0
81.00	2884.0
82.00	673.0
83.00	912.0
84.00	310.0
85.00	660.0
86.00	916.0
87.00	340.0
91.10	825.0
92.00	730.0
93.00	4716.0
93.80	326.0
96.00	315.0
98.00	3343.0
99.00	2704.0
100.90	1791.0
102.90	430.0
104.00	1071.0
105.00	924.0
105.90	401.0
107.00	12033.0
108.00	1863.0
109.10	513.0
110.00	21328.0
111.00	3456.0
111.90	526.0
115.90	621.0
117.00	9166.0
118.00	617.0
122.00	885.0
122.90	1249.0
124.00	640.0
124.90	428.0
127.00	40792.0
128.00	3222.0
129.00	17232.0
130.00	1141.0
134.00	565.0
135.10	1581.0
136.00	587.0
137.00	705.0
141.00	2339.0
141.90	810.0
143.00	579.0
146.00	426.0
147.00	1474.0
148.00	2457.0
148.90	613.0
151.00	389.0
153.00	965.0
154.00	547.0
155.00	1188.0
156.00	1762.0
157.10	397.0
157.90	425.0
159.00	434.0
159.90	796.0
161.00	1275.0
162.00	303.0
164.90	1204.0
165.90	662.0
167.00	4944.0
168.00	2460.0
168.90	426.0
172.00	493.0
173.10	596.0

Instrument :
BNA_M
ClientSampleId :
DFTPP79

174.00	1019.0
175.00	2209.0
176.00	667.0
176.90	1211.0
178.90	3692.0
180.10	2835.0
181.00	1201.0
185.00	1580.0
186.00	14410.0
187.00	4132.0
187.90	546.0
188.90	959.0
191.00	541.0
192.00	1206.0
193.00	1263.0
193.90	370.0
196.00	3341.0
196.80	564.0
198.00	101272.0
198.90	7136.0
200.00	598.0
201.30	506.0
201.80	479.0
203.00	807.0
204.00	4112.0
205.00	6614.0
206.00	27784.0
207.00	4288.0
207.90	1043.0
208.90	366.0
210.10	420.0
210.90	1262.0
215.00	365.0
215.90	709.0
216.90	7667.0
217.90	1030.0
221.00	4167.0
221.80	1075.0
222.90	2041.0
224.00	16552.0
225.00	4142.0
226.10	482.0
227.00	6857.0
228.00	1009.0
229.00	1593.0
231.00	557.0
233.90	505.0
234.90	501.0
237.10	583.0
238.90	377.0
241.00	454.0
241.90	730.0
243.00	968.0
244.00	12809.0
245.10	1549.0
246.00	2702.0
247.00	684.0
248.90	344.0
252.80	313.0
255.00	67920.0
256.00	9754.0
256.90	710.0
258.00	3419.0
258.90	524.0
265.00	1612.0
265.90	301.0
273.00	1601.0
274.00	5407.0
275.00	31032.0
276.00	4144.0
277.00	2820.0
277.90	479.0
283.00	374.0
285.00	530.0
293.00	516.0
296.00	8402.0
297.00	1288.0
303.00	994.0
314.00	429.0
314.90	934.0
316.00	477.0
321.00	358.0
323.00	2787.0
324.00	608.0
326.90	391.0
334.10	1864.0
335.00	405.0
345.90	716.0
352.00	827.0
353.00	514.0
354.00	1061.0
365.00	3897.0
366.10	509.0
370.90	334.0
372.00	1452.0

Instrument :
BNA_M
ClientSampleId :
DFTPP79

373.10	351.0
383.00	407.0
401.90	533.0
403.00	703.0
420.90	734.0
422.00	864.0
423.10	5058.0
424.10	1012.0
441.10	14205.0
442.10	98168.0
443.10	18984.0
444.00	1665.0

Instrument :
BNA_M
ClientSampleId :
DFTPP79

m/z	Abundance
39.90	410.0
41.00	405.0
43.10	367.0
44.00	1255.0
55.00	327.0
207.00	528.0

Instrument :
BNA_M
ClientSampleId :
DFTPP79