




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072324\
Data File : BM046771.D
Acq On : 23 Jul 2024 10:52
Operator : MA/JU
Sample : PB162090BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK090

Manual IntegrationsAPPROVED

Quant Time: Jul 23 11:36:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 19 11:38:04 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

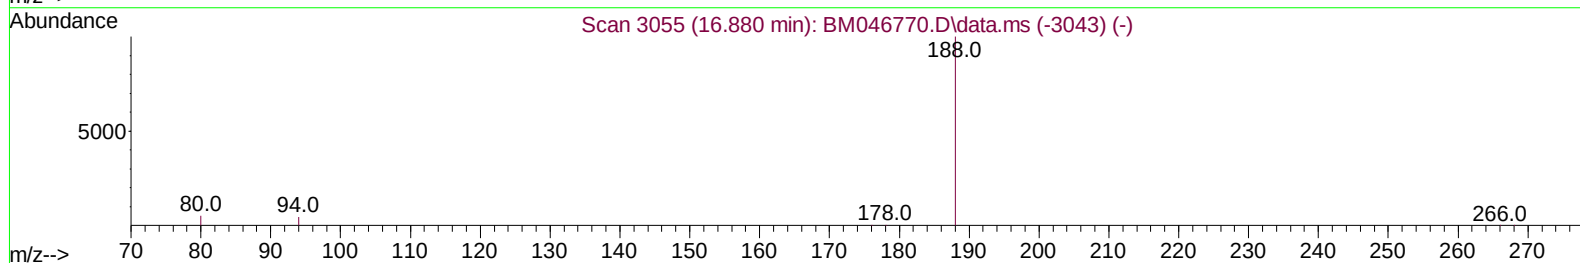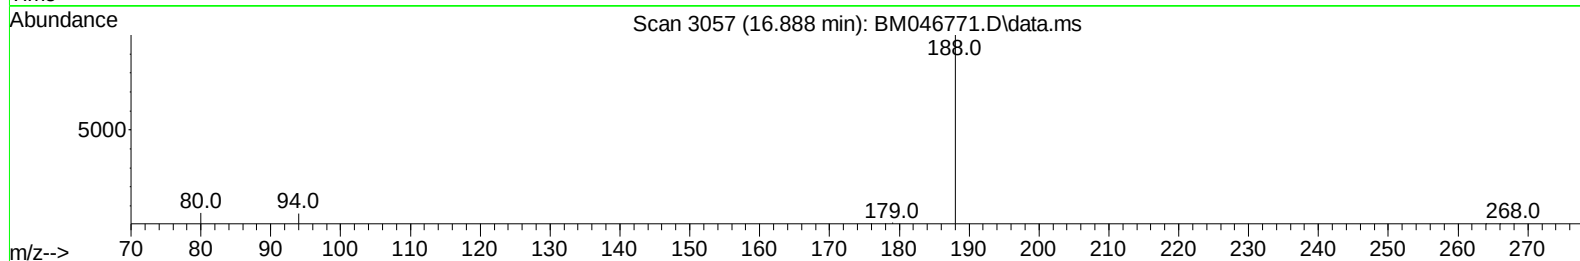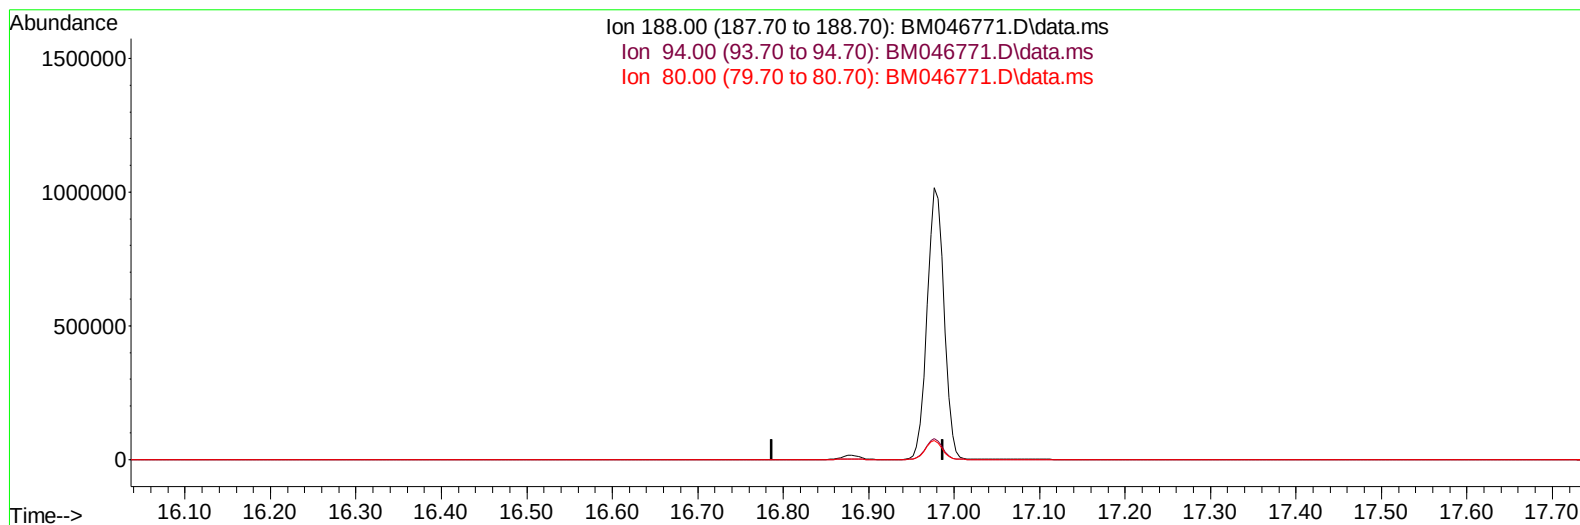

TIC: BM046771.D\data.ms

(13) Phenanthrene-d10 (I)

16.887min (-16.887) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.40	0.00#
80.00	6.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072324\
Data File : BM046771.D
Acq On : 23 Jul 2024 10:52
Operator : MA/JU
Sample : PB162090BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK090

Manual IntegrationsAPPROVED

Quant Time: Jul 23 11:36:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 19 11:38:04 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

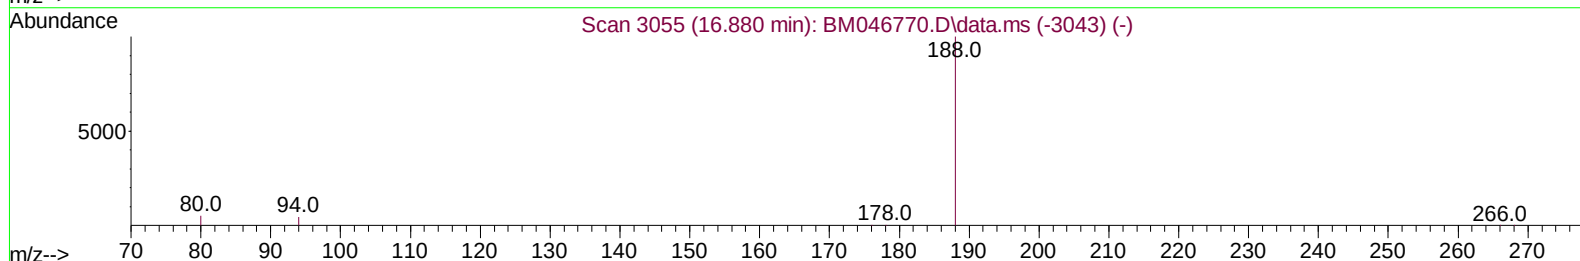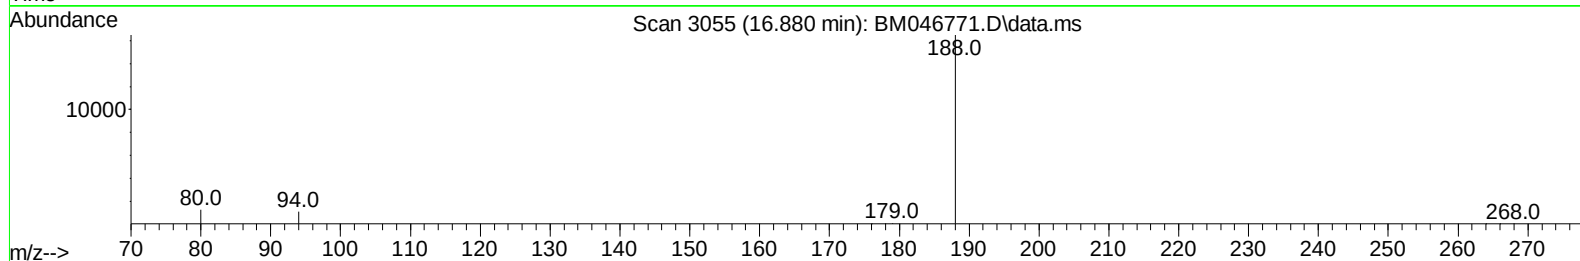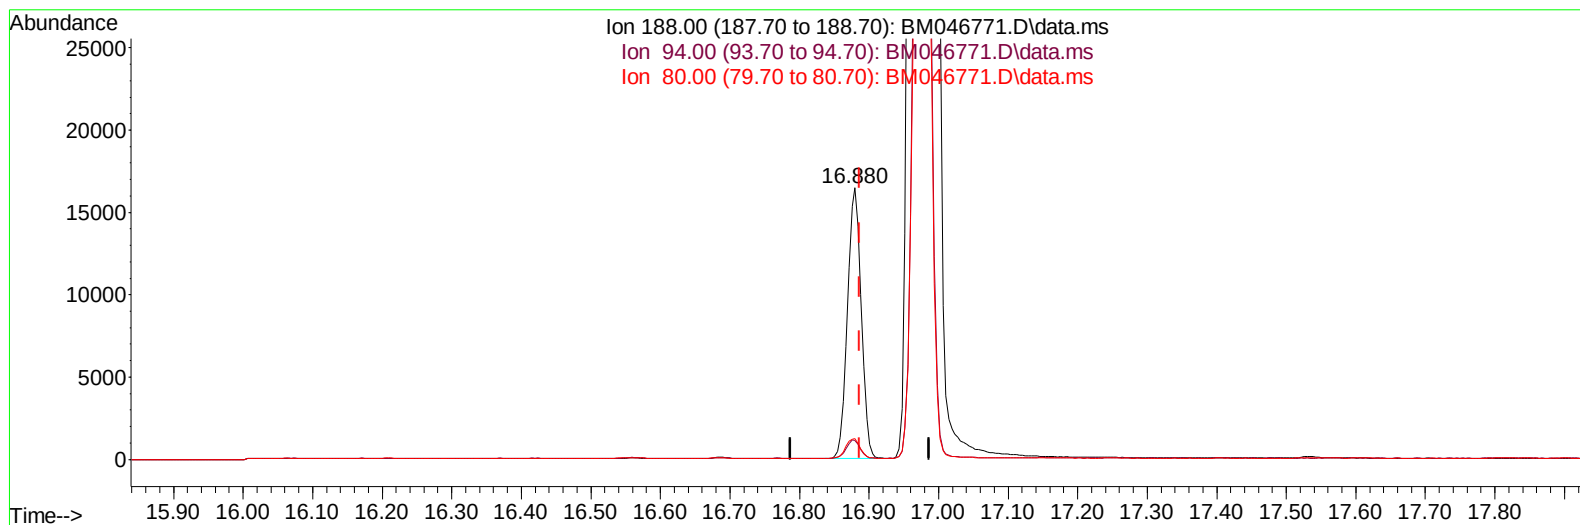

TIC: BM046771.D\data.ms

(13) Phenanthrene-d10 (I)

16.880min (-0.007) 0.40 ng/ul m

response 22519

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.40	6.91
80.00	6.60	7.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072324\
 Data File : BM046771.D
 Acq On : 23 Jul 2024 10:52
 Operator : MA/JU
 Sample : PB162090BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK090

Manual IntegrationsAPPROVED

Quant Time: Jul 23 11:36:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 19 11:38:04 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/24/2024
 Supervised By :mohammad ahmed 07/25/2024

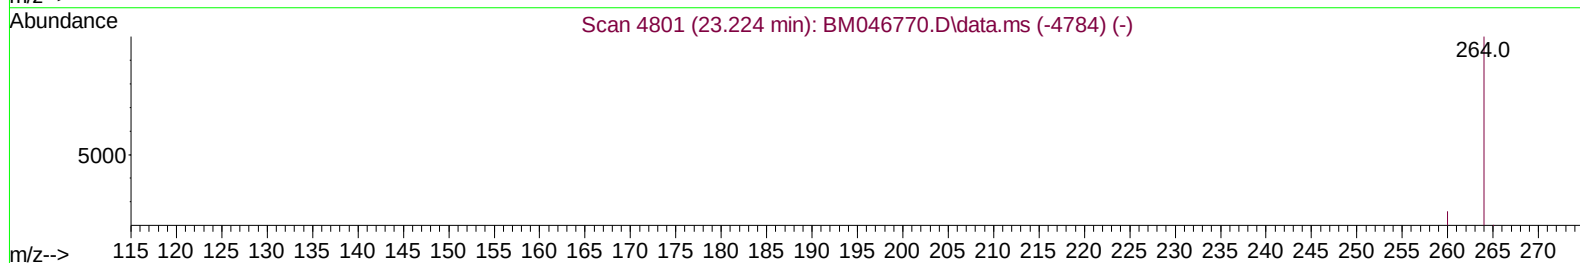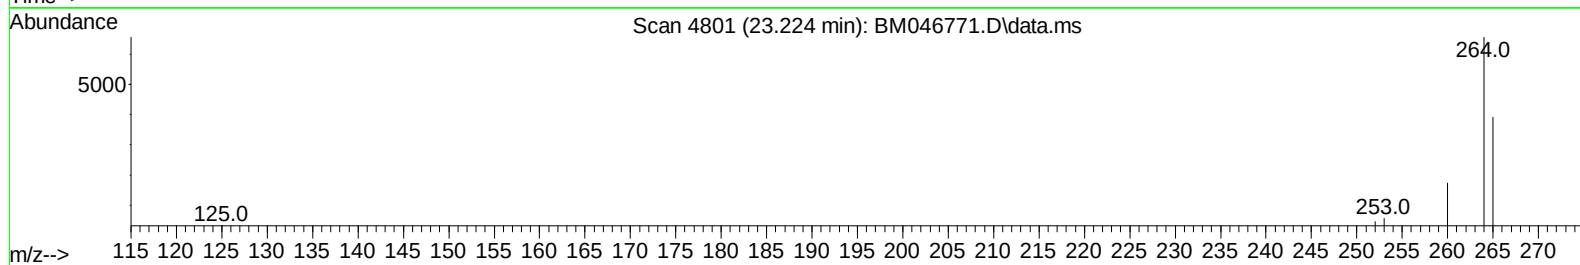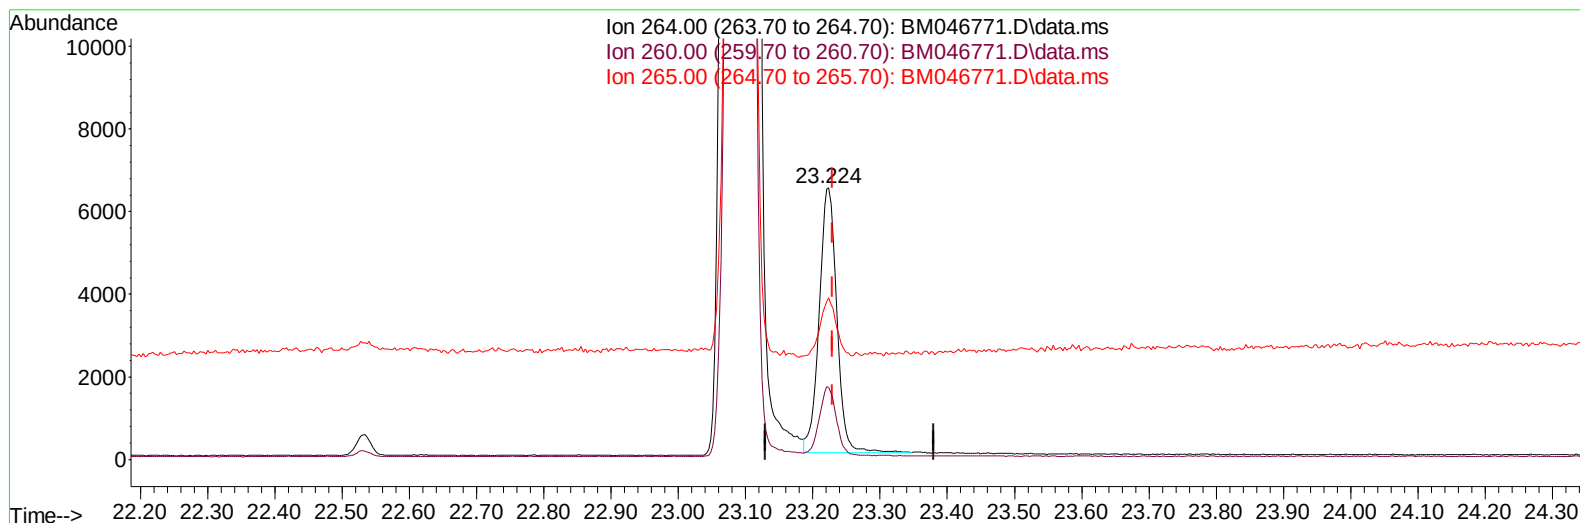

TIC: BM046771.D\data.ms

(23) Perylene-d12 (I)

23.224min (-0.006) 0.40 ng/u1

response 11650

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	26.43
265.00	88.90	59.59#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072324\
Data File : BM046771.D
Acq On : 23 Jul 2024 10:52
Operator : MA/JU
Sample : PB162090BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK090

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

Quant Time: Jul 23 11:36:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 19 11:38:04 2024
Response via : Initial Calibration

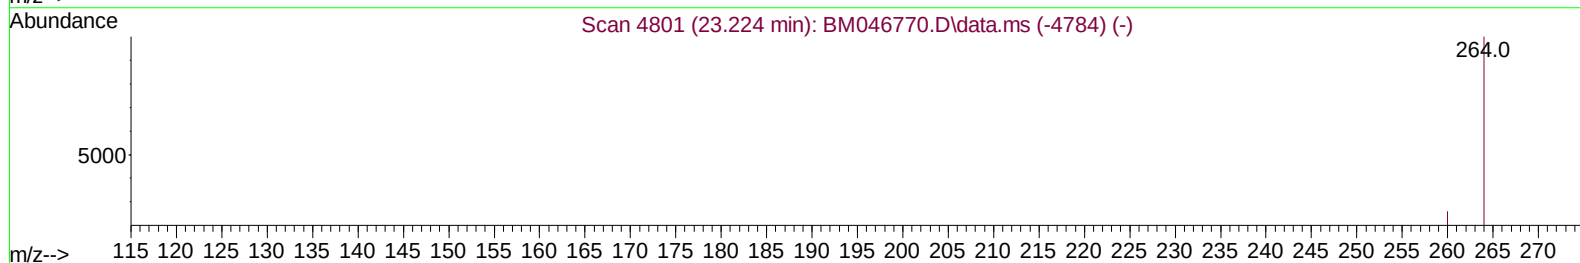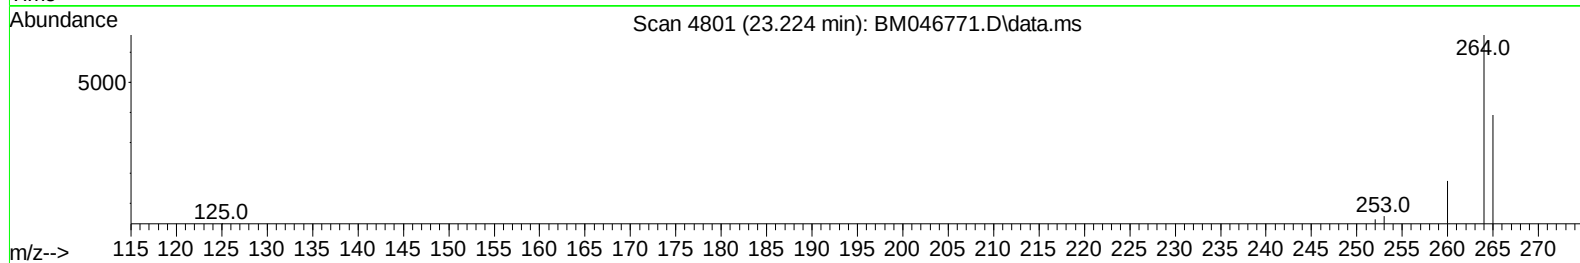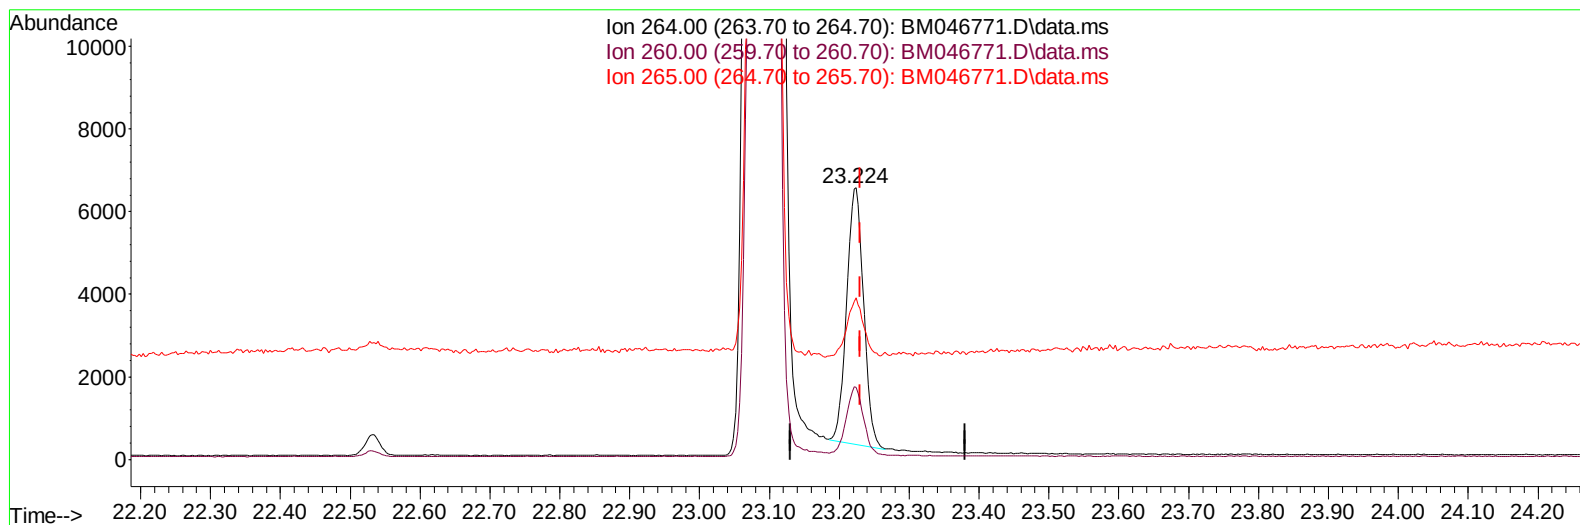

TIC: BM046771.D\data.ms

(23) Perylene-d12 (I)

23.224min (-0.006) 0.40 ng/ul m

response 10500

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	26.43
265.00	88.90	59.59#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072324\
 Data File : BM046771.D
 Acq On : 23 Jul 2024 10:52
 Operator : MA/JU
 Sample : PB162090BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK090

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
 Supervised By :mohammad ahmed 07/25/2024

Quant Time: Jul 23 11:36:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 19 11:38:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.477	152	2943	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.238	136	8436	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.123	164	9977	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.880	188	22519m	0.400	ng/ul	0.00
17) Chrysene-d12	21.091	240	11725	0.400	ng/ul	# 0.00
23) Perylene-d12	23.224	264	10500m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.105	96	12048	4.983	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.839	152	6724	0.494	ng/ul	0.00
18) Fluoranthene-d10	18.919	212	16130	0.452	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072324\
Data File : BM046771.D
Acq On : 23 Jul 2024 10:52
Operator : MA/JU
Sample : PB162090BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK090

Manual IntegrationsAPPROVED

Quant Time: Jul 23 11:36:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 19 11:38:04 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

