

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM072325\  
Data File : BM050491.D  
Acq On : 23 Jul 2025 15:33  
Operator : RC/JU  
Sample : PB168971BSD  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB168971BSD

Quant Time: Jul 24 06:57:48 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM070925.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 17 16:20:15 2025  
Response via : Initial Calibration

| Compound                    | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|-----------------------------|-------|------|----------|-------|-------|----------|
| Internal Standards          |       |      |          |       |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 0.000 | 152  | 0        | 0.000 | ng    | -7.85    |
| 21) Naphthalene-d8          | 0.000 | 136  | 0        | 0.000 | ng    | -10.64   |
| 39) Acenaphthene-d10        | 0.000 | 164  | 0        | 0.000 | ng    | -14.47   |
| 64) Phenanthrene-d10        | 0.000 | 188  | 0        | 0.000 | ng    | -17.21   |
| 76) Chrysene-d12            | 0.000 | 240  | 0        | 0.000 | ng    | -21.43   |
| 86) Perylene-d12            | 0.000 | 264  | 0        | 0.000 | ng    | -24.46   |
| System Monitoring Compounds |       |      |          |       |       |          |
| 5) 2-Fluorophenol           | 5.169 | 112  | 267      | 0.000 | ng    | -0.26    |
| 7) Phenol-d6                | 0.000 | 99   | 0        | 0.000 | ng    |          |
| 23) Nitrobenzene-d5         | 0.000 | 82   | 0        | 0.000 | ng    |          |
| 42) 2,4,6-Tribromophenol    | 0.000 | 330  | 0        | 0.000 | ng    |          |
| 45) 2-Fluorobiphenyl        | 0.000 | 172  | 0        | 0.000 | ng    |          |
| 79) Terphenyl-d14           | 0.000 | 244  | 0        | 0.000 | ng    |          |


| Target Compounds | Qvalue |
|------------------|--------|
|------------------|--------|

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM072325\  
Data File : BM050491.D  
Acq On : 23 Jul 2025 15:33  
Operator : RC/JU  
Sample : PB168971BSD  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB168971BSD

Quant Time: Jul 24 06:57:48 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM070925.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 17 16:20:15 2025  
Response via : Initial Calibration

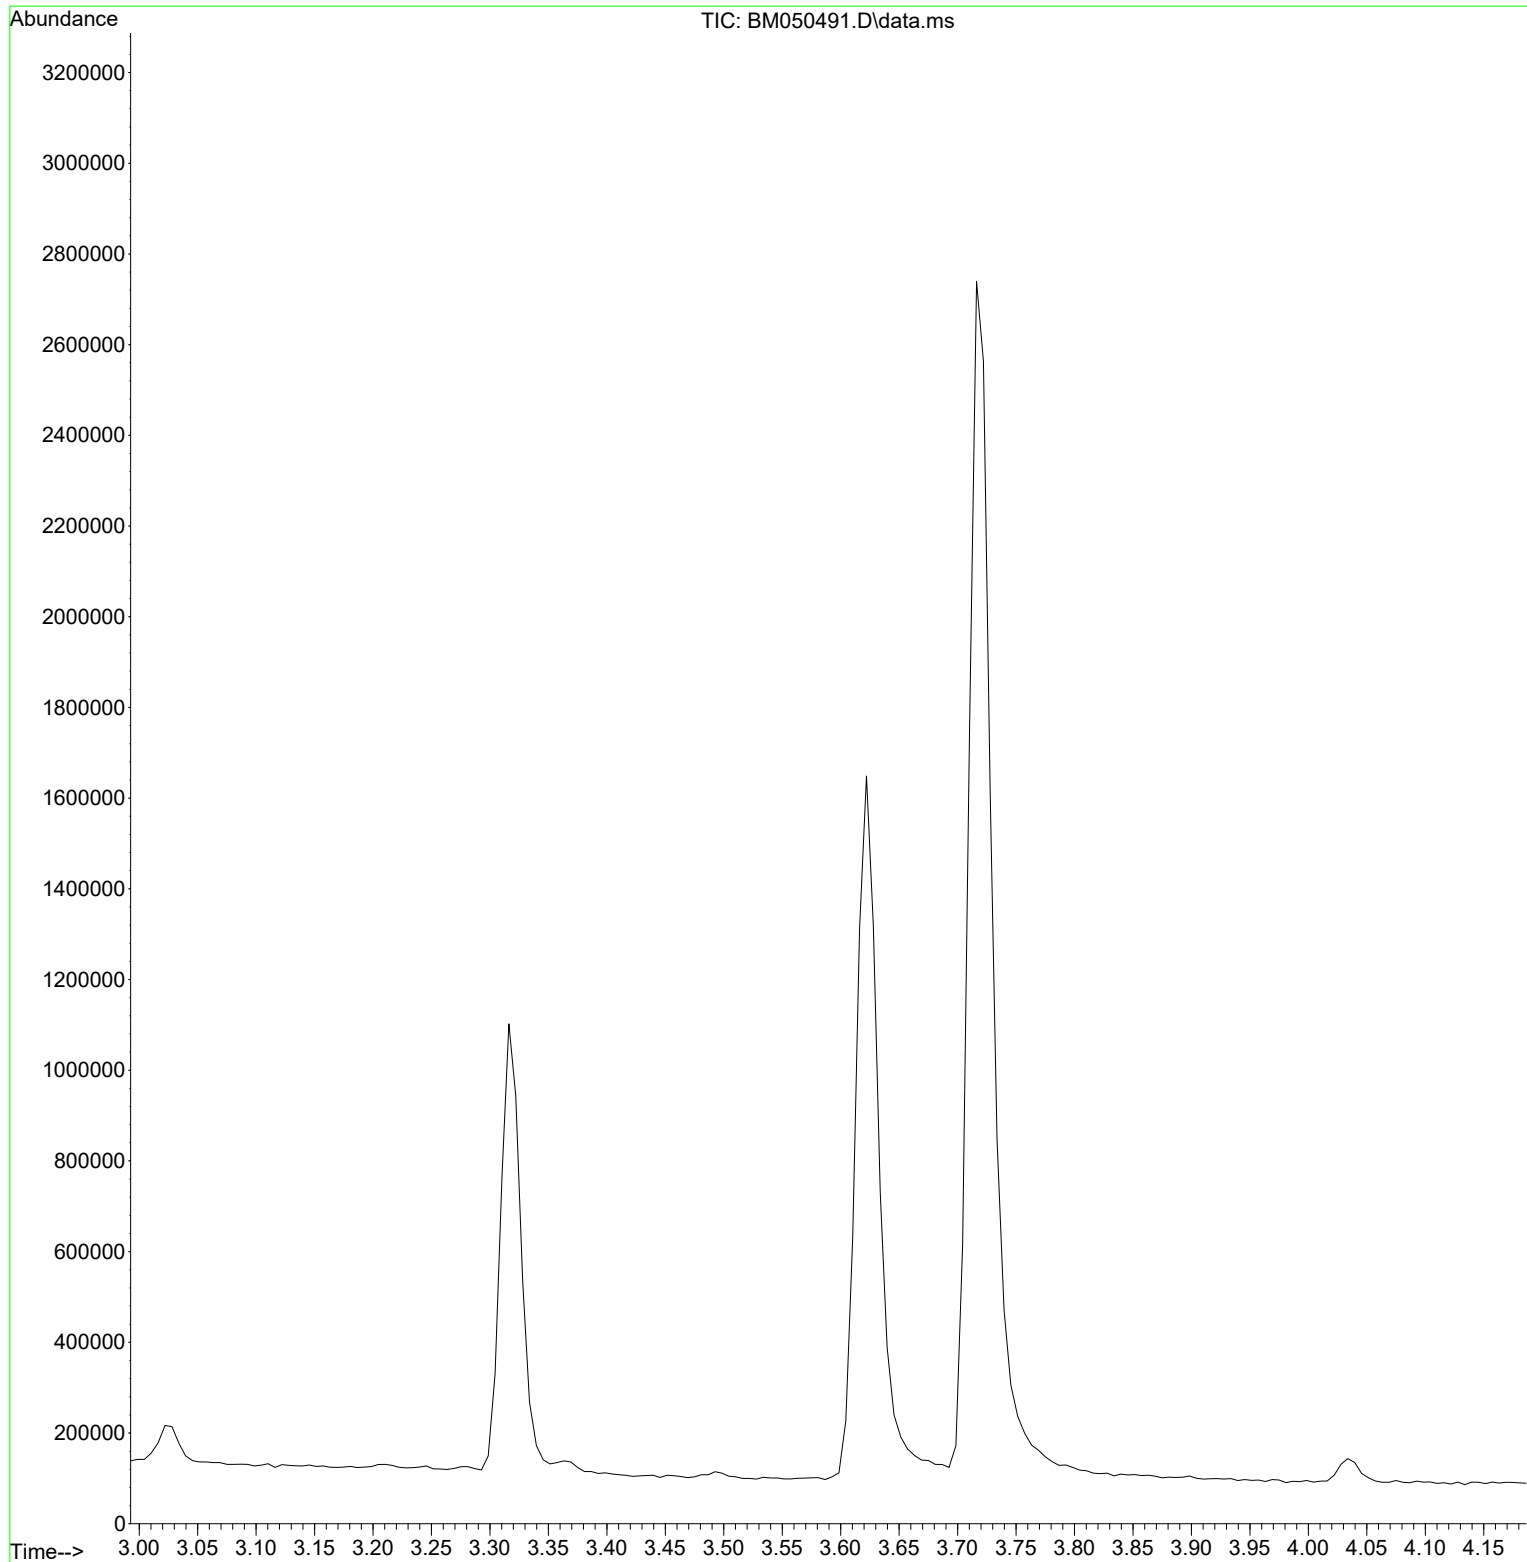

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM072325\  
Data File : BM050491.D  
Acq On : 23 Jul 2025 15:33  
Operator : RC/JU  
Sample : PB168971BSD  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB168971BSD

Quant Time: Jul 24 06:57:48 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM070925.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 17 16:20:15 2025  
Response via : Initial Calibration

