


Data Path : Z:\HPCHEM1\BNA M\DATA\BM072417\
 Data File : BM010958.D
 Acq On : 24 Jul 2017 11:29
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM071217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 12 14:21:16 2017

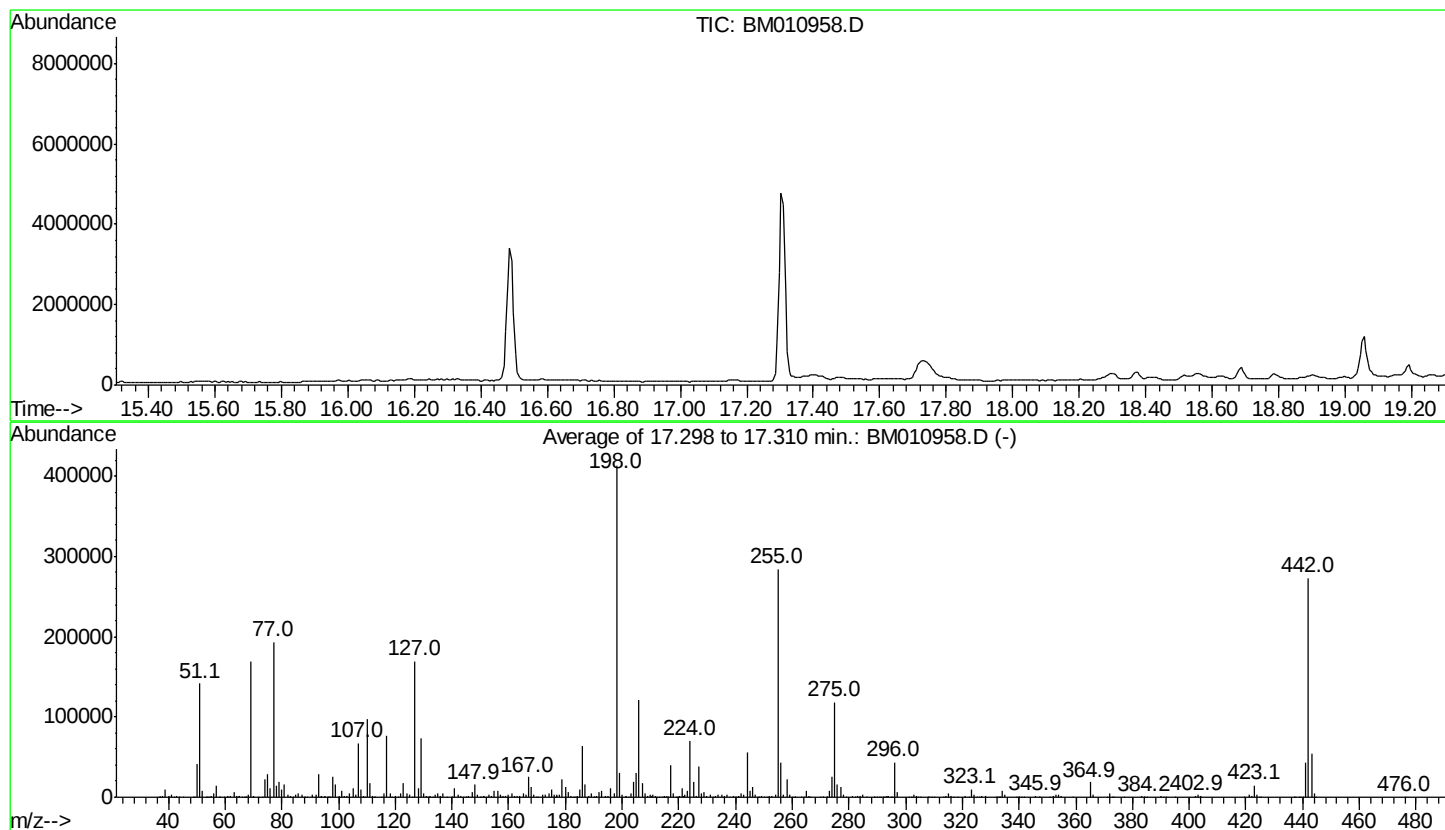

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	141653	PASS
68	69	0.00	2	1.7	2949	PASS
69	198	0.00	100	41.1	169646	PASS
70	69	0.00	2	0.6	1097	PASS
127	198	10	80	41.0	169573	PASS
197	198	0.00	2	1.0	4317	PASS
198	198	100	100	100.0	413138	PASS
199	198	5	9	7.2	29606	PASS
275	198	10	60	28.7	118498	PASS
365	198	1	100	4.5	18492	PASS
441	443	0.01	100	79.1	43525	PASS
442	198	50	100	66.2	273322	PASS
443	442	15	24	20.1	55042	PASS