
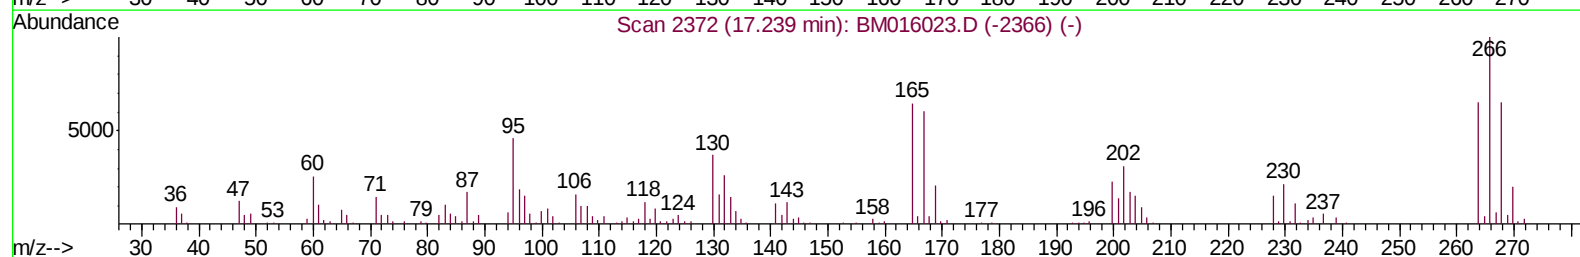
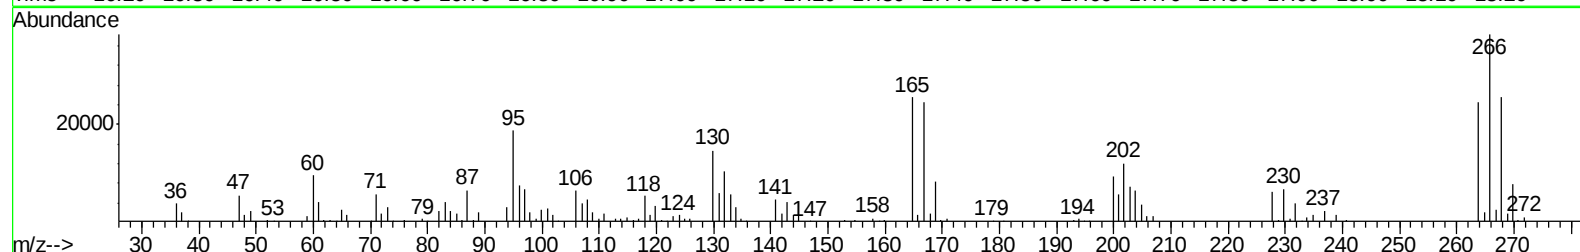


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072518\
Data File : BM016070.D
Acq On : 25 Jul 2018 08:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 07:36:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 23 16:08:38 2018
Response via : Initial Calibration

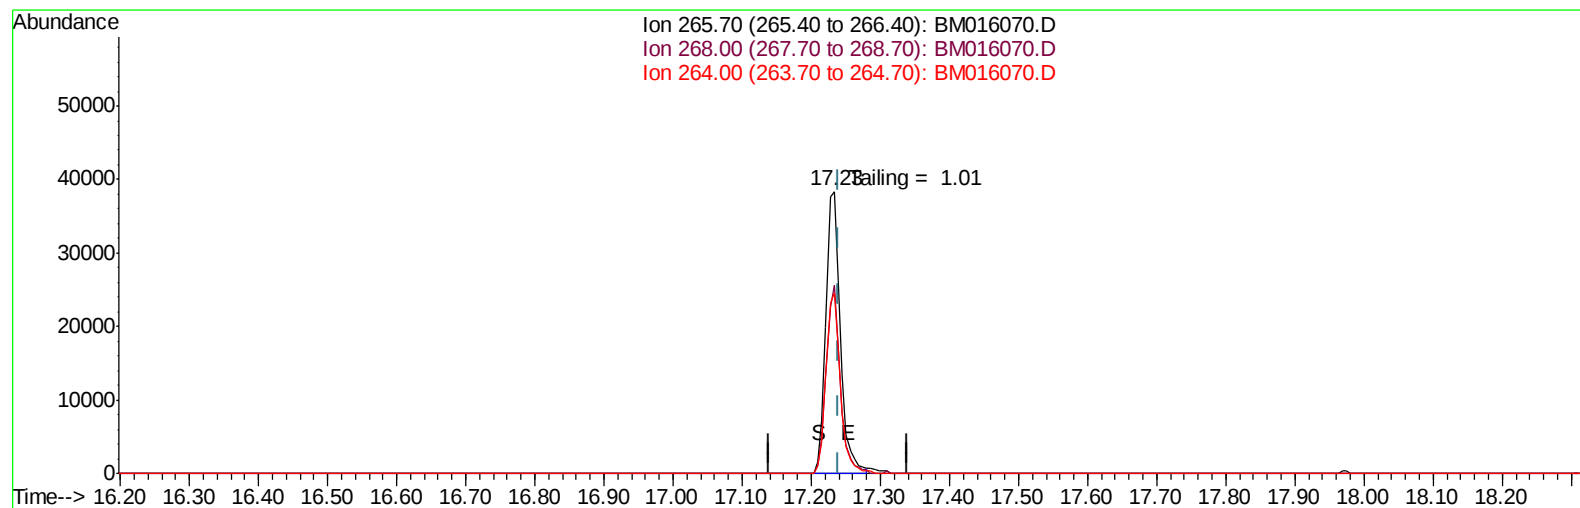

TIC: BM016070.D

(69) Pentachlorophenol (C)




17.233min (-0.006) 0.00ng

response 56245

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	66.69
264.00	61.20	64.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072518\
Data File : BM016070.D
Acq On : 25 Jul 2018 08:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 07:36:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 23 16:08:38 2018
Response via : Initial Calibration

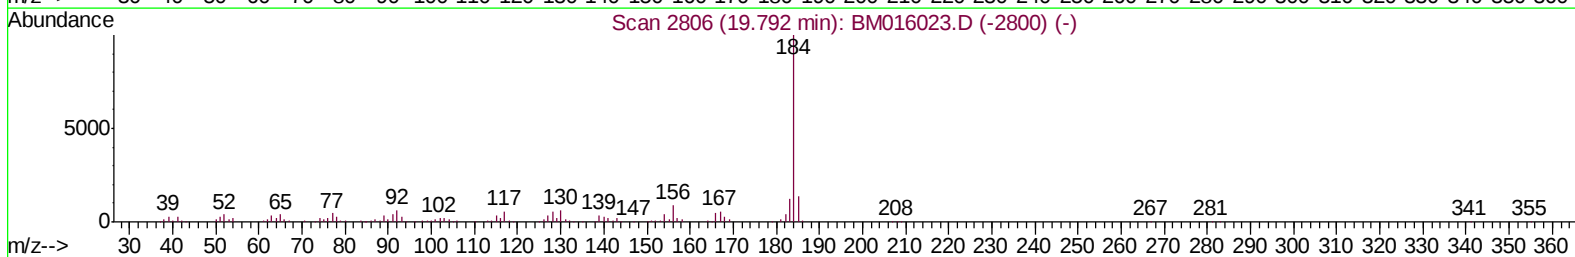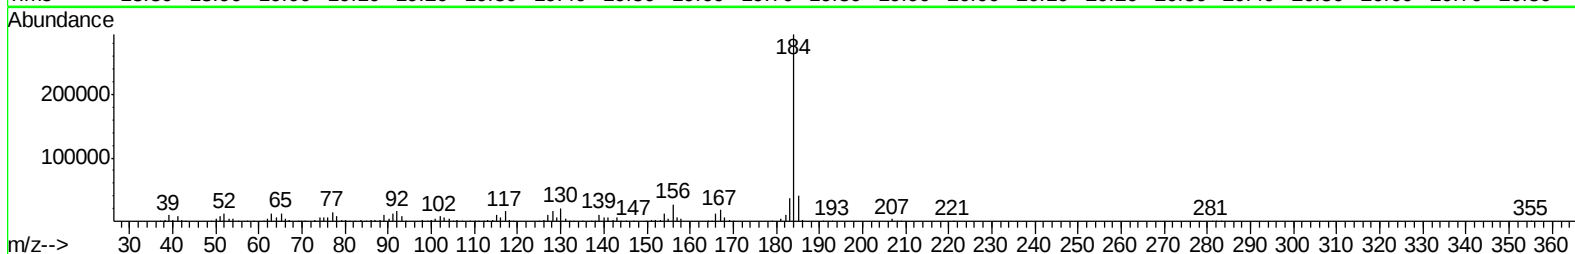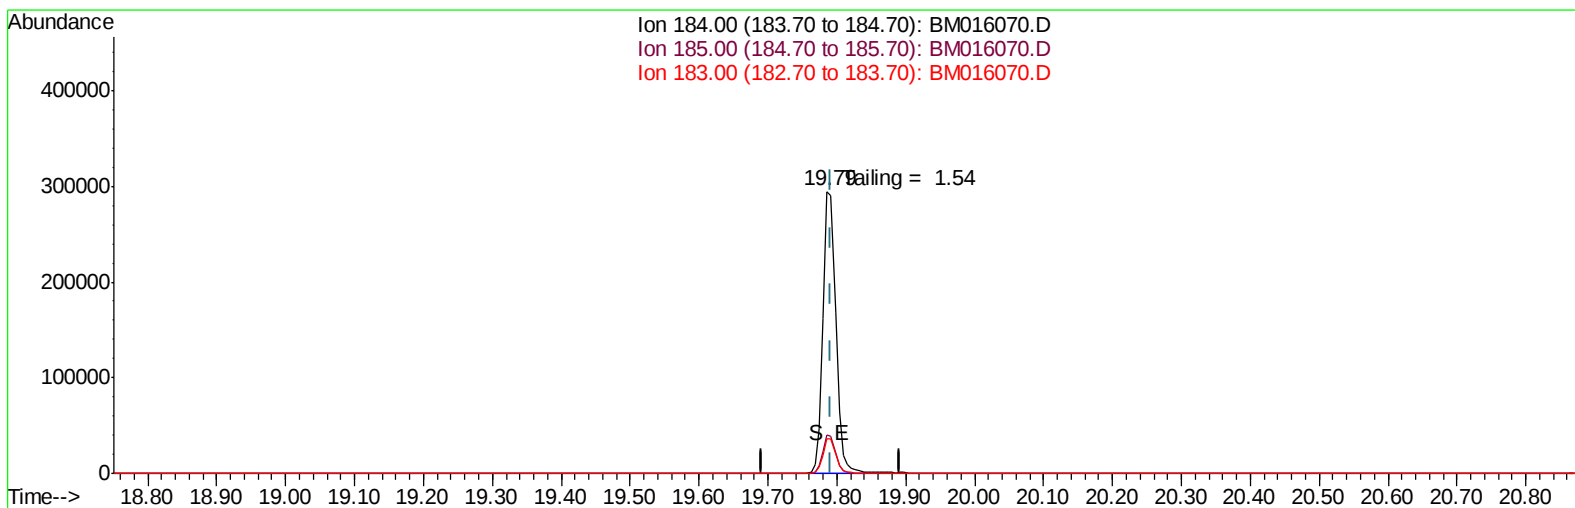

TIC: BM016070.D

(76) Benzidine

19.786min (-0.006) 11088.23ng

response 383598

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.72
183.00	11.10	12.34
0.00	0.00	0.00