


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072518\
Data File : BM016070.D
Acq On : 25 Jul 2018 08:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 23 16:08:38 2018

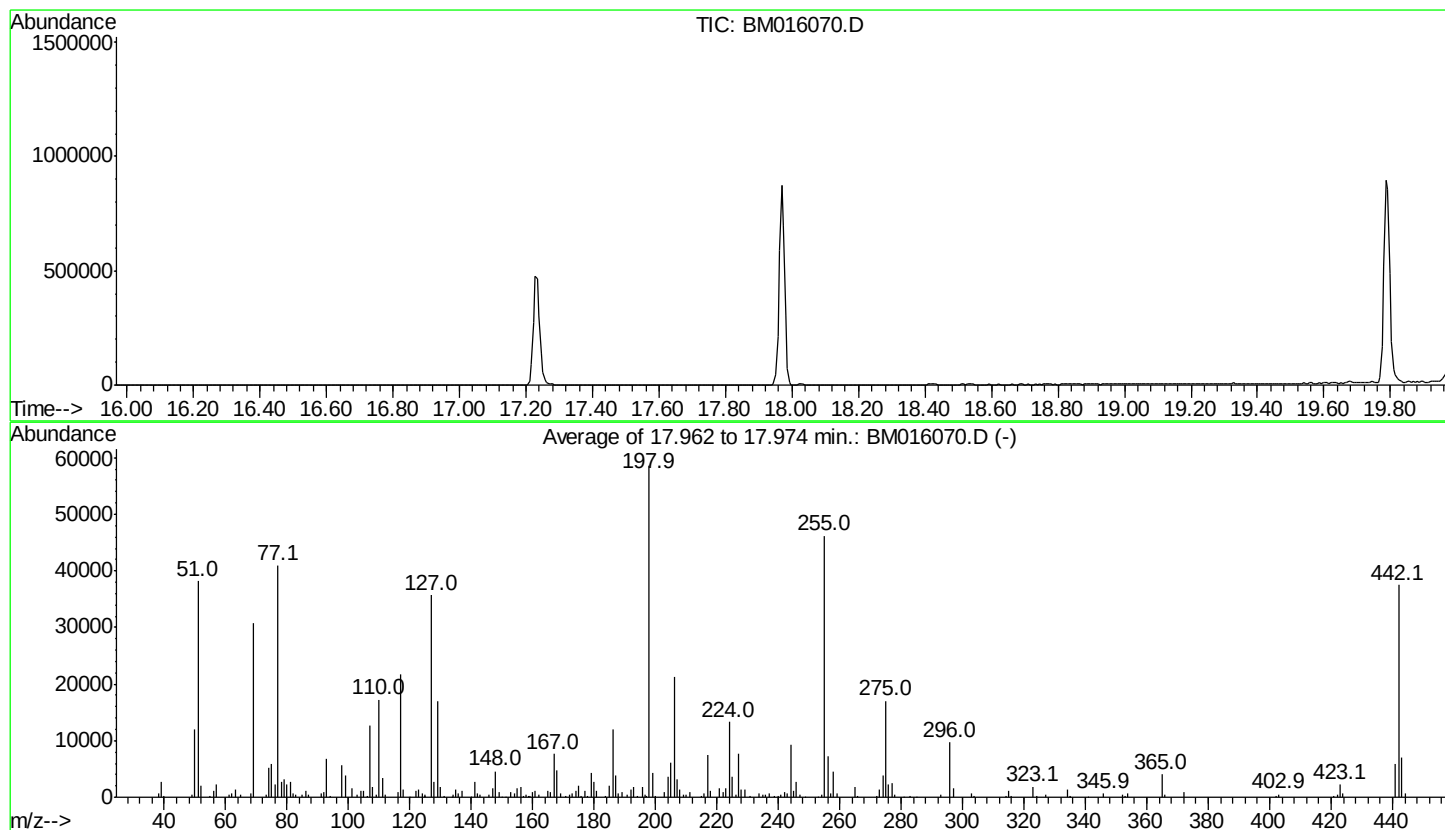

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.2	38224	PASS
68	69	0.00	2	2.0	606	PASS
69	198	0.00	100	52.4	30685	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	61.0	35720	PASS
197	198	0.00	2	0.7	426	PASS
198	198	100	100	100.0	58597	PASS
199	198	5	9	7.2	4208	PASS
275	198	10	60	29.1	17039	PASS
365	198	1	100	6.9	4038	PASS
441	198	0.01	100	10.2	5989	PASS
442	198	50	100	64.0	37493	PASS
443	442	15	24	18.6	6957	PASS