




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072524\
Data File : BM046792.D
Acq On : 25 Jul 2024 09:51
Operator : MA/JU
Sample : PB162099BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK099

Manual IntegrationsAPPROVED

Quant Time: Jul 25 10:58:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

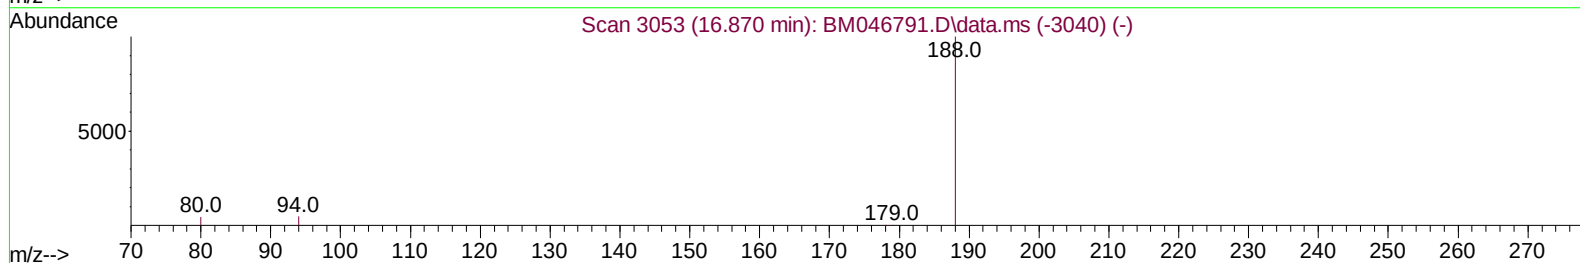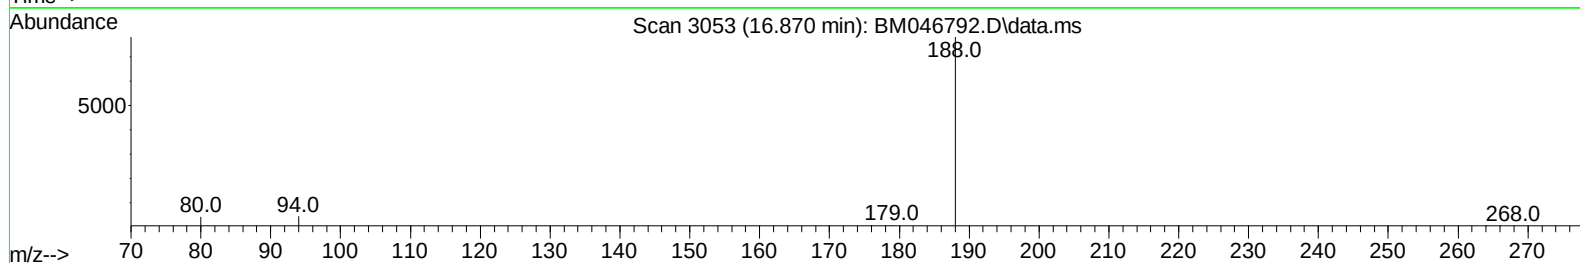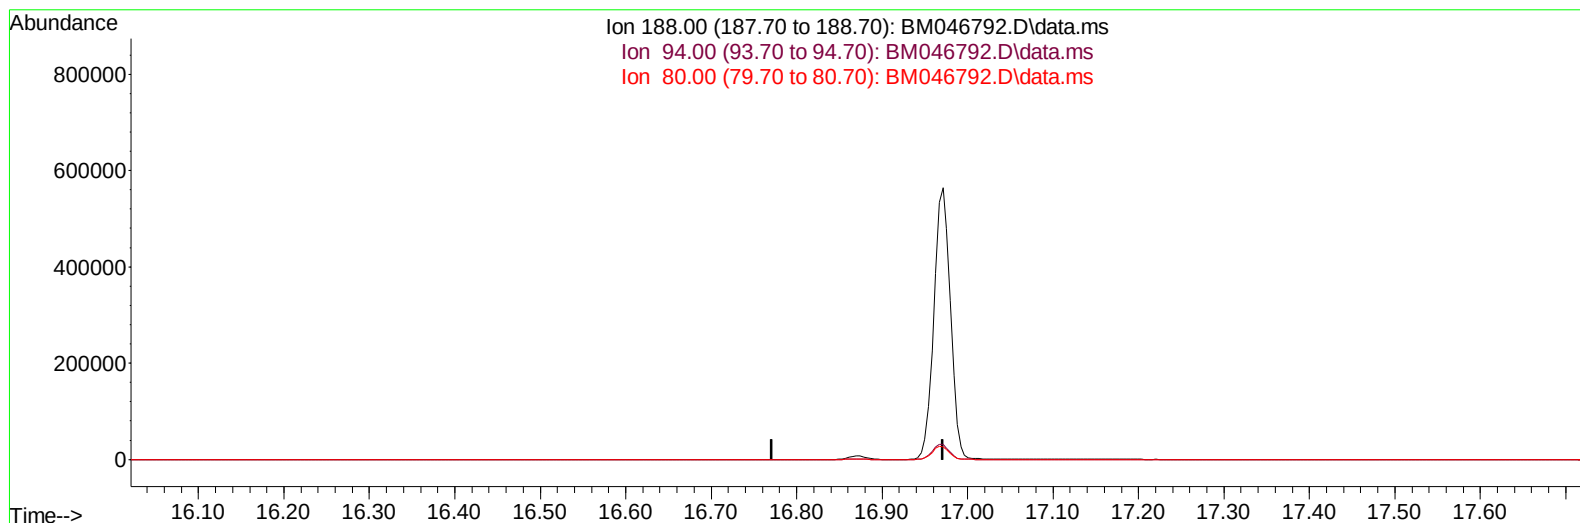

TIC: BM046792.D\data.ms

(13) Phenanthrene-d10 (I)

16.871min (-16.871) 0.00 ng/ul

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.60	0.00#
80.00	6.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072524\
Data File : BM046792.D
Acq On : 25 Jul 2024 09:51
Operator : MA/JU
Sample : PB162099BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK099

Manual IntegrationsAPPROVED

Quant Time: Jul 25 10:58:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

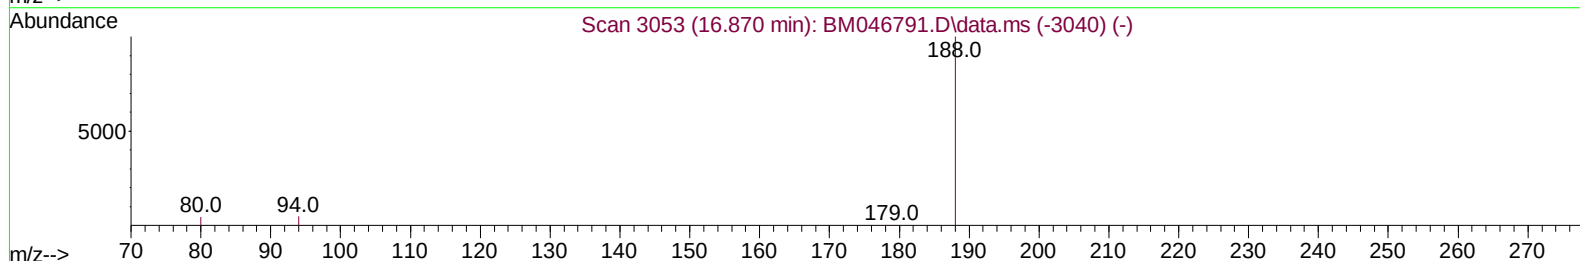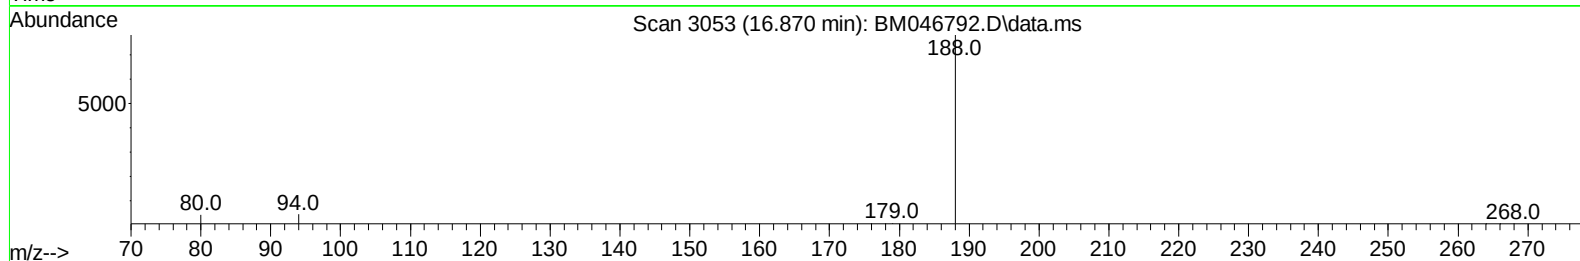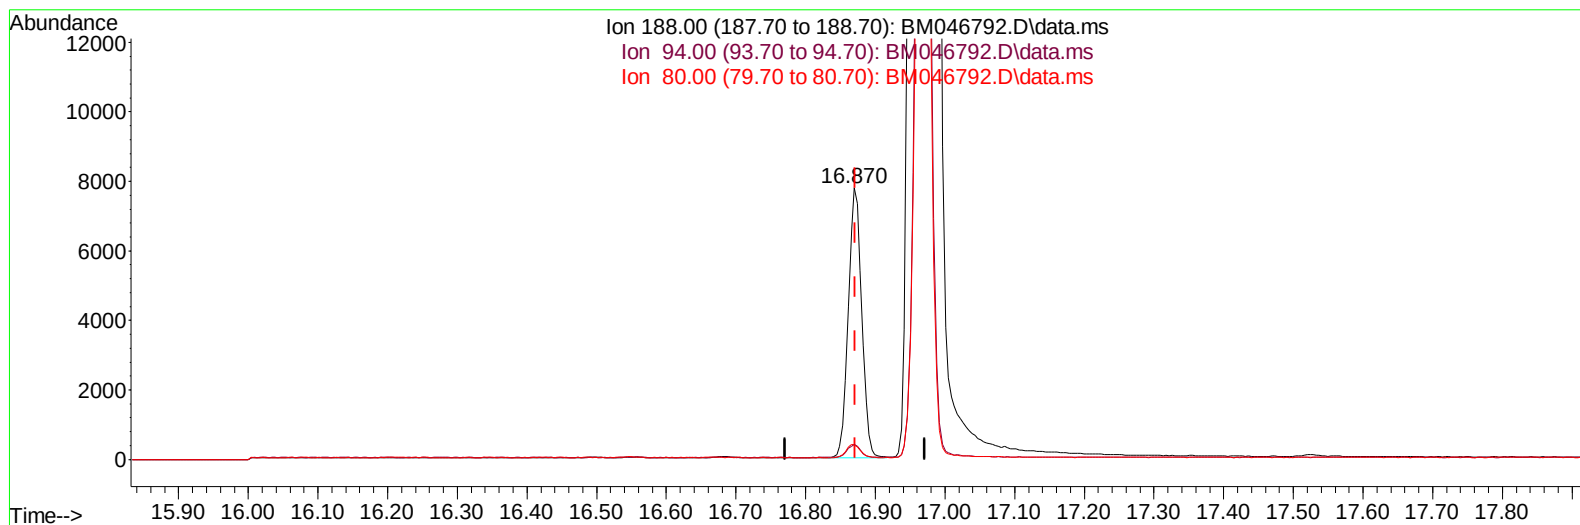

TIC: BM046792.D\data.ms

(13) Phenanthrene-d10 (I)

16.870min (-0.001) 0.40 ng/ul m

response 10392

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.60	5.56
80.00	6.30	5.43
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072524\
 Data File : BM046792.D
 Acq On : 25 Jul 2024 09:51
 Operator : MA/JU
 Sample : PB162099BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK099

Manual IntegrationsAPPROVED

Quant Time: Jul 25 10:58:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 24 15:10:37 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

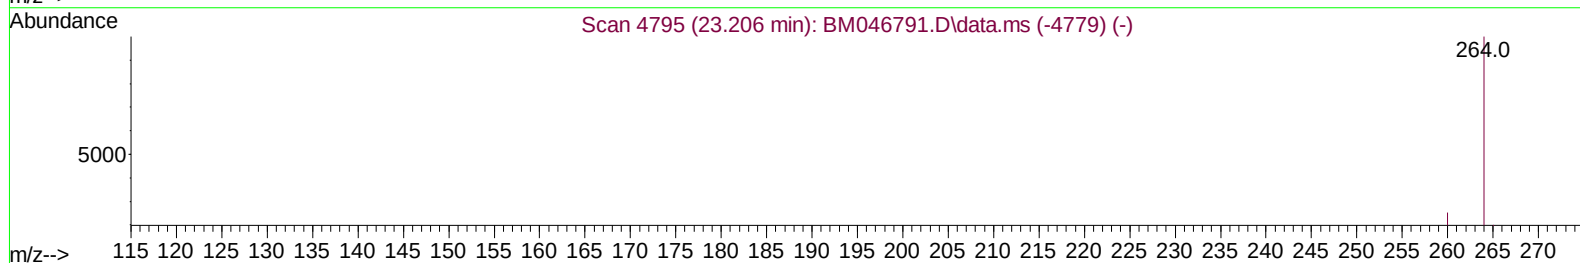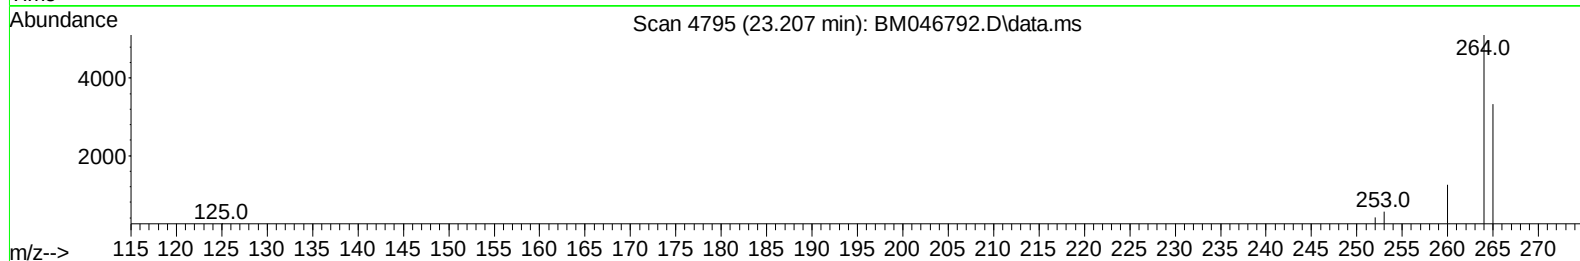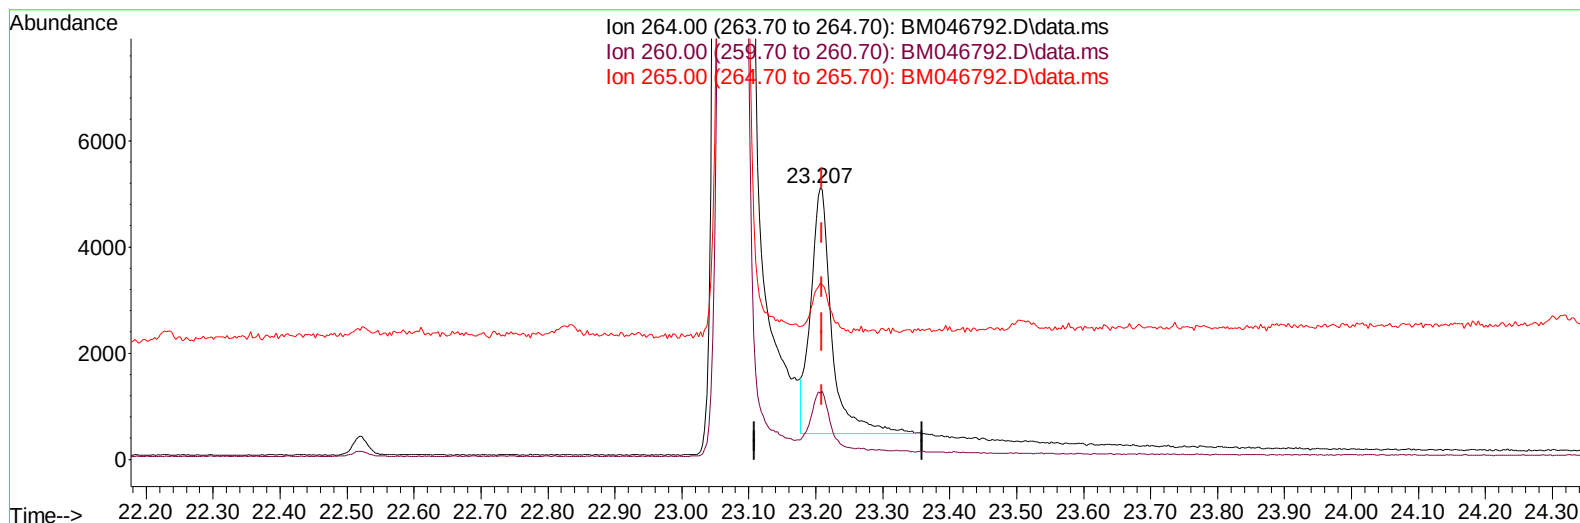

TIC: BM046792.D\data.ms

(23) Perylene-d12 (I)

23.207min (-0.002) 0.40 ng/u1

response 10136

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	24.44
265.00	89.90	65.02#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072524\
Data File : BM046792.D
Acq On : 25 Jul 2024 09:51
Operator : MA/JU
Sample : PB162099BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK099

Manual IntegrationsAPPROVED

Quant Time: Jul 25 10:58:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

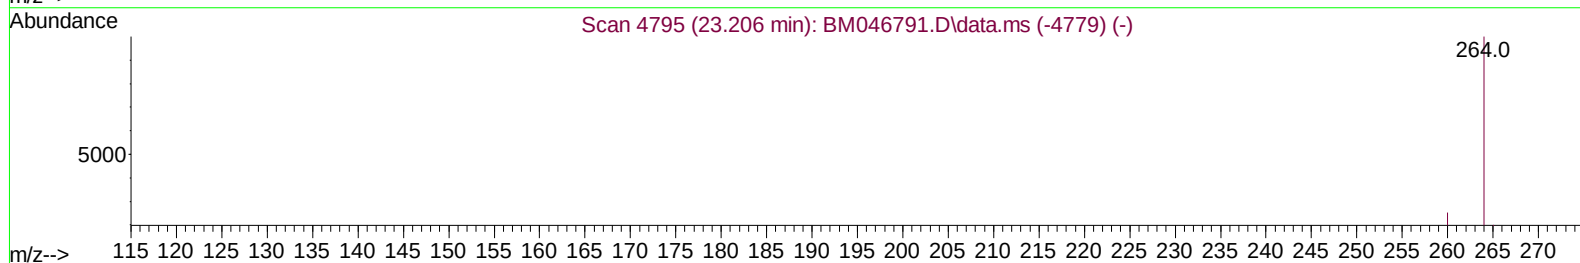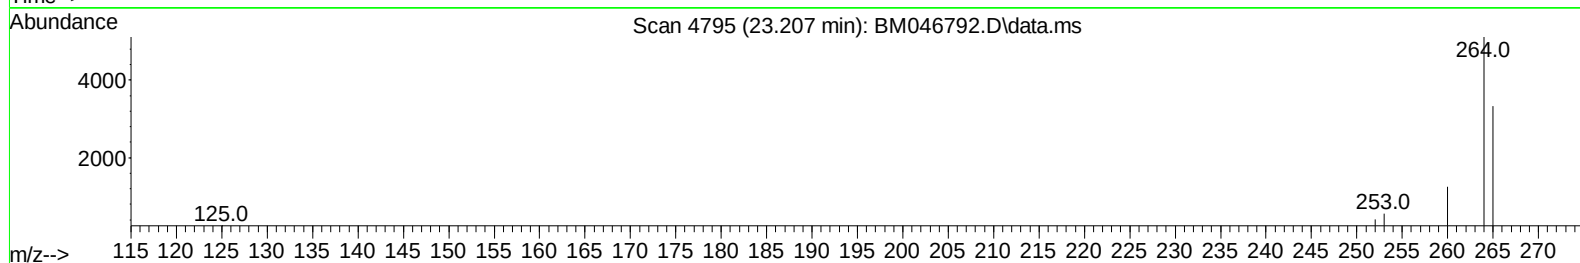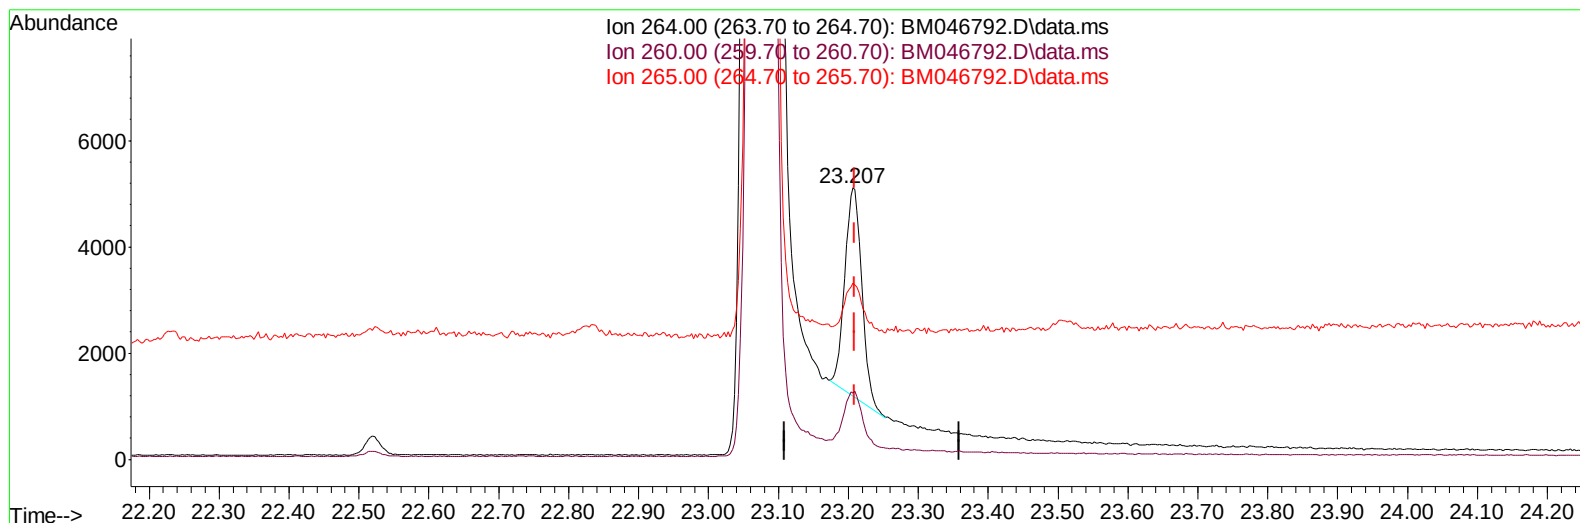

TIC: BM046792.D\data.ms

(23) Perylene-d12 (I)

23.207min (-0.002) 0.40 ng/ul m

response 6584

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	24.44
265.00	89.90	65.02#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072524\
 Data File : BM046792.D
 Acq On : 25 Jul 2024 09:51
 Operator : MA/JU
 Sample : PB162099BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK099

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

Quant Time: Jul 25 10:58:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 24 15:10:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.472	152	2401	0.400	ng/ul	0.00
4) Naphthalene-d8	10.231	136	6487	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.117	164	4452	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.870	188	10392m	0.400	ng/ul	0.00
17) Chrysene-d12	21.082	240	7696	0.400	ng/ul	0.00
23) Perylene-d12	23.207	264	6584m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.101	96	10421	6.199	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.832	152	3246	0.315	ng/ul	0.00
18) Fluoranthene-d10	18.913	212	8032	0.320	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072524\
Data File : BM046792.D
Acq On : 25 Jul 2024 09:51
Operator : MA/JU
Sample : PB162099BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK099

Manual IntegrationsAPPROVED

Quant Time: Jul 25 10:58:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

