

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072524\
 Data File : BM046801.D
 Acq On : 25 Jul 2024 15:56
 Operator : MA/JU
 Sample : P3264-21
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4D63

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

Quant Time: Jul 25 16:33:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 24 15:10:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.472	152	3724	0.400	ng/ul	0.00
4) Naphthalene-d8	10.231	136	10839	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.117	164	7478	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.874	188	15870m	0.400	ng/ul	0.00
17) Chrysene-d12	21.079	240	8723	0.400	ng/ul	# 0.00
23) Perylene-d12	23.209	264	7280m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.101	96	6869	2.634	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.832	152	6077	0.353	ng/ul	0.00
18) Fluoranthene-d10	18.913	212	13591	0.478	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.281	128	775	0.028	ng/ul#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072524\
Data File : BM046801.D
Acq On : 25 Jul 2024 15:56
Operator : MA/JU
Sample : P3264-21
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A4D63

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024


Quant Time: Jul 25 16:33:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

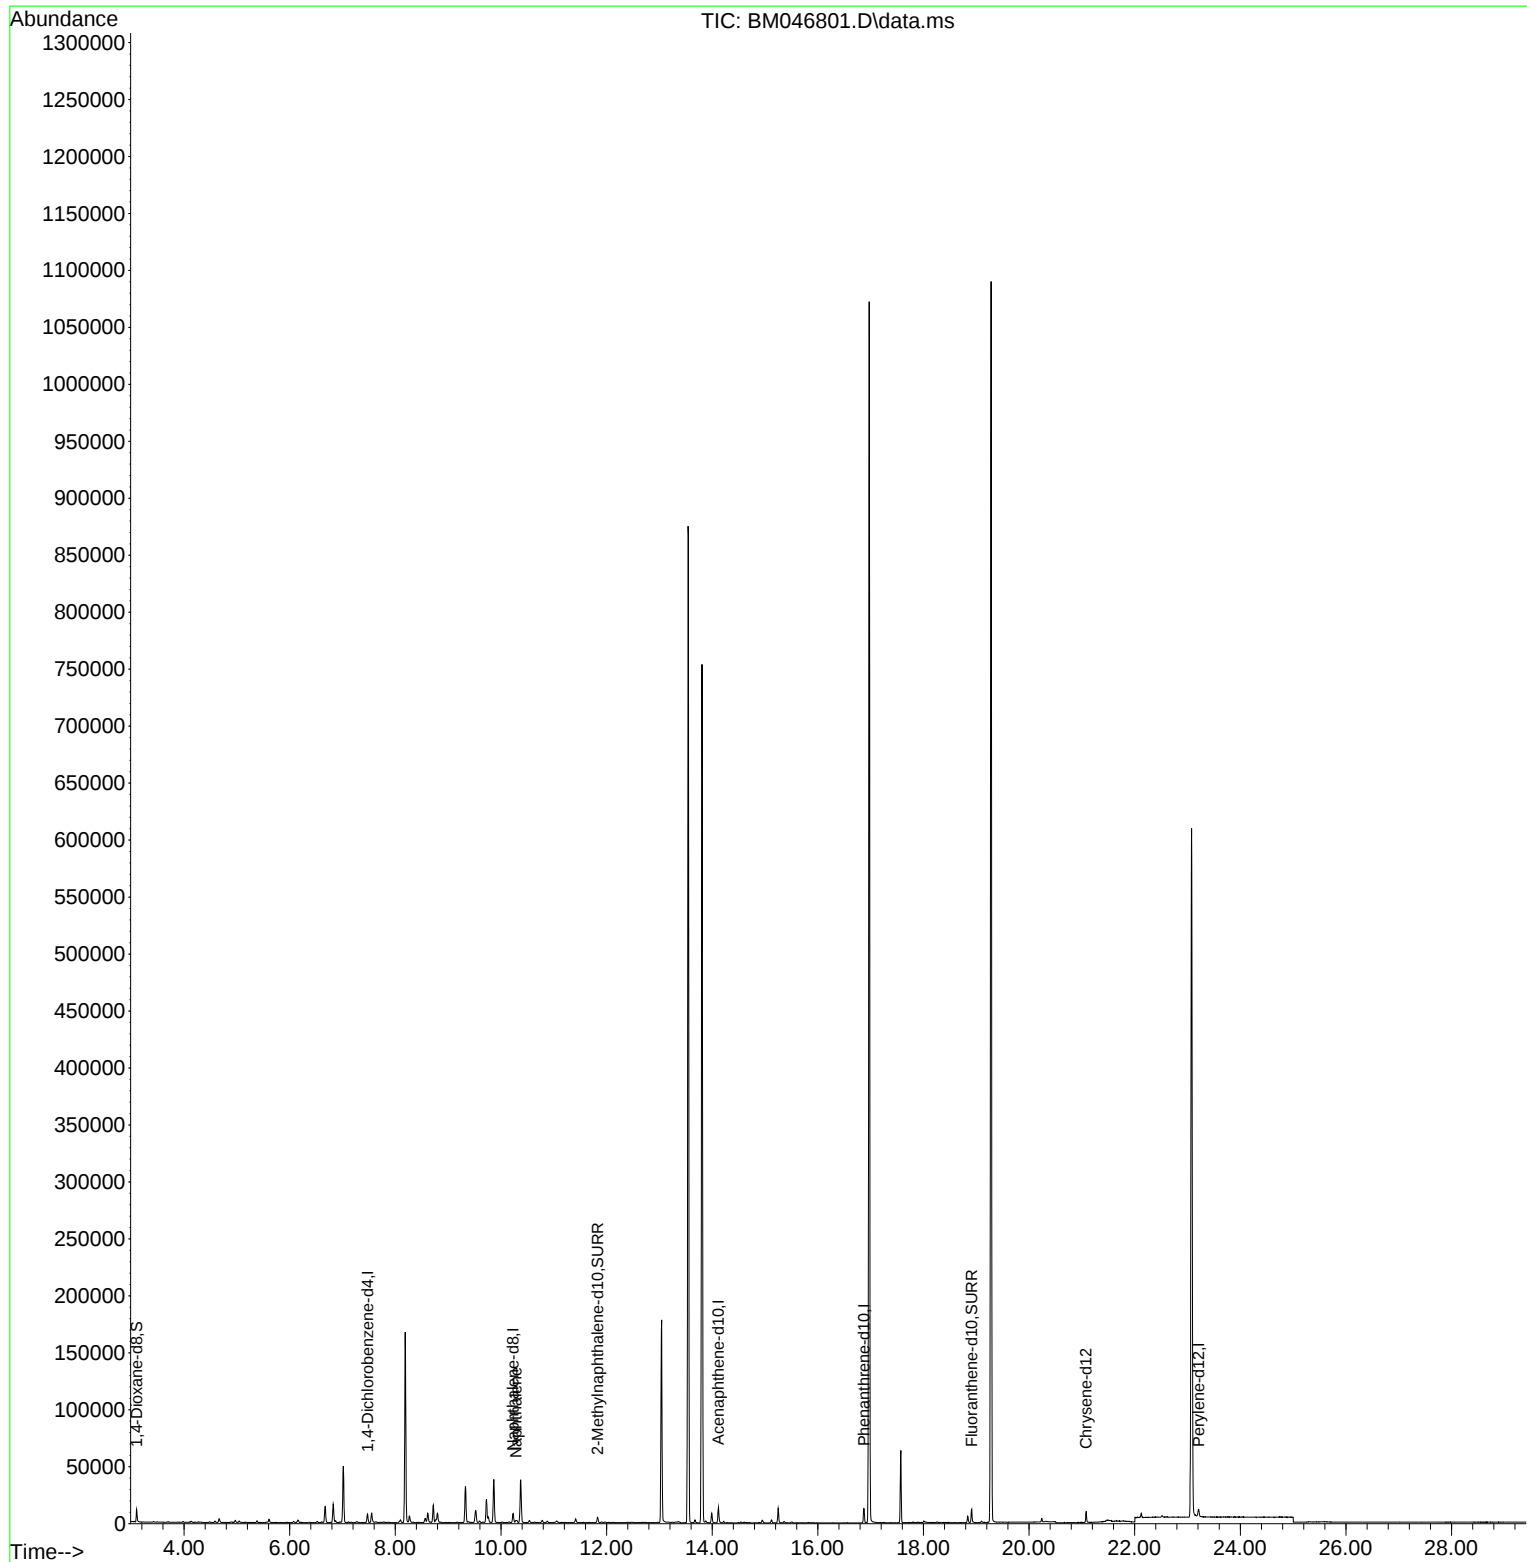

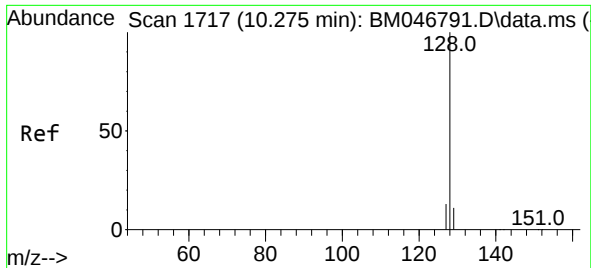

#5
Naphthalene
Concen: 0.028 ng/ul
RT: 10.281 min Scan# 1718
Delta R.T. 0.004 min
Lab File: BM046801.D
Acq: 25 Jul 2024 15:56

Instrument :
BNA_M
ClientSampleId :
A4D63

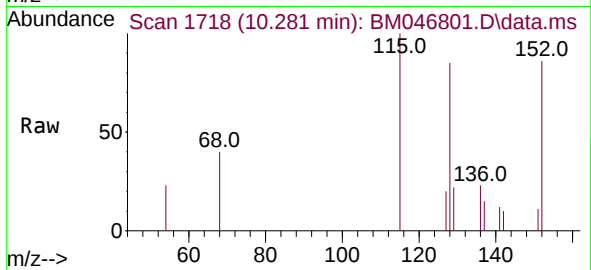

Tgt Ion:128 Resp: 779
Ion Ratio Lower Upper
128 100
129 25.7 10.1 15.1
127 23.7 11.5 17.3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

