

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006677.D
 Acq On : 27 Jul 2016 07:47
 Operator : UM/SJ
 Sample : H4094-04
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJD7

Quant Time: Jul 27 08:38:04 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 15:24:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	176216	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	771475	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	439957	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	1023549	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1233109	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	1316975	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	9023	1.99	ng/uL	0.00
5) Phenol-d5	6.79	99	348425	22.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	222778	23.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	269465	22.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	276299	22.74	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	130537	21.92	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	143332	22.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	256042	21.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	374807	31.27	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	860237	24.50	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1047812	23.74	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	130134	21.54	ng/ul	0.00
57) Fluorene-d10	15.26	176	742623	24.39	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	102402	18.36	ng/ul	0.00
70) Anthracene-d10	17.11	188	1181116	24.73	ng/ul	0.00
76) Pyrene-d10	19.42	212	1385337	24.22	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1513553	25.40	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.72	163	885614	25.22	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006677.D
Acq On : 27 Jul 2016 07:47
Operator : UM/SJ
Sample : H4094-04
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJD7

Quant Time: Jul 27 08:38:04 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 15:24:14 2016
Response via : Initial Calibration

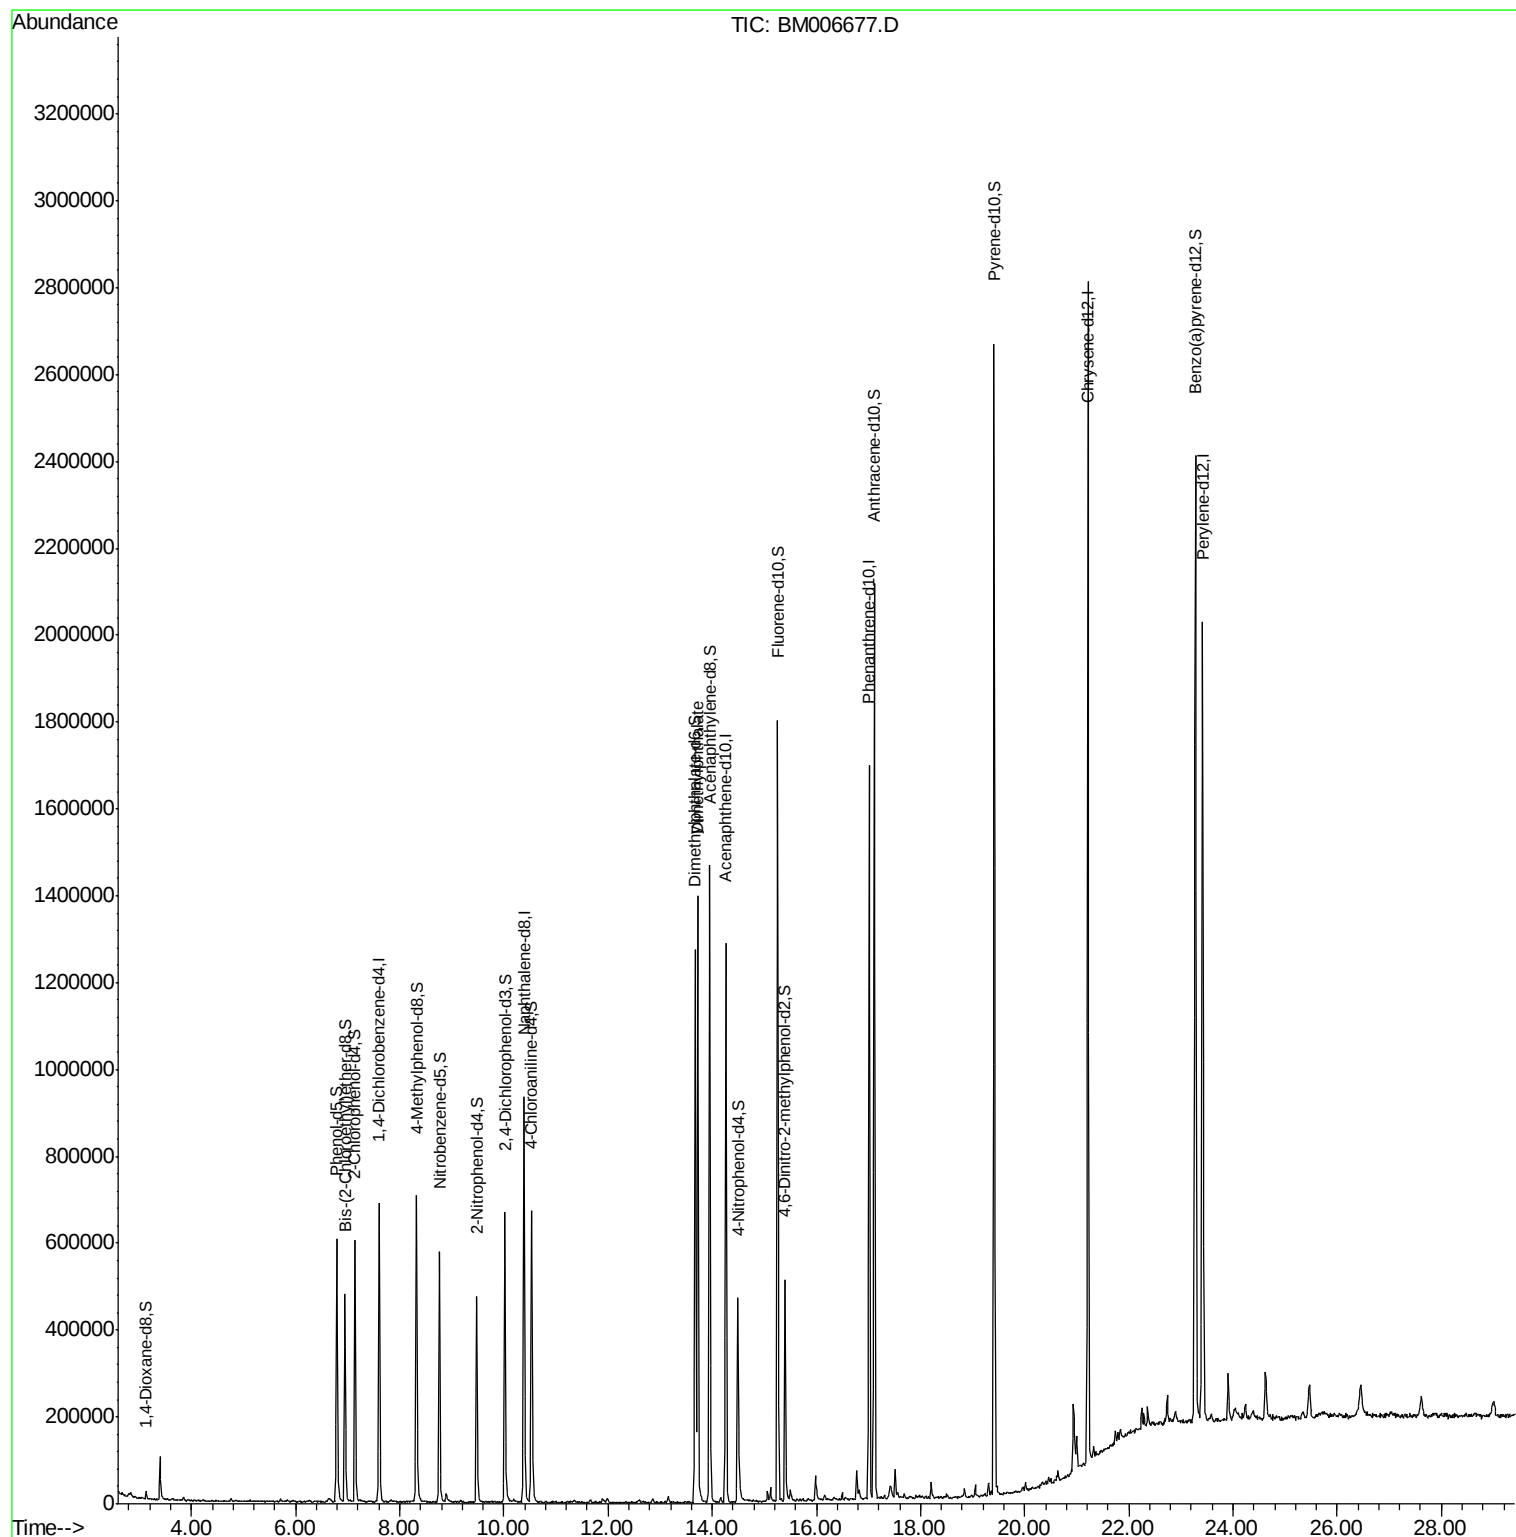

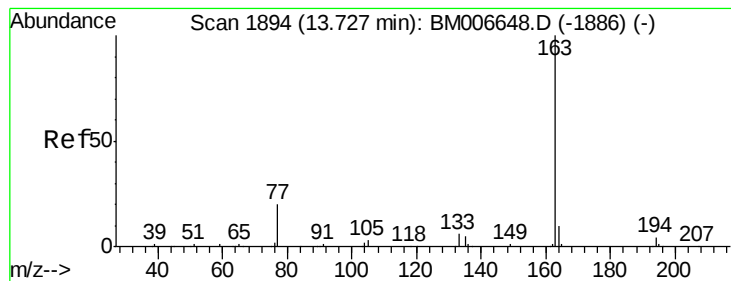

#44

Dimethylphthalate

Concen: 25.22 ng/ul

RT: 13.72 min Scan# 1893

Delta R.T. -0.01 min

Lab File: BM006677.D

Acq: 27 Jul 2016 07:47

Instrument :

BNA_M

ClientSampleId :

BDJD7

Tgt Ion:163 Resp: 885614

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 10.2 7.8 11.8

