

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006673.D
 Acq On : 27 Jul 2016 05:24
 Operator : UM/SJ
 Sample : H4062-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJC0

Manual Integration

Quant Time: Jul 27 06:44:08 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 15:24:14 2016
 Response via : Initial Calibration

sohil
 7/27/2016 7:10:08 PM

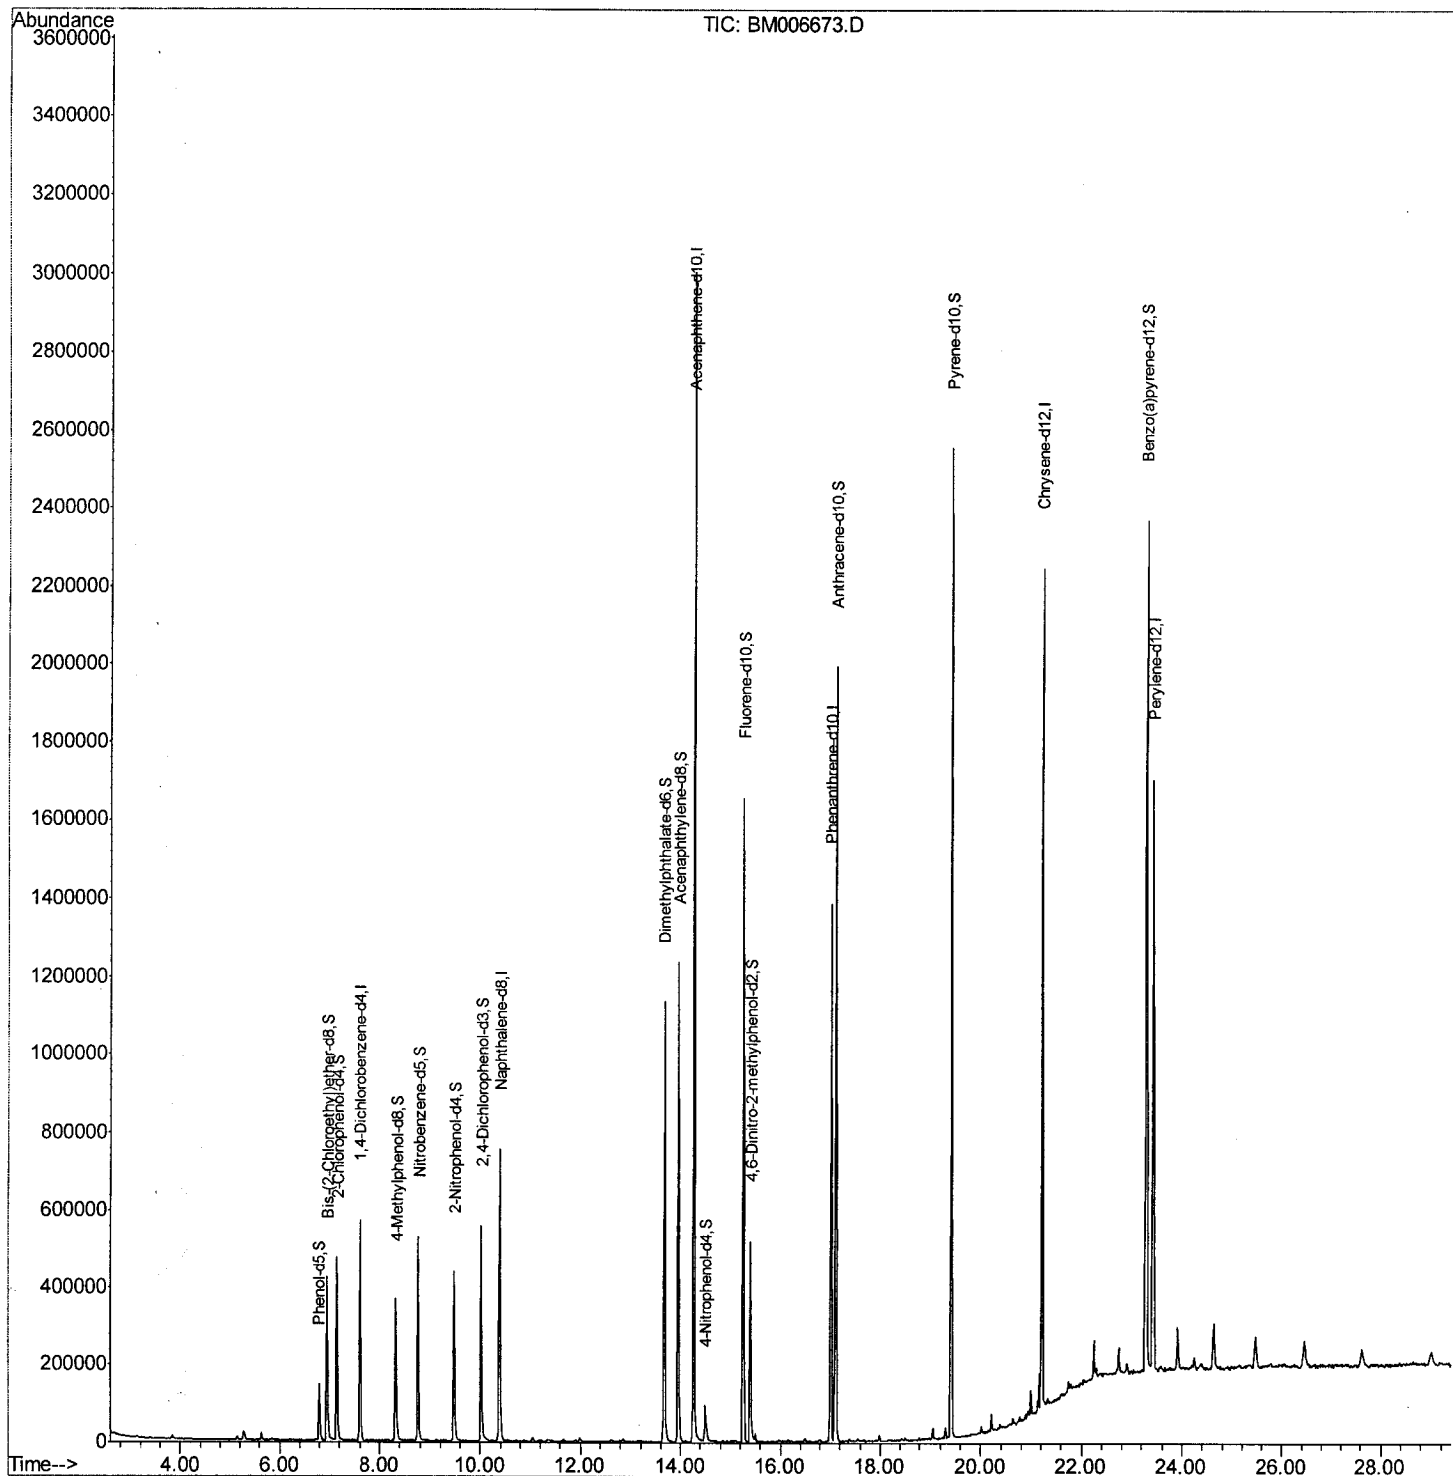

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006673.D
 Acq On : 27 Jul 2016 05:24
 Operator : UM/SJ
 Sample : H4062-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJC0

Manual Integration

sohil
 7/27/2016 7:10:08 PM

Quant Time: Jul 27 06:10:05 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 15:24:14 2016
 Response via : Initial Calibration

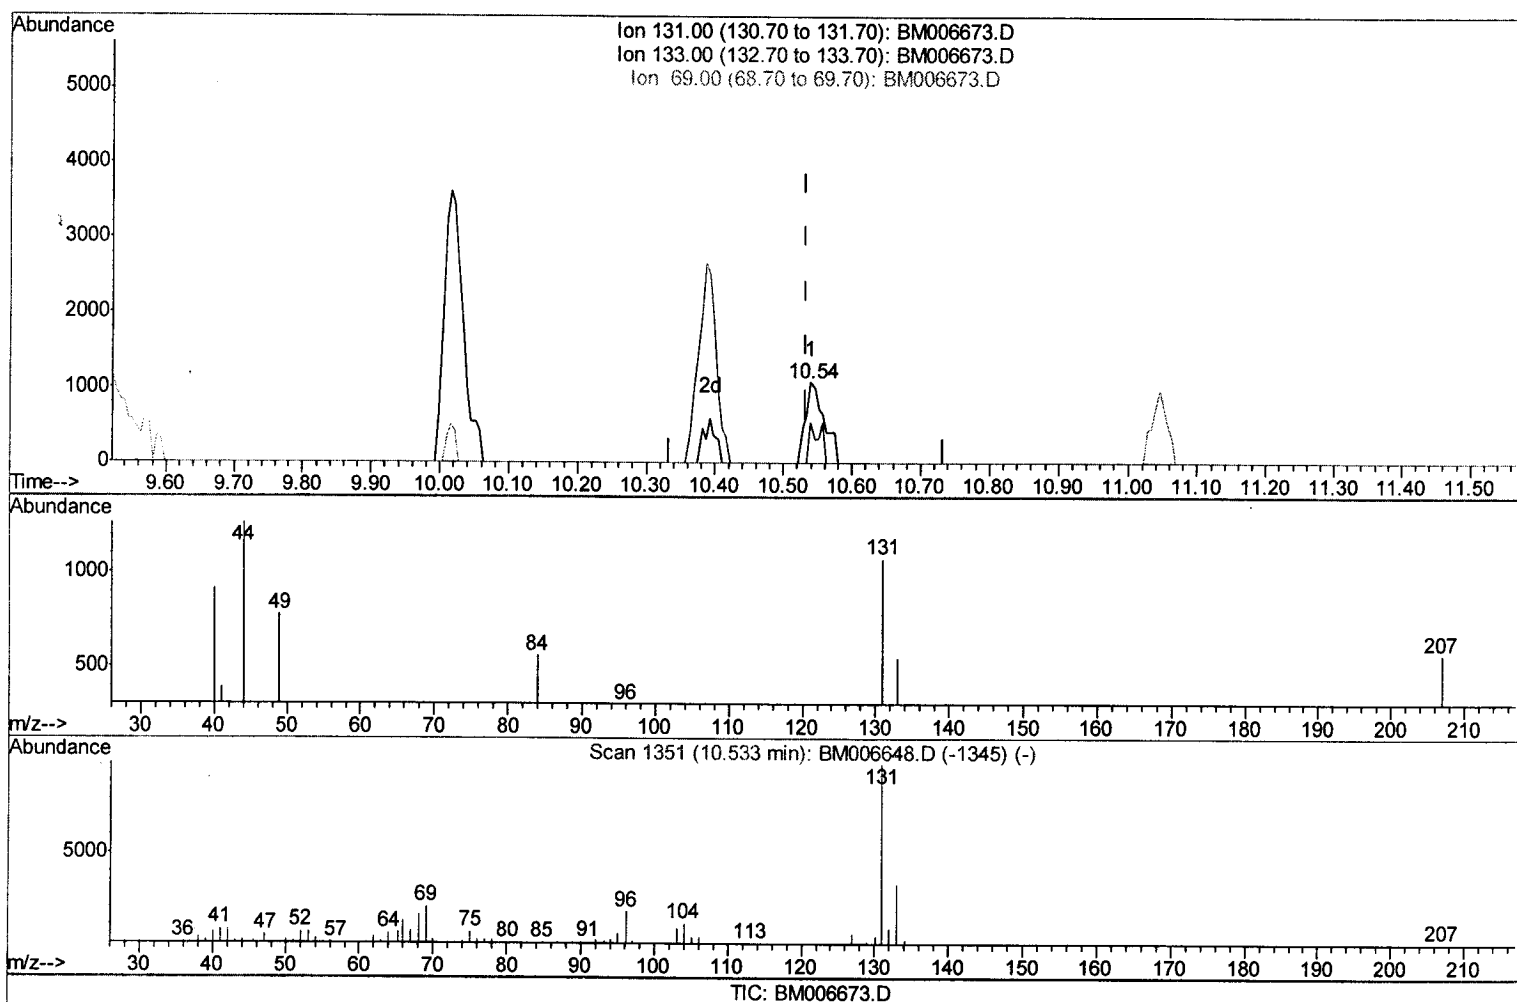

(29) 4-Chloroaniline-d4 (S)

10.539min (+0.006) 0.21ng/ul m U.M

response 2046

Ion	Exp%	Act%
131.00	100	100
133.00	32.70	50.93#
69.00	20.30	0.00#
0.00	0.00	0.00

07/28/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006673.D
 Acq On : 27 Jul 2016 05:24
 Operator : UM/SJ
 Sample : H4062-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJC0

Quant Time: Jul 27 06:10:05 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 15:24:14 2016
 Response via : Initial Calibration

Manual Integration

sohil
 7/27/2016 7:10:08 PM

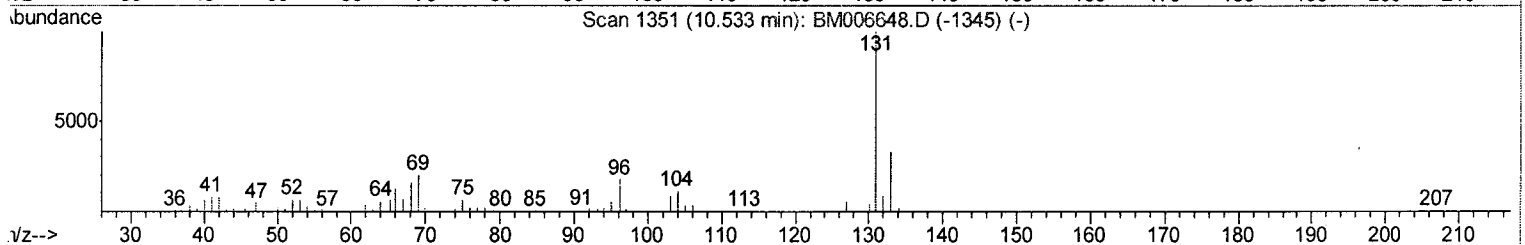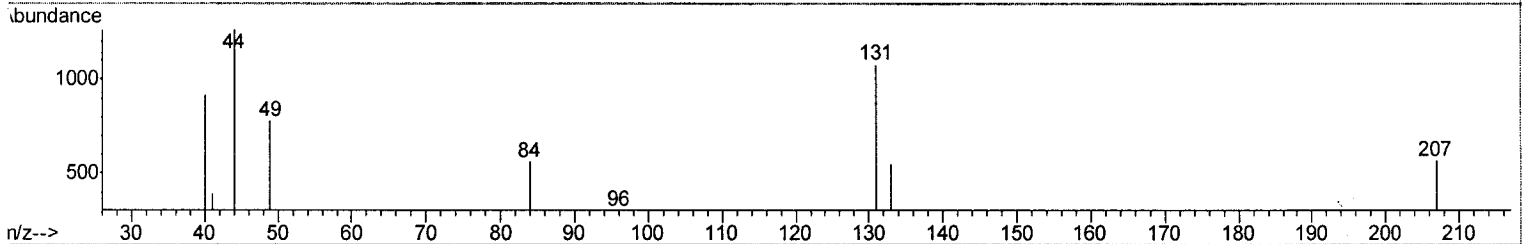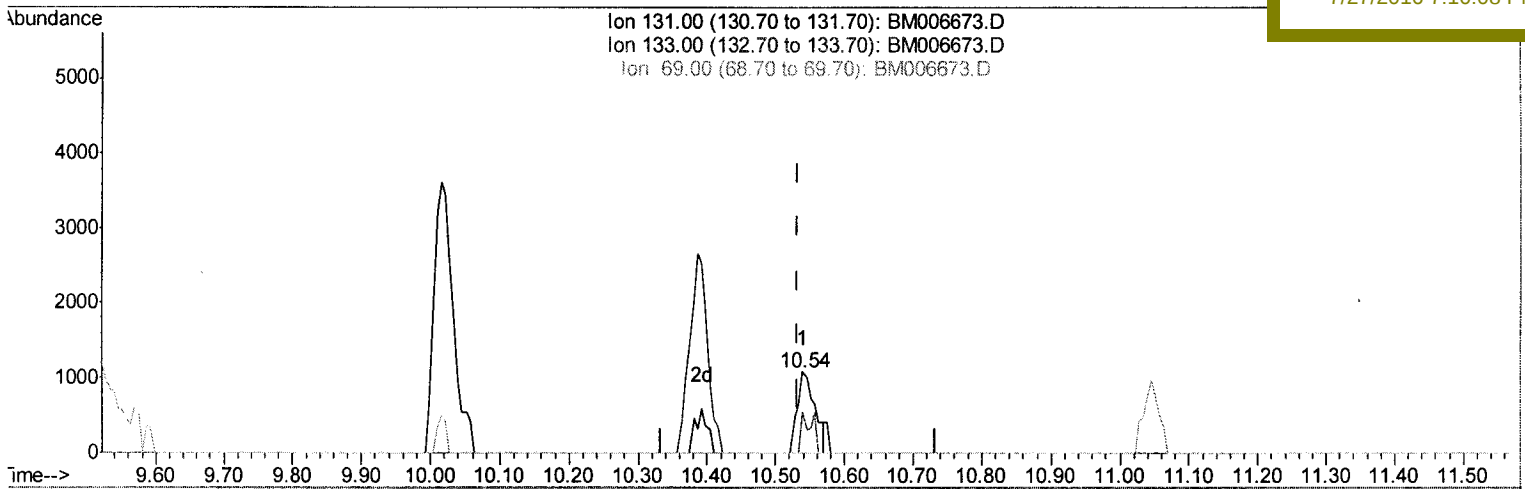

TIC: BM006673.D

(29) 4-Chloroaniline-d4 (S)

10.539min (+0.006) 0.19ng/ul

response 1904

Ion	Exp%	Act%
131.00	100	100
133.00	32.70	50.93#
69.00	20.30	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006673.D
Acq On : 27 Jul 2016 05:24
Operator : UM/SJ
Sample : H4062-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC0

Quant Time: Jul 27 06:44:08 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 15:24:14 2016
Response via : Initial Calibration

Manual Integration

sohil
7/27/2016 7:10:08 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	150386	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	633274	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	345595	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	810145	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1021733	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	1103187	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	2533	0.65	ng/uL	0.00
5) Phenol-d5	6.79	99	87601	6.63	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	204345	25.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	215632	20.80	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	143092	13.80	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	123644	25.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	134691	25.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	215882	22.29	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	2046m	0.21	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	765438	27.76	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	922155	26.60	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	28204	5.94	ng/ul	0.00
57) Fluorene-d10	15.26	176	678427	28.36	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	110071	24.93	ng/ul	0.00
70) Anthracene-d10	17.11	188	1155570	30.57	ng/ul	0.00
76) Pyrene-d10	19.42	212	1357207	28.63	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1524939	30.55	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U.M
07/28/16