

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006658.D
 Acq On : 26 Jul 2016 20:21
 Operator : UM/SJ
 Sample : H4062-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJC2

Quant Time: Jul 27 03:55:12 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 15:24:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	177326	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	825366	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	485763	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	1106010	20.00	ng/ul	0.00
75) Chrysene-d12	21.21	240	1249828	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	1299731	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	8284	1.82	ng/uL	0.00
5) Phenol-d5	6.79	99	305201	19.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	192704	20.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	239282	19.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	245120	20.05	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	116421	18.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	128080	18.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	227245	18.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	333321	26.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	735943	18.99	ng/ul	0.00
46) Acenaphthylene-d8	13.96	160	922928	18.94	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	90556	13.58	ng/ul	0.00
57) Fluorene-d10	15.26	176	650458	19.35	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	65111	10.80	ng/ul	0.00
70) Anthracene-d10	17.12	188	1010991	19.59	ng/ul	0.00
76) Pyrene-d10	19.42	212	1140590	19.67	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1178789	20.04	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.72	163	319482	8.24	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006658.D
Acq On : 26 Jul 2016 20:21
Operator : UM/SJ
Sample : H4062-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC2

Quant Time: Jul 27 03:55:12 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 15:24:14 2016
Response via : Initial Calibration

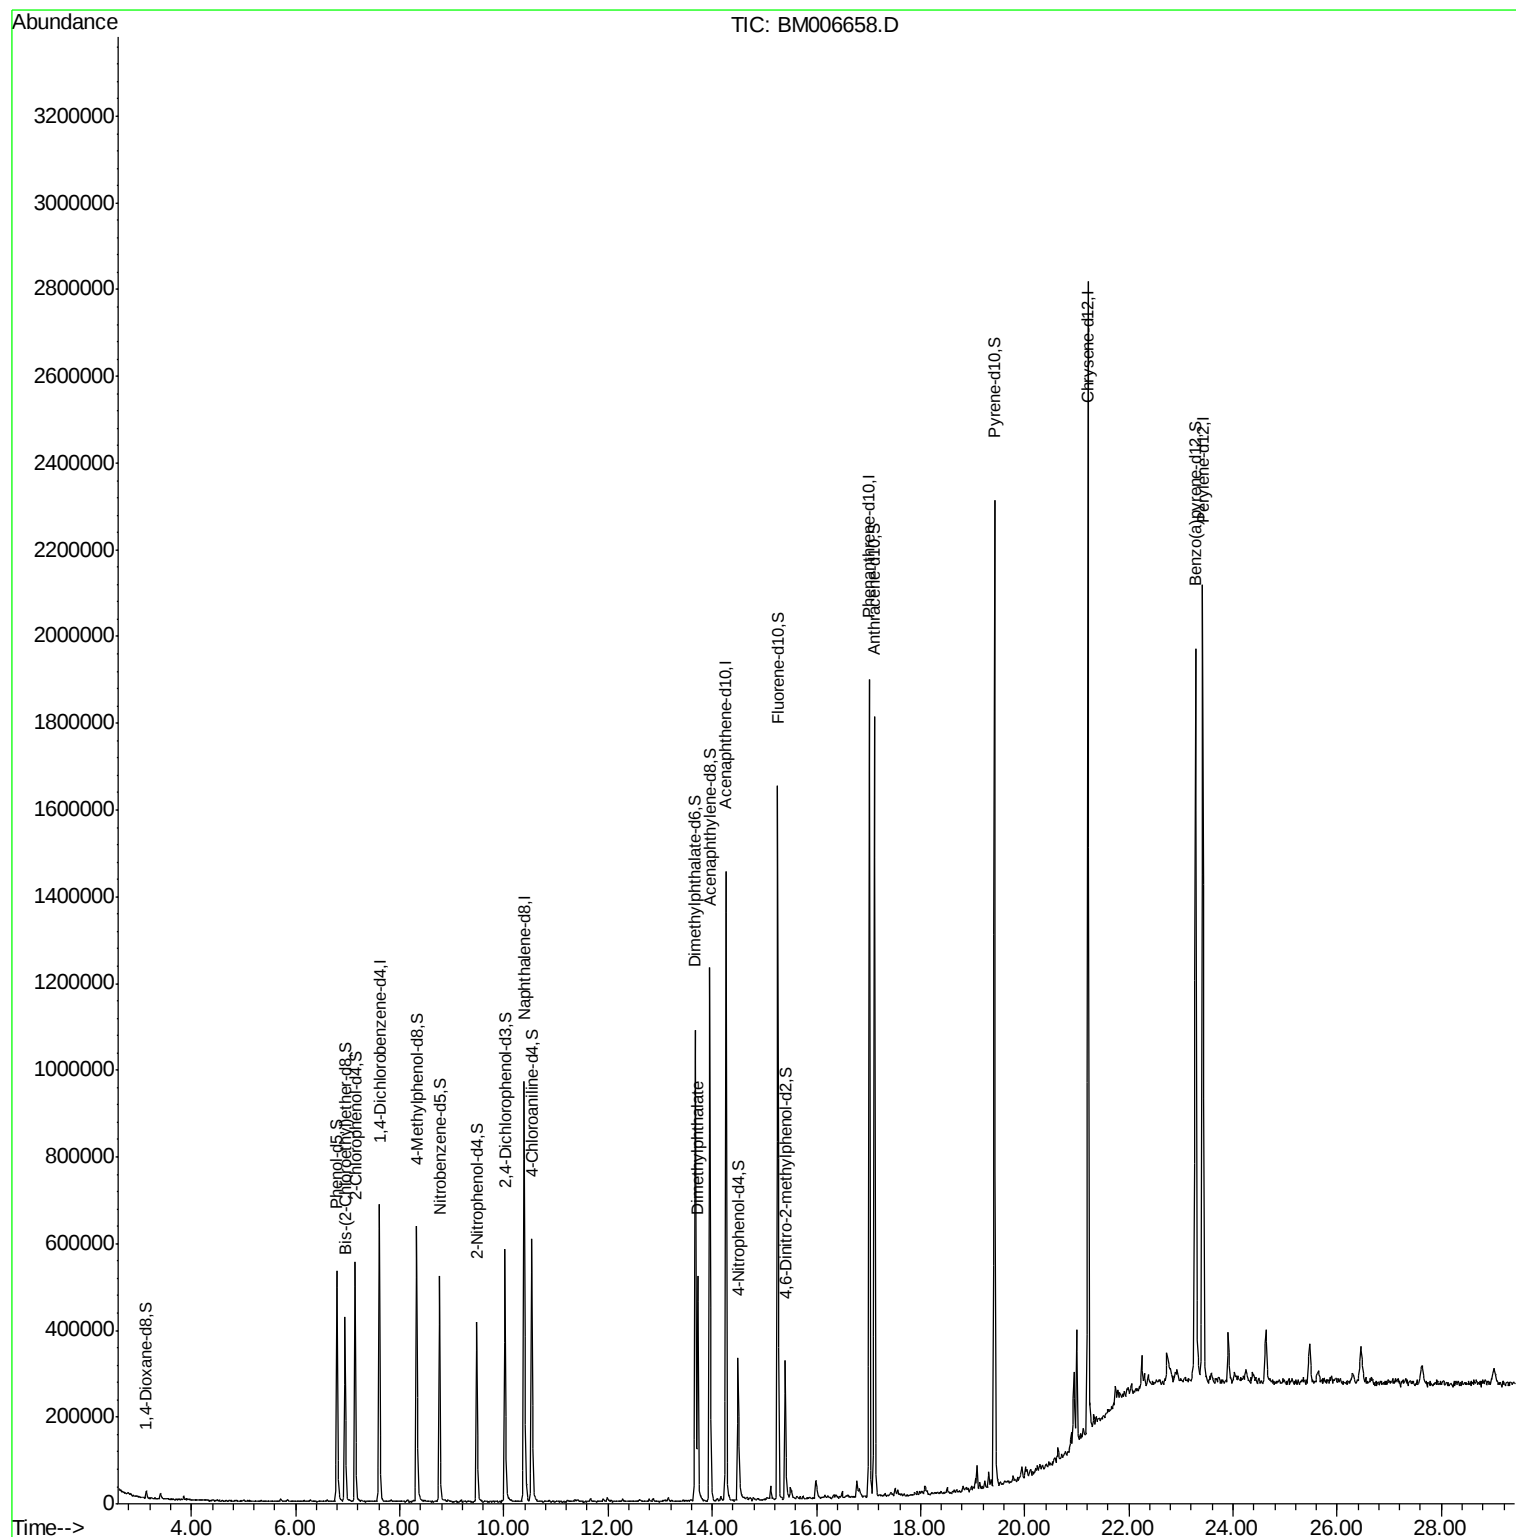

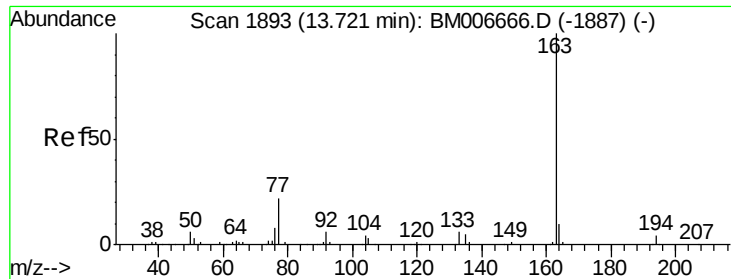

#44

Dimethylphthalate

Concen: 8.24 ng/ul

RT: 13.72 min Scan# 1893

Delta R.T. -0.01 min

Lab File: BM006658.D

Acq: 26 Jul 2016 20:21

Instrument :

BNA_M

ClientSampleId :

BDJC2


Tgt Ion:163 Resp: 319482

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 10.1 7.8 11.8

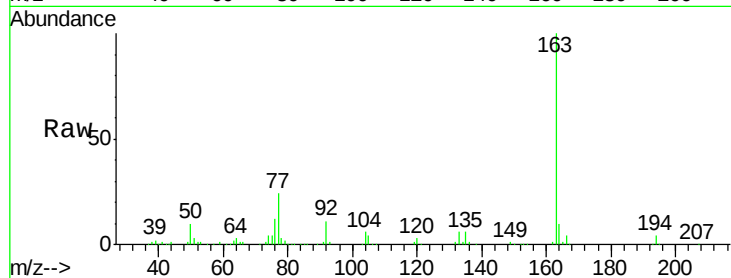

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

