

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006661.D
 Acq On : 26 Jul 2016 22:10
 Operator : UM/SJ
 Sample : H4062-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJC6

Quant Time: Jul 27 03:55:38 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 15:24:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	174926	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	765943	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	441242	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	1010949	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1199819	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	1244864	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	7964	1.77	ng/uL	0.00
5) Phenol-d5	6.79	99	298218	19.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	199368	21.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	239460	19.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	242330	20.09	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	117445	19.86	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	126461	19.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	222413	18.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	331431	27.85	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	746602	21.21	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	913730	20.64	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	101125	16.69	ng/ul	0.00
57) Fluorene-d10	15.26	176	647265	21.19	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	71498	12.98	ng/ul	0.00
70) Anthracene-d10	17.12	188	1003556	21.27	ng/ul	0.00
76) Pyrene-d10	19.42	212	1167055	20.97	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1251337	22.21	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.72	163	285982	8.12 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006661.D
Acq On : 26 Jul 2016 22:10
Operator : UM/SJ
Sample : H4062-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC6

Quant Time: Jul 27 03:55:38 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 15:24:14 2016
Response via : Initial Calibration

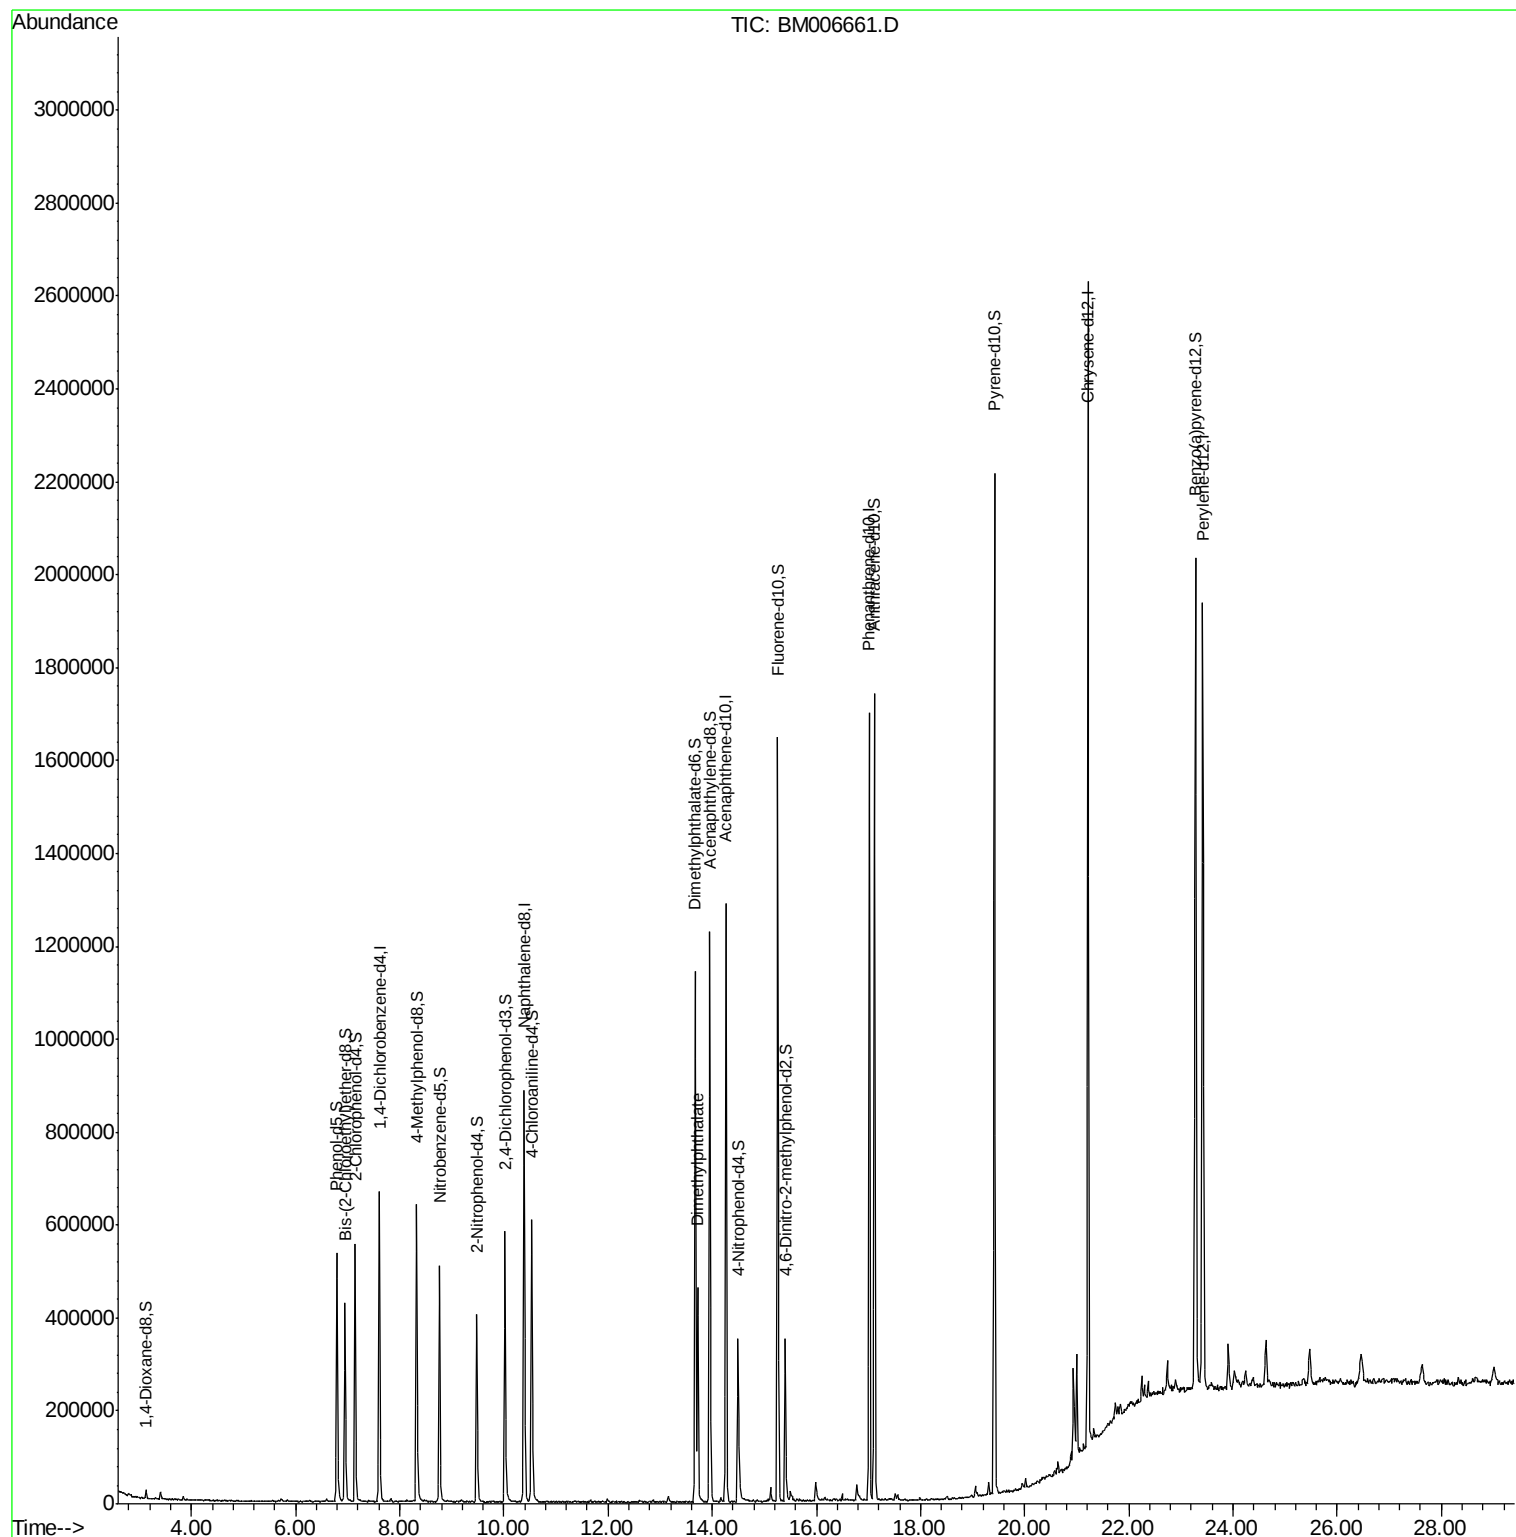

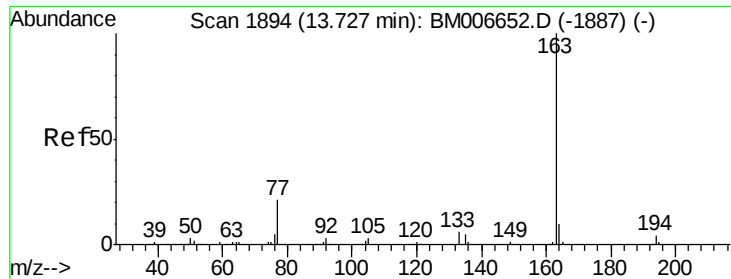

#44

Dimethylphthalate

Concen: 8.12 ng/ul

RT: 13.72 min Scan# 1893

Delta R.T. -0.01 min

Lab File: BM006661.D

Acq: 26 Jul 2016 22:10

Instrument :

BNA_M

ClientSampleId :

BDJC6


Tgt Ion:163 Resp: 285982

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 9.8 7.8 11.8

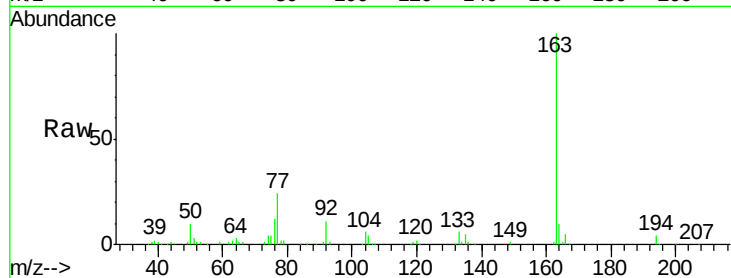

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

