

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006662.D
 Acq On : 26 Jul 2016 22:47
 Operator : UM/SJ
 Sample : H4062-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJC7

Quant Time: Jul 27 03:55:45 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 15:24:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	161033	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	689584	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	386628	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	889548	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1077388	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	1141264	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	7473	1.80	ng/uL	0.00
5) Phenol-d5	6.79	99	267063	18.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	174008	20.02	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	208496	18.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	207564	18.70	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	100066	18.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	107015	18.61	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	186115	17.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	275172	25.69	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	601380	19.49	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	751185	19.37	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	81121	15.28	ng/ul	0.00
57) Fluorene-d10	15.26	176	527311	19.71	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	59997	12.37	ng/ul	0.00
70) Anthracene-d10	17.12	188	829889	19.99	ng/ul	0.00
76) Pyrene-d10	19.42	212	955920	19.13	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1042190	20.18	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.72	163	227261	7.36	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006662.D
Acq On : 26 Jul 2016 22:47
Operator : UM/SJ
Sample : H4062-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC7

Quant Time: Jul 27 03:55:45 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 15:24:14 2016
Response via : Initial Calibration

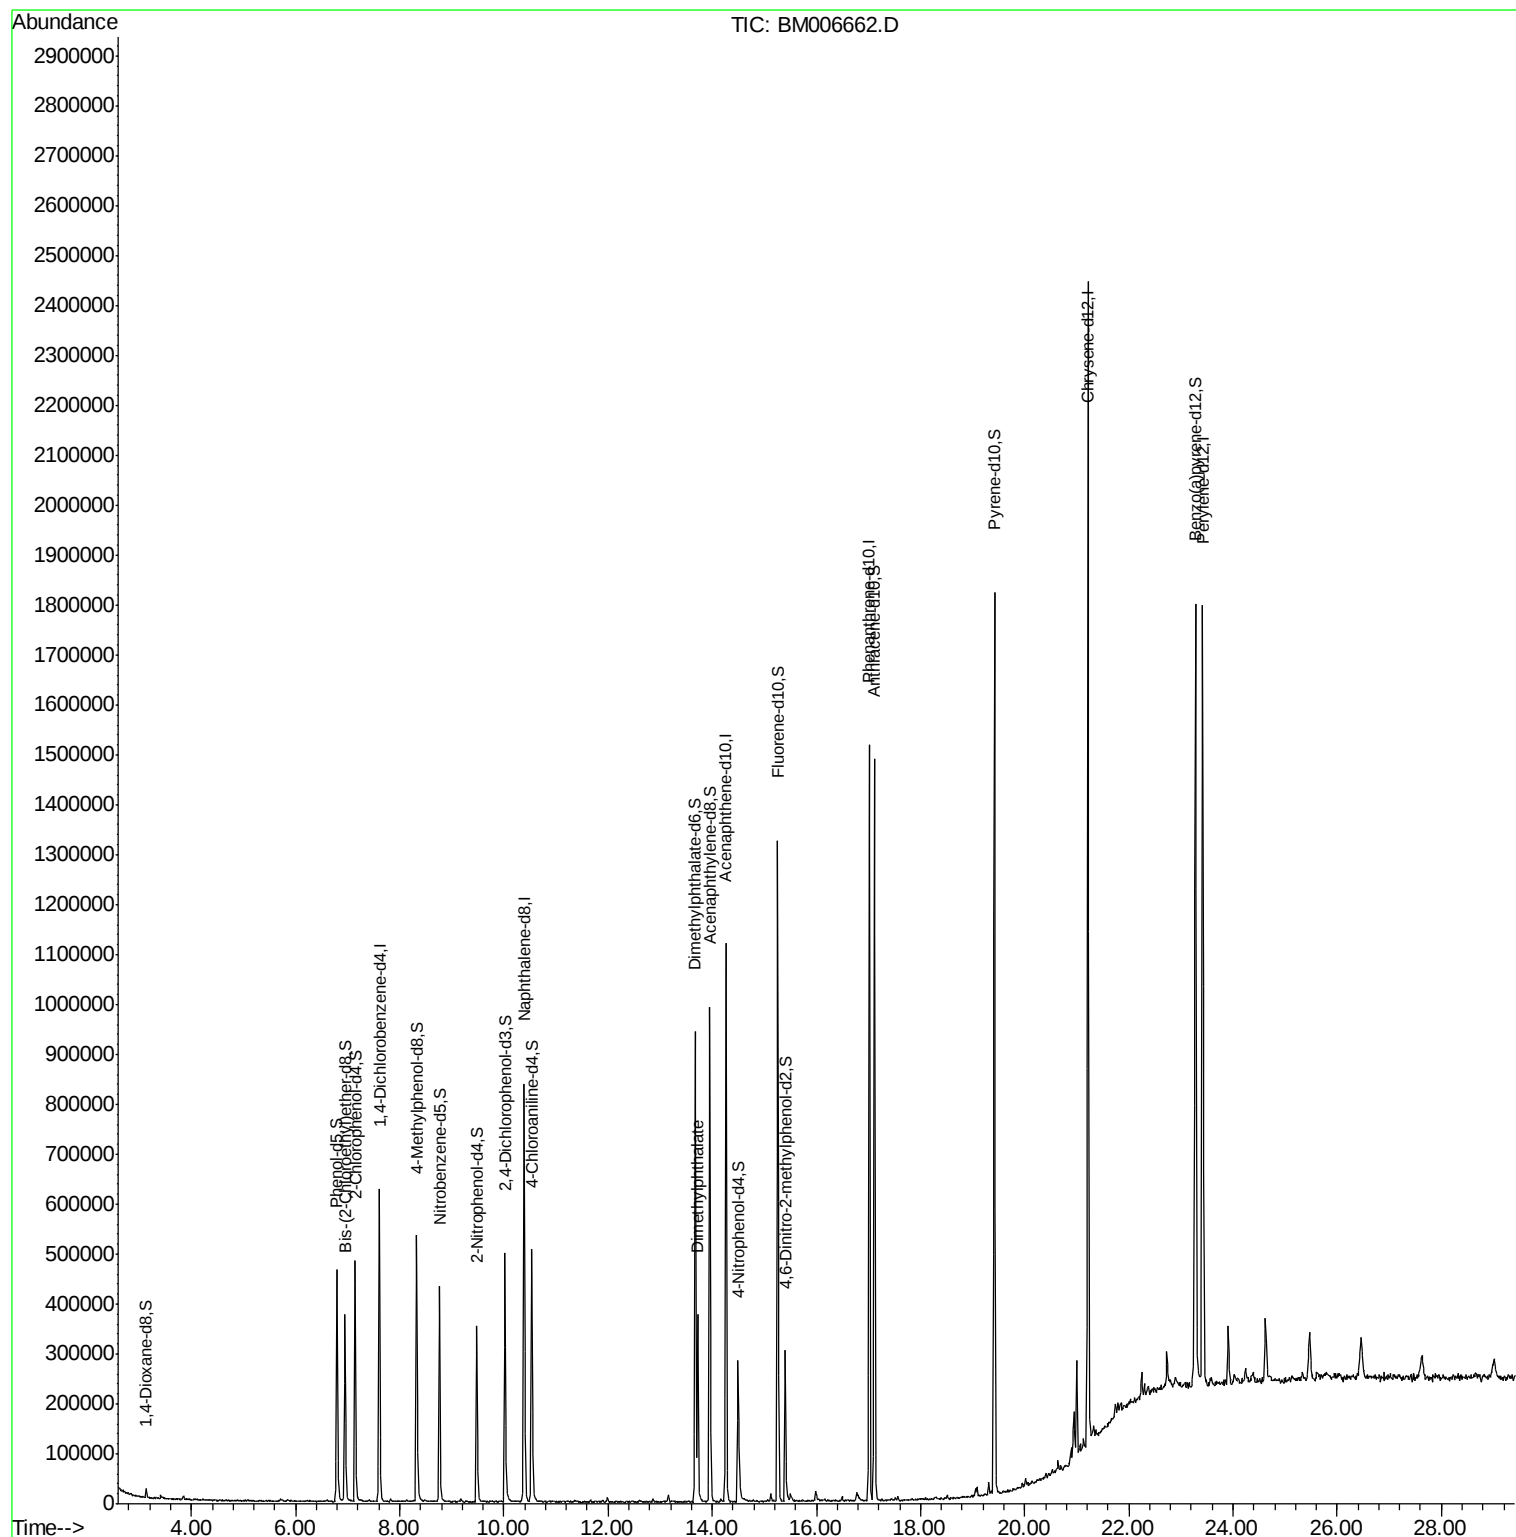

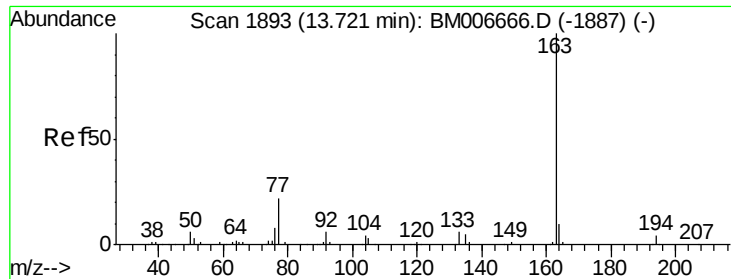

#44
 Dimethylphthalate
 Concen: 7.36 ng/ul
 RT: 13.72 min Scan# 1893
 Delta R.T. -0.01 min
 Lab File: BM006662.D
 Acq: 26 Jul 2016 22:47

Instrument :
 BNA_M
 ClientSampleId :
 BDJC7

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.4	5.0
164	10.9	7.8	11.8

