

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006665.D
 Acq On : 27 Jul 2016 00:35
 Operator : UM/SJ
 Sample : H4062-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJD2

Quant Time: Jul 27 03:56:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 15:24:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	145641	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	630378	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	361495	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	843003	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1013587	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	1064518	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	7280	1.94	ng/uL	0.00
5) Phenol-d5	6.79	99	271848	21.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	176818	22.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	213524	21.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	217214	21.63	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	101851	20.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	108717	20.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	196777	20.41	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	289976	29.61	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	651130	22.57	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	804398	22.18	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	88760	17.88	ng/ul	0.00
57) Fluorene-d10	15.26	176	567504	22.68	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	60273	13.12	ng/ul	0.00
70) Anthracene-d10	17.12	188	896025	22.78	ng/ul	0.00
76) Pyrene-d10	19.42	212	1033964	21.99	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1122287	23.30	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.72	163	247612	8.58	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006665.D
Acq On : 27 Jul 2016 00:35
Operator : UM/SJ
Sample : H4062-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJD2

Quant Time: Jul 27 03:56:06 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 15:24:14 2016
Response via : Initial Calibration

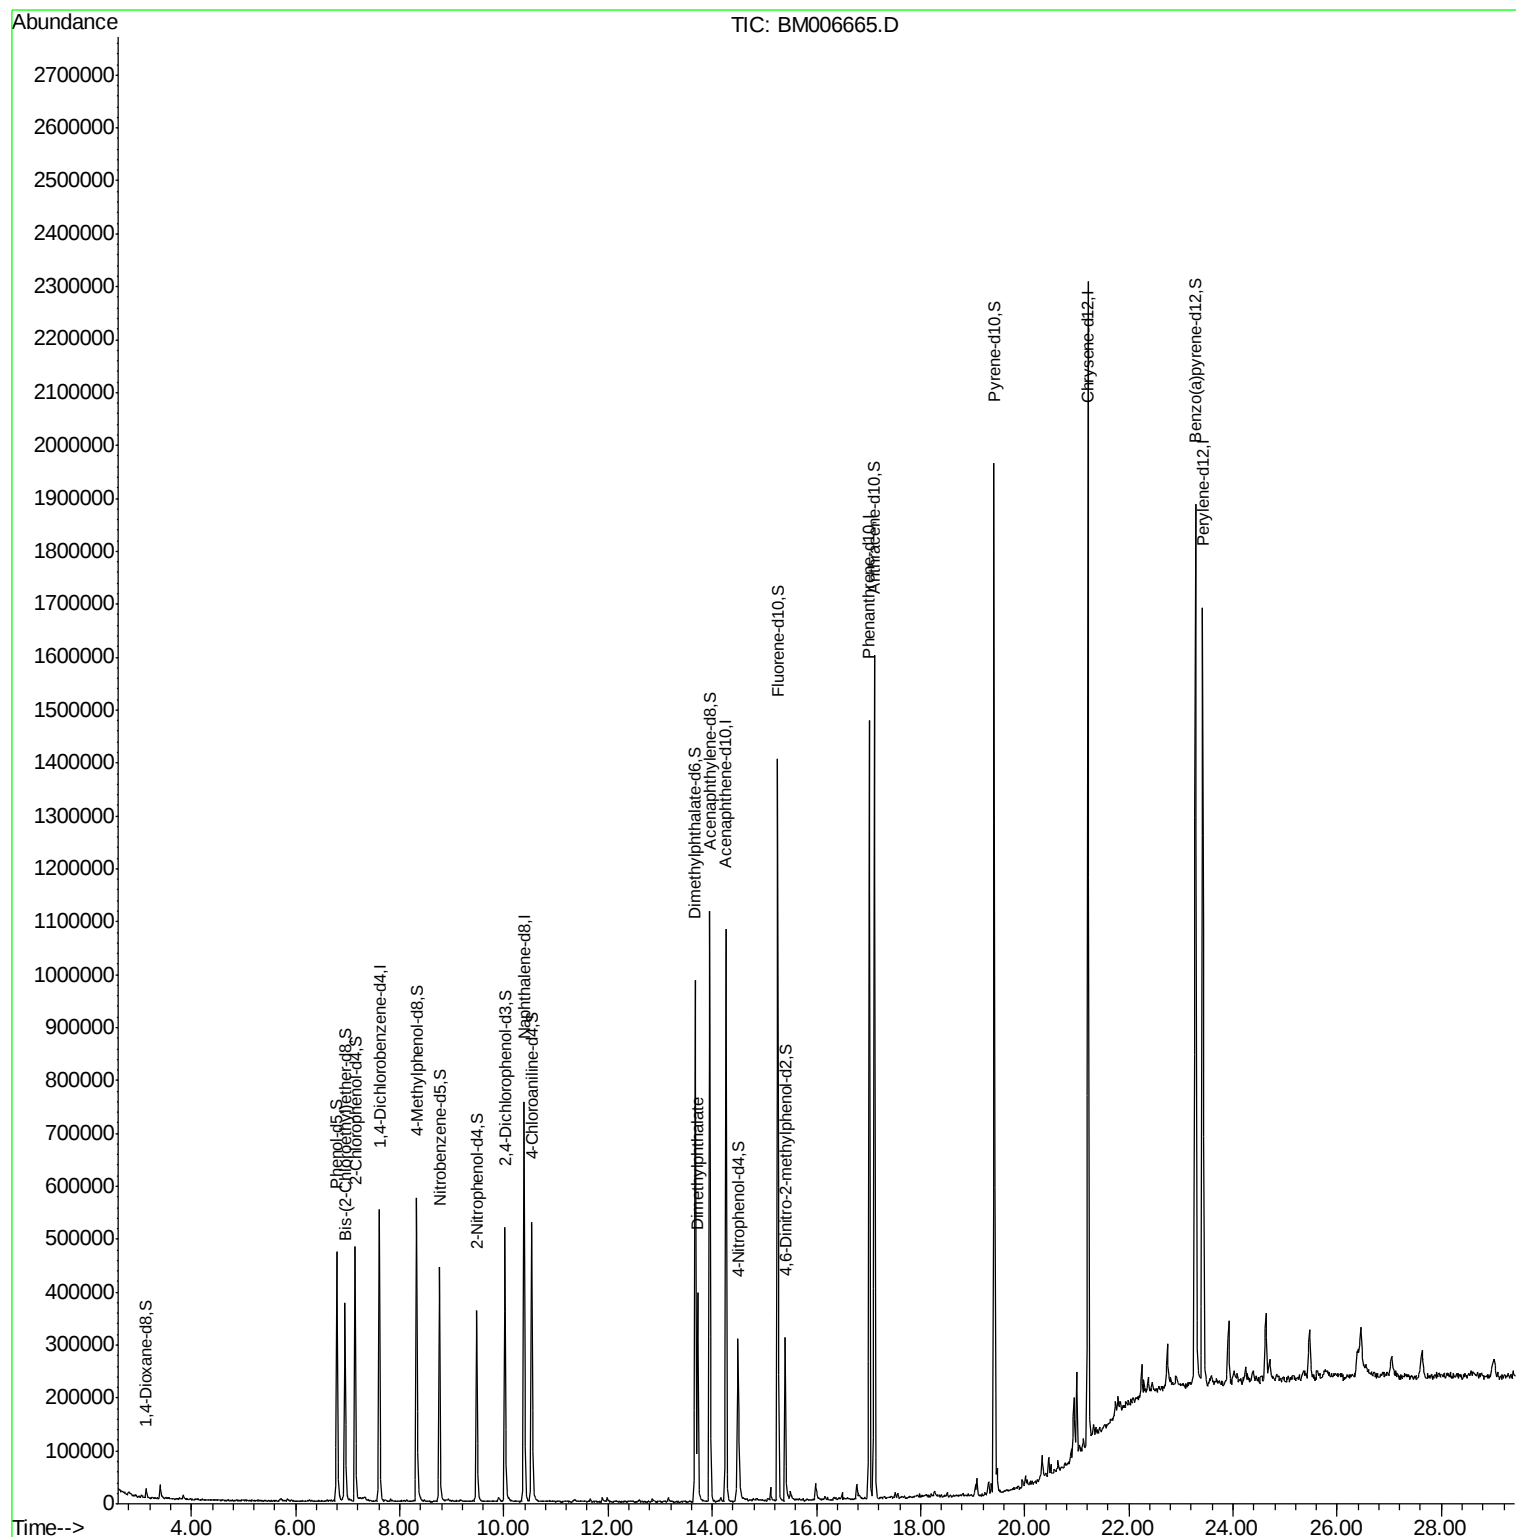

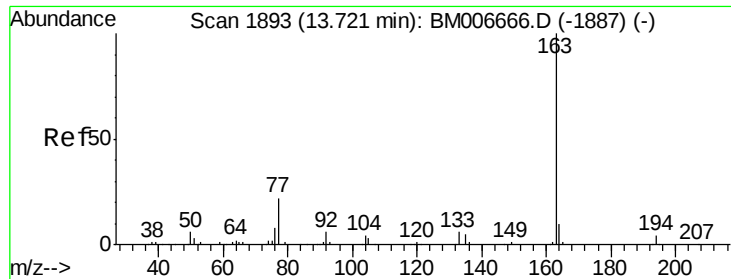

#44

Dimethylphthalate

Concen: 8.58 ng/ul

RT: 13.72 min Scan# 1893

Delta R.T. -0.01 min

Lab File: BM006665.D

Acq: 27 Jul 2016 00:35

Instrument :

BNA_M

ClientSampleId :

BDJD2



Tgt Ion:163 Resp: 247612

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.0

164 10.0 7.8 11.8

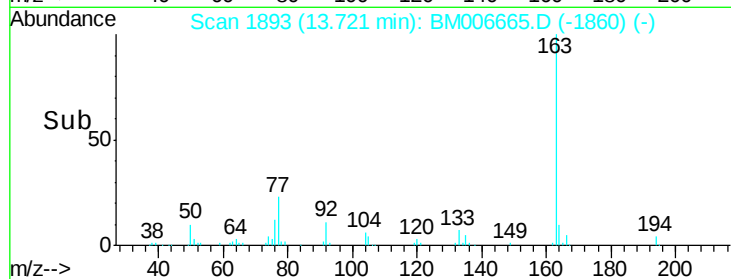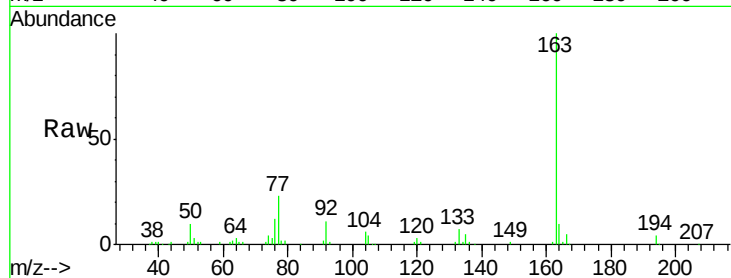

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

