

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006667.D
 Acq On : 27 Jul 2016 01:47
 Operator : UM/SJ
 Sample : H4062-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJC5

Quant Time: Jul 27 03:56:41 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 15:24:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	153019	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	683874	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	399331	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	924291	20.00	ng/ul	0.00
75) Chrysene-d12	21.21	240	1059404	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	1133507	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	4876	1.24	ng/uL	0.00
5) Phenol-d5	6.79	99	194198	14.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	126598	15.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	153351	14.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	150000	14.22	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	70884	13.43	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	75824	13.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	137671	13.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	201704	18.99	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	466310	14.63	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	566995	14.15	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	56318	10.27	ng/ul	0.00
57) Fluorene-d10	15.26	176	406072	14.69	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	41083	8.16	ng/ul	0.00
70) Anthracene-d10	17.12	188	631681	14.65	ng/ul	0.00
76) Pyrene-d10	19.42	212	722292	14.70	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	778088	15.17	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.72	163	175503	5.51	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006667.D
Acq On : 27 Jul 2016 01:47
Operator : UM/SJ
Sample : H4062-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC5

Quant Time: Jul 27 03:56:41 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 15:24:14 2016
Response via : Initial Calibration

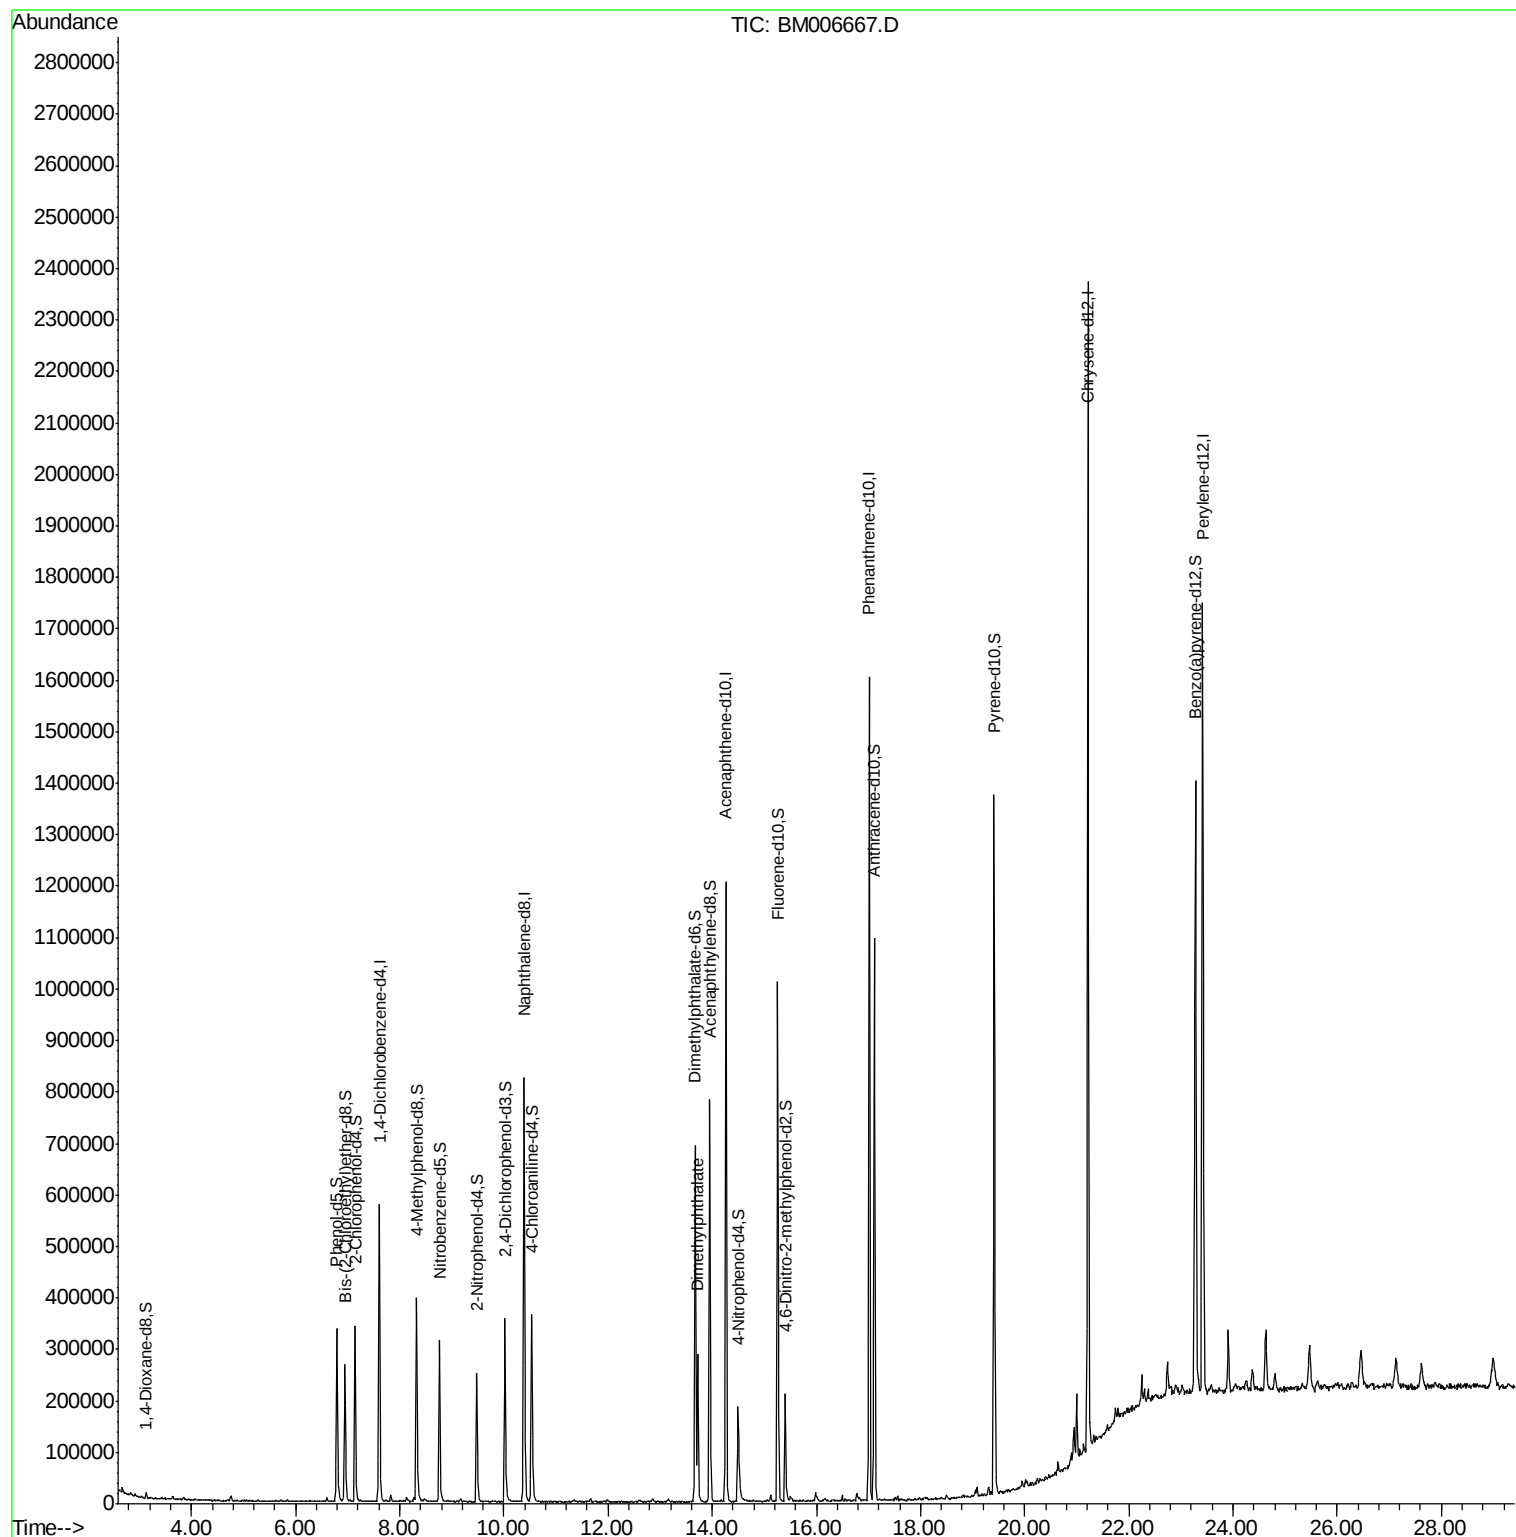

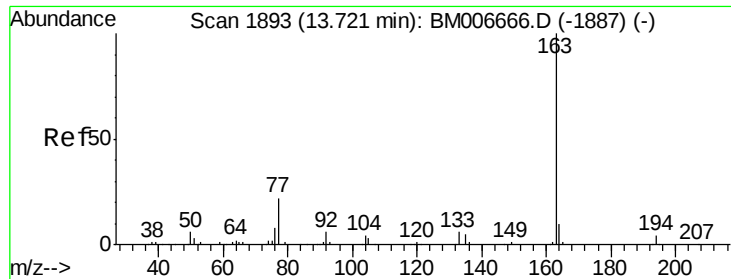

#44

Dimethylphthalate

Concen: 5.51 ng/ul

RT: 13.72 min Scan# 1893

Delta R.T. -0.01 min

Lab File: BM006667.D

Acq: 27 Jul 2016 01:47

Instrument :

BNA_M

ClientSampleId :

BDJC5

Tgt Ion:163 Resp: 175503

Ion Ratio Lower Upper

163 100

194 3.7 3.4 5.0

164 10.2 7.8 11.8

