

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006669.D
 Acq On : 27 Jul 2016 02:59
 Operator : UM/SJ
 Sample : H4062-13
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJD0

Quant Time: Jul 27 03:56:55 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 15:24:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	151152	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	630304	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	359890	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	839377	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1028417	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	1094124	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	5507	1.42	ng/uL	0.00
5) Phenol-d5	6.79	99	210909	15.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	132890	16.29	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	163121	15.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	164561	15.79	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	75049	15.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	78927	15.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	146978	15.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	213478	21.80	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	474070	16.51	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	585672	16.22	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	54305	10.99	ng/ul	0.00
57) Fluorene-d10	15.26	176	420158	16.87	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	39044	8.53	ng/ul	0.00
70) Anthracene-d10	17.11	188	663309	16.93	ng/ul	0.00
76) Pyrene-d10	19.42	212	764672	16.03	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	837972	16.92	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.72	163	188542	6.56	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006669.D
Acq On : 27 Jul 2016 02:59
Operator : UM/SJ
Sample : H4062-13
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJD0

Quant Time: Jul 27 03:56:55 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 15:24:14 2016
Response via : Initial Calibration

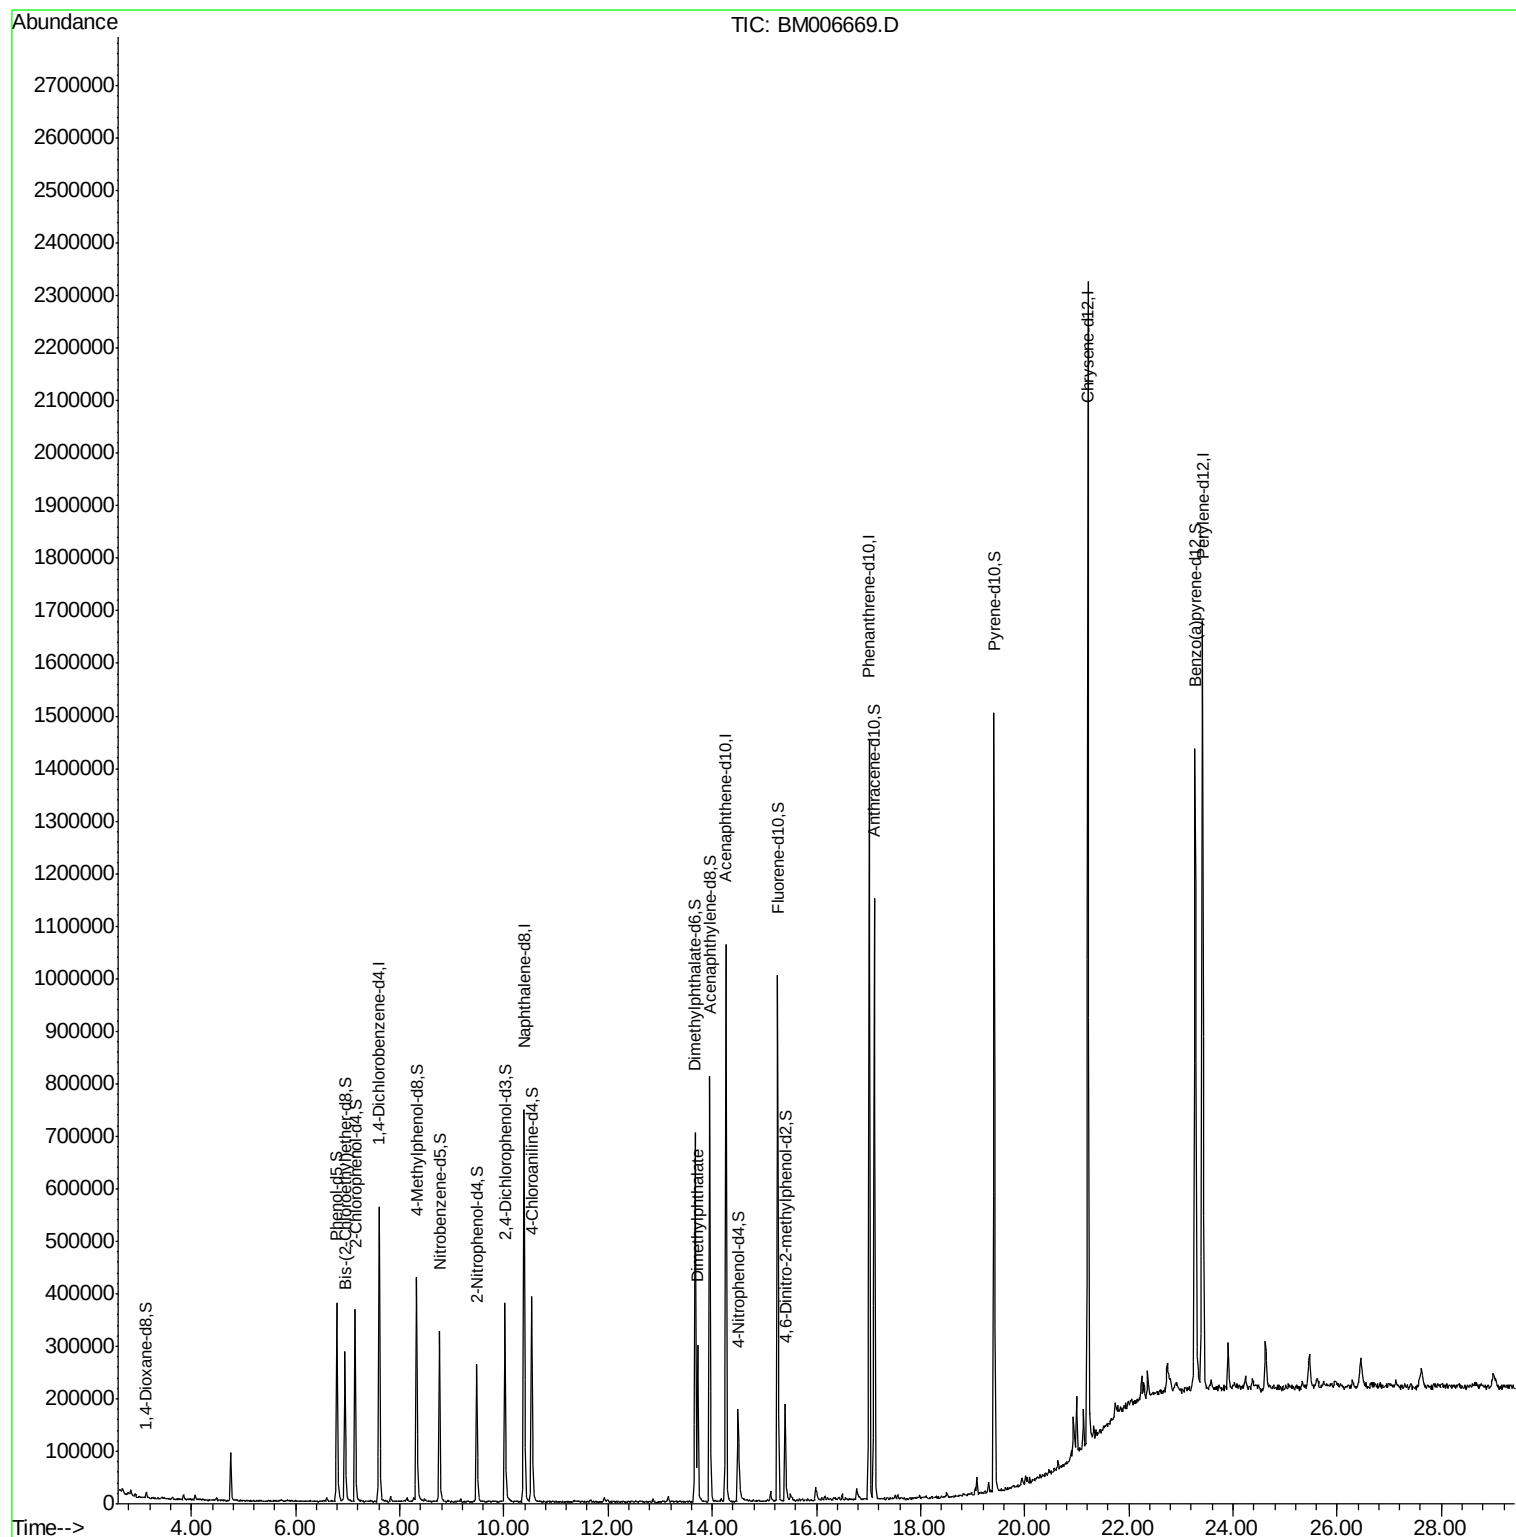


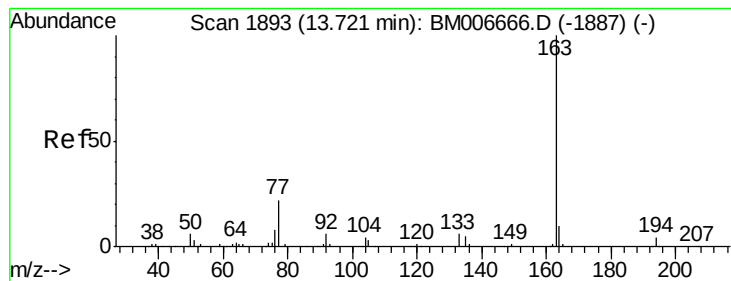

#44
 Dimethylphthalate
 Concen: 6.56 ng/ul
 RT: 13.72 min Scan# 1893
 Delta R.T. -0.01 min
 Lab File: BM006669.D
 Acq: 27 Jul 2016 02:59

Instrument :
 BNA_M
 ClientSampleId :
 BDJD0

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.4	5.0
164	9.9	7.8	11.8

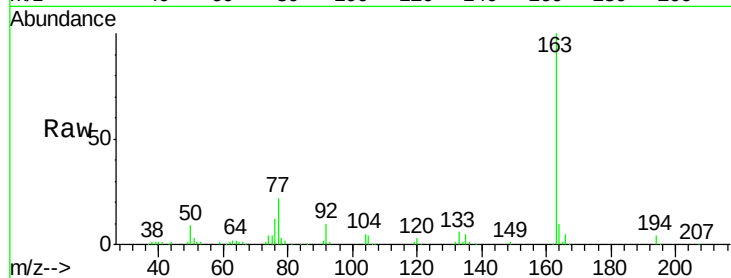

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

