

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006670.D
 Acq On : 27 Jul 2016 03:36
 Operator : UM/SJ
 Sample : H4062-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJD3

Quant Time: Jul 27 04:54:41 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 15:24:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	168701	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	745497	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	433144	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	1001287	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1161179	20.00	ng/ul	0.00
83) Perylene-d12	23.42	264	1222423	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	8010	1.85	ng/uL	0.00
5) Phenol-d5	6.79	99	296180	19.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	196147	21.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	242525	20.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	240697	20.70	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	115817	20.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	118653	19.08	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	218225	19.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	327274	28.26	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	744817	21.55	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	927279	21.34	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	77327	13.00	ng/ul	0.00
57) Fluorene-d10	15.26	176	670688	22.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	56245	10.31	ng/ul	0.00
70) Anthracene-d10	17.11	188	1064858	22.79	ng/ul	0.00
76) Pyrene-d10	19.42	212	1211980	22.50	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.28	264	1301407	23.53	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.72	163	410537	11.87	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006670.D
Acq On : 27 Jul 2016 03:36
Operator : UM/SJ
Sample : H4062-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJD3

Quant Time: Jul 27 04:54:41 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 15:24:14 2016
Response via : Initial Calibration

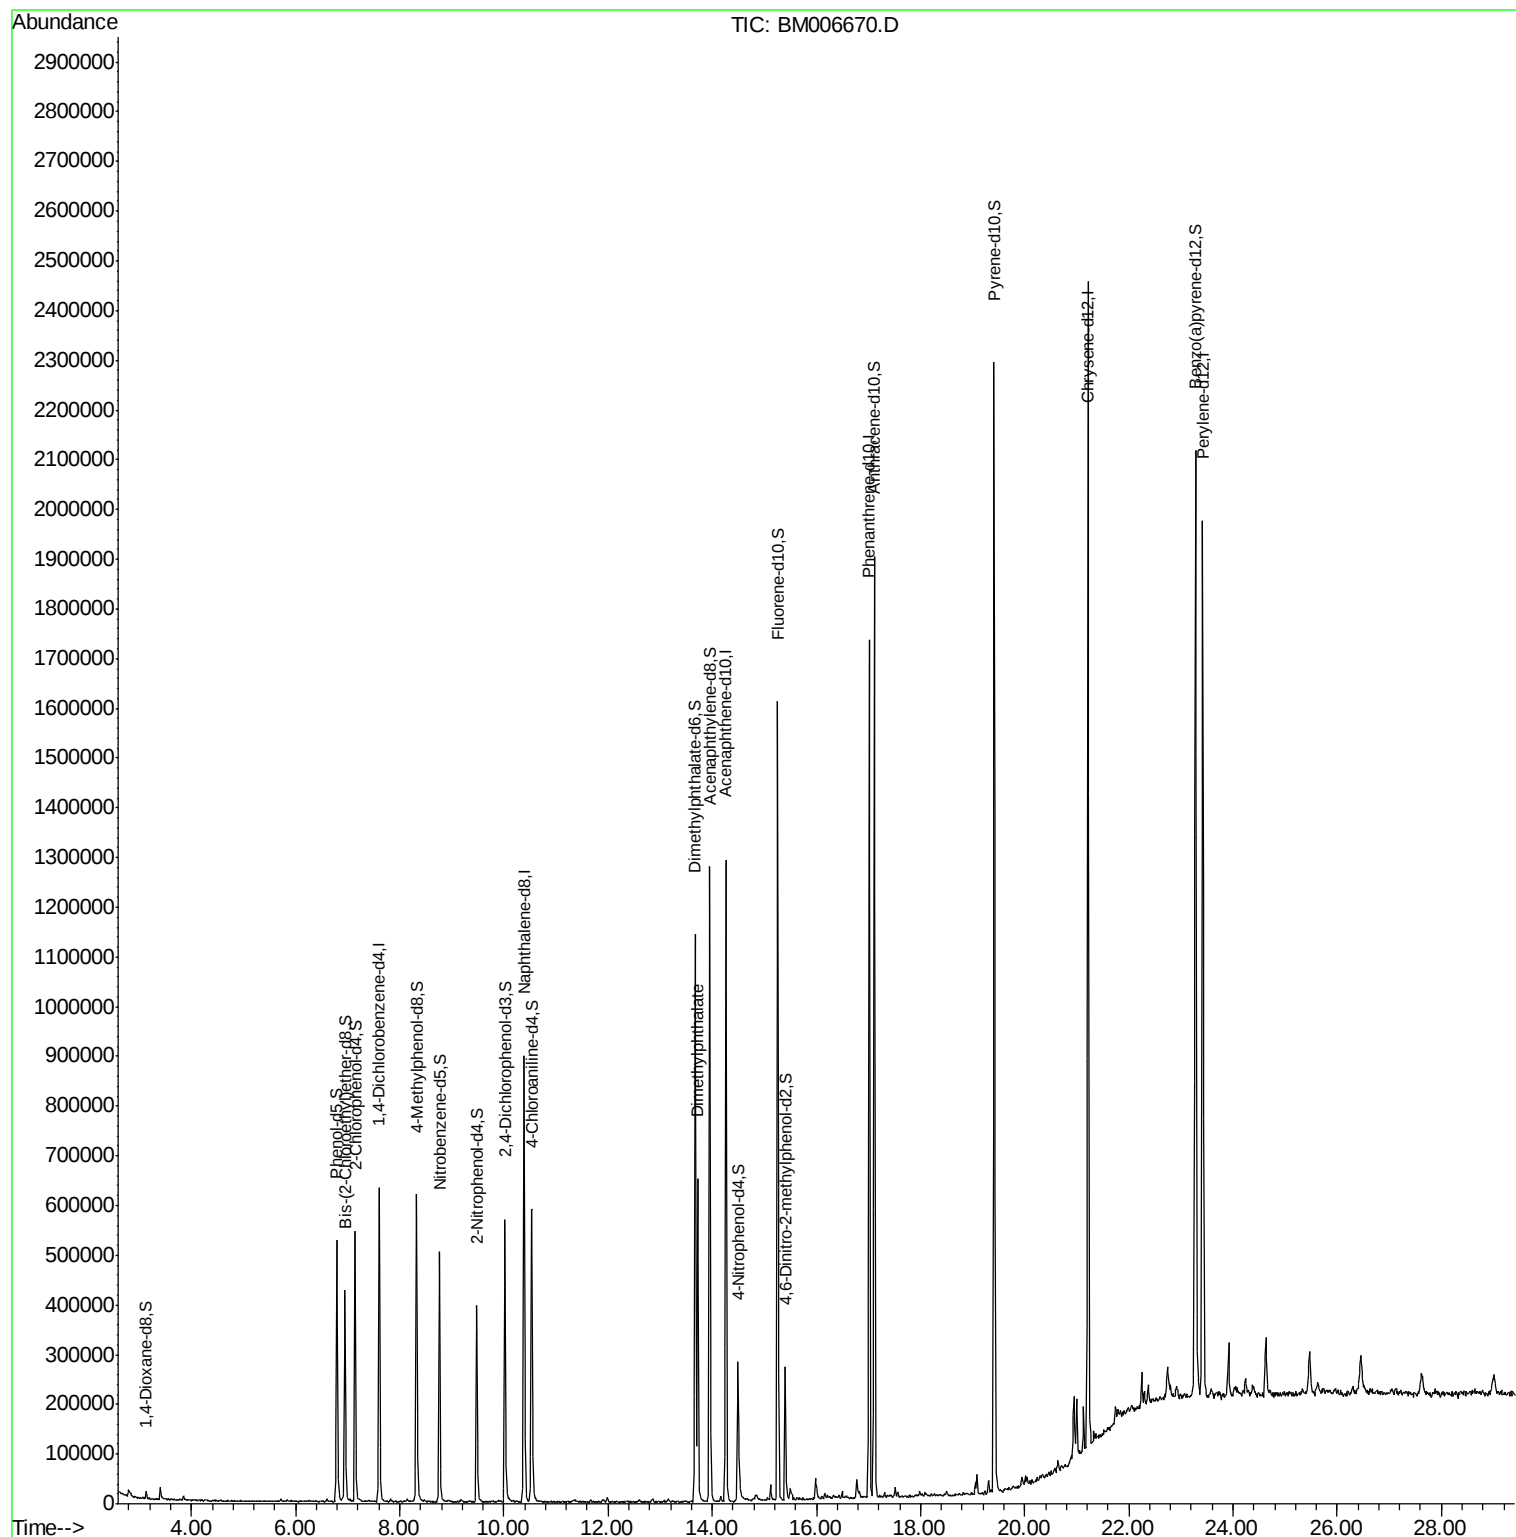


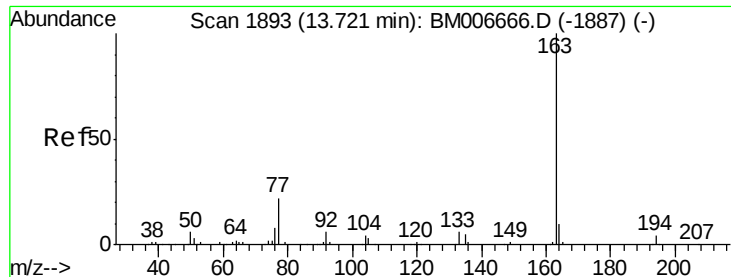

#44
 Dimethylphthalate
 Concen: 11.87 ng/ul
 RT: 13.72 min Scan# 1893
 Delta R.T. -0.01 min
 Lab File: BM006670.D
 Acq: 27 Jul 2016 03:36

Instrument :
 BNA_M
 ClientSampleId :
 BDJD3

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.4	5.0
164	10.2	7.8	11.8

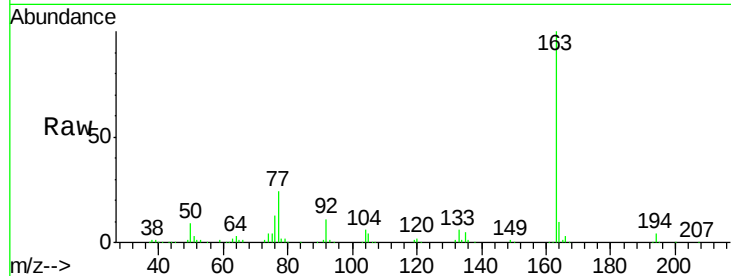

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

