

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006680.D
 Acq On : 27 Jul 2016 09:36
 Operator : UM/SJ
 Sample : H4094-07
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJE0

Quant Time: Jul 27 11:38:03 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 26 15:24:14 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	158257	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	671774	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	380807	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	862447	20.00	ng/ul	0.00
75) Chrysene-d12	21.22	240	1083659	20.00	ng/ul	0.00
83) Perylene-d12	23.41	264	1179511	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	6369	1.56	ng/uL	0.00
5) Phenol-d5	6.79	99	249912	17.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	152804	17.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.14	132	191251	17.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.32	113	195526	17.92	ng/ul	0.00
19) Nitrobenzene-d5	8.76	128	88691	17.10	ng/ul	0.00
22) 2-Nitrophenol-d4	9.48	143	99915	17.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	174726	17.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	262960	25.20	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	598115	19.68	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	723064	18.93	ng/ul	0.00
51) 4-Nitrophenol-d4	14.49	143	75912	14.52	ng/ul	0.00
57) Fluorene-d10	15.26	176	524630	19.90	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	59853	12.73	ng/ul	0.00
70) Anthracene-d10	17.11	188	843029	20.95	ng/ul	0.00
76) Pyrene-d10	19.42	212	985936	19.61	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.27	264	1114287	20.88	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.72	163	300161	9.87	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006680.D
Acq On : 27 Jul 2016 09:36
Operator : UM/SJ
Sample : H4094-07
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJE0

Quant Time: Jul 27 11:38:03 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 26 15:24:14 2016
Response via : Initial Calibration

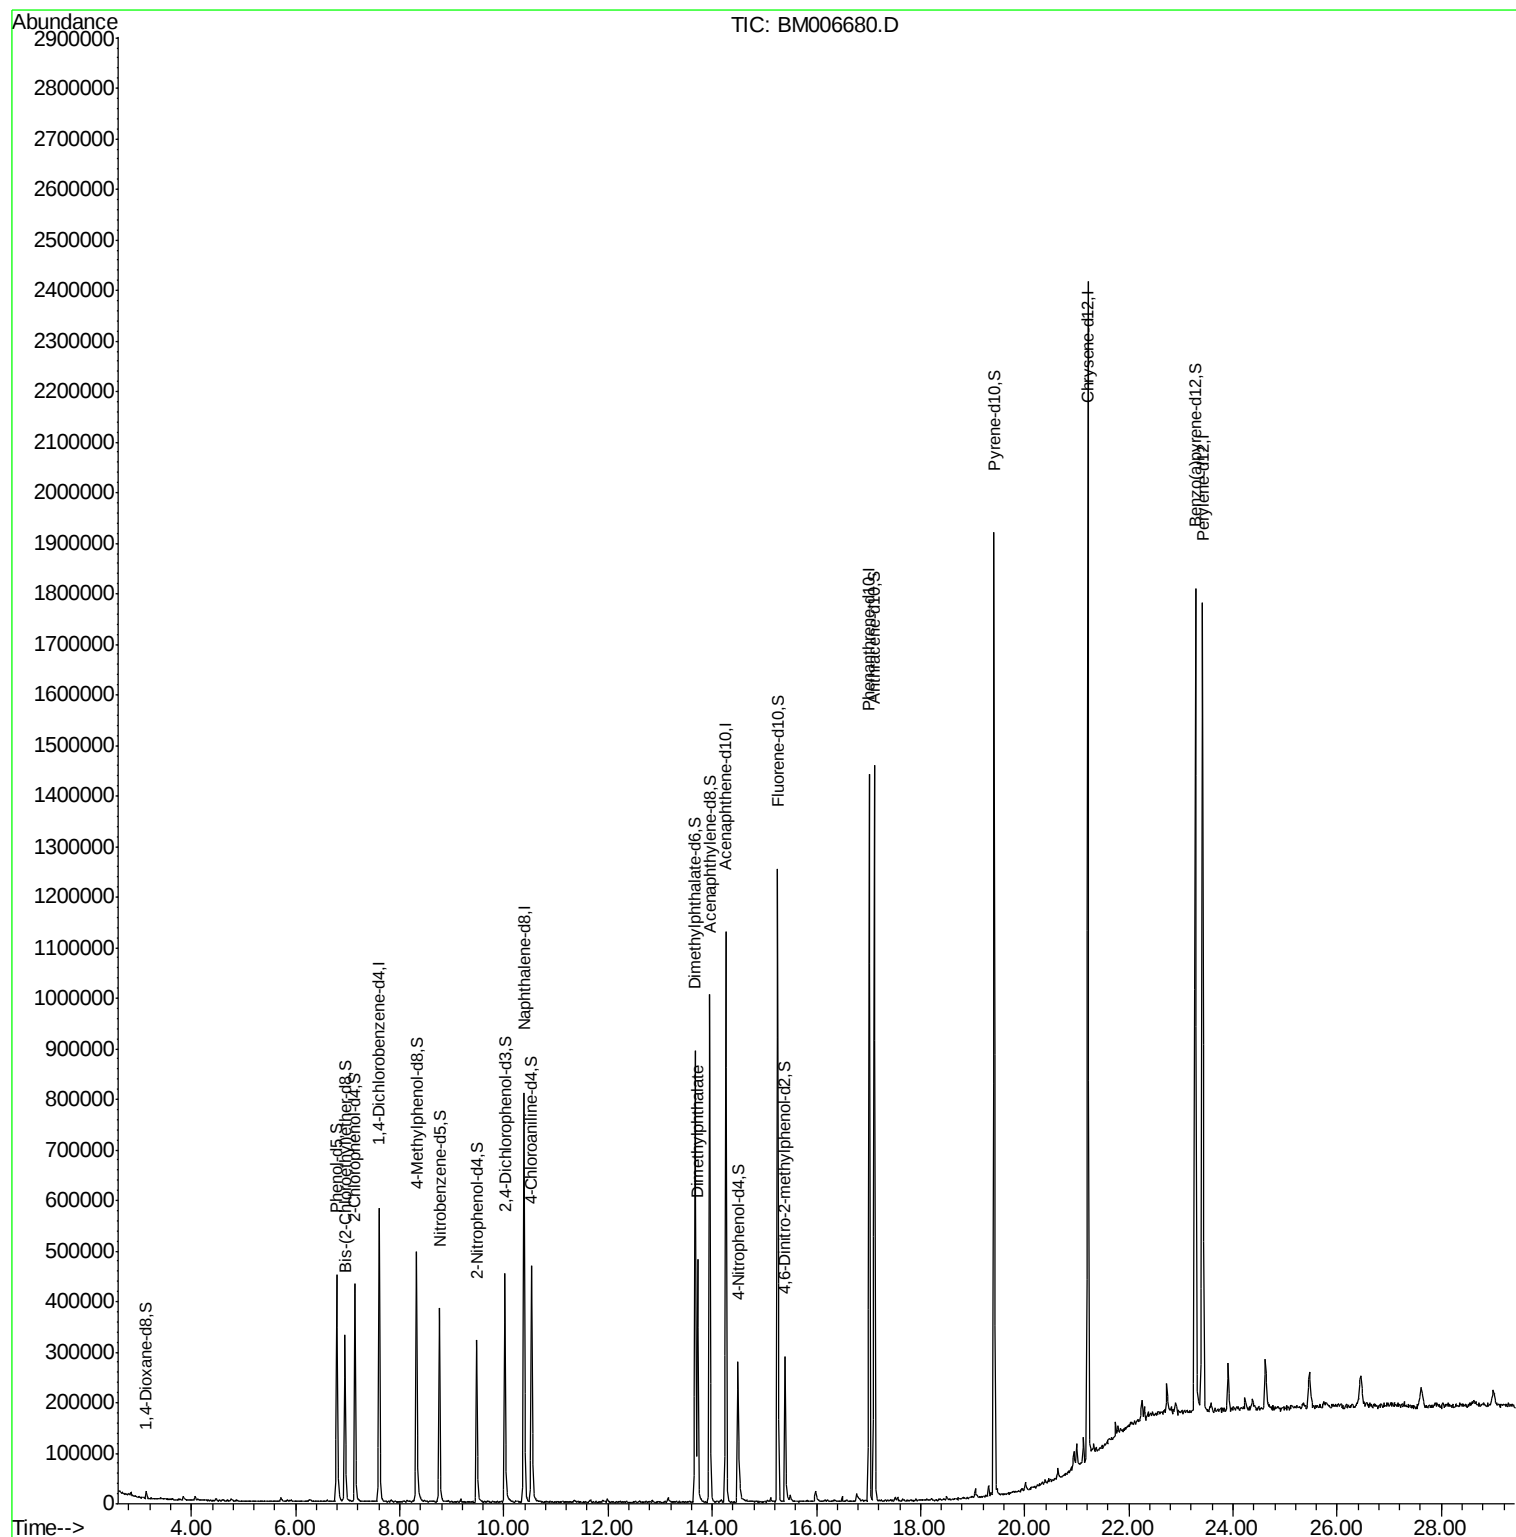

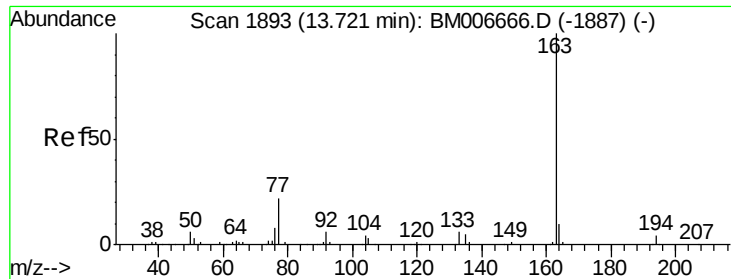

#44
 Dimethylphthalate
 Concen: 9.87 ng/ul
 RT: 13.72 min Scan# 1893
 Delta R.T. -0.01 min
 Lab File: BM006680.D
 Acq: 27 Jul 2016 09:36

Instrument :
 BNA_M
 ClientSampleId :
 BDJE0

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.5	3.4	5.0
164	9.7	7.8	11.8

