

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006660.D
 Acq On : 26 Jul 2016 21:34
 Operator : UM/SJ
 Sample : H4062-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJC4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.834	39	42	48	rVB	36642	41228	1.27%	0.134%
2	3.634	174	178	183	rBV2	38225	47907	1.47%	0.156%
3	6.792	702	715	727	rBV	325967	574372	17.64%	1.866%
4	6.951	735	742	753	rBV	276042	435351	13.37%	1.414%
5	7.145	768	775	786	rVB	353517	568512	17.46%	1.847%
6	7.610	843	854	866	rBV	598724	980655	30.12%	3.186%
7	8.322	969	975	984	rBV	348064	588960	18.09%	1.913%
8	8.763	1044	1050	1062	rBV	321364	560672	17.22%	1.821%
9	9.481	1165	1172	1182	rBV	254885	465043	14.28%	1.511%
10	10.022	1258	1264	1280	rBV	368385	657406	20.19%	2.136%
11	10.386	1319	1326	1332	rBV	797023	1409585	43.29%	4.579%
12	10.433	1332	1334	1342	rVB	75124	120148	3.69%	0.390%
13	10.533	1342	1351	1370	rBV	339651	659378	20.25%	2.142%
14	13.674	1879	1885	1890	rBV	723987	1053964	32.37%	3.424%
15	13.721	1890	1893	1902	rVB	310448	455456	13.99%	1.480%
16	13.957	1920	1933	1944	rBV	784765	1339250	41.13%	4.350%
17	14.263	1978	1985	1993	rBV2	1141298	1864558	57.27%	6.057%
18	14.498	2019	2025	2040	rBV	177787	379133	11.64%	1.232%
19	15.127	2128	2132	2142	rVB6	20105	36459	1.12%	0.118%
20	15.262	2149	2155	2162	rBV	1108635	1617436	49.68%	5.254%
21	15.404	2175	2179	2190	rBV	157818	272319	8.36%	0.885%
22	15.527	2198	2200	2206	rVB3	24193	32629	1.00%	0.106%
23	15.986	2274	2278	2279	rBV	36632	39711	1.22%	0.129%
24	16.780	2408	2413	2418	rBV2	28138	51439	1.58%	0.167%
25	16.833	2418	2422	2426	rVB3	25878	39068	1.20%	0.127%
26	17.015	2447	2453	2459	rBV2	1526054	2347367	72.10%	7.625%
27	17.115	2464	2470	2481	rVB2	1187860	1820678	55.92%	5.914%
28	17.892	2598	2602	2607	rBV	23353	38802	1.19%	0.126%
29	18.086	2630	2635	2640	rBV2	52520	95108	2.92%	0.309%
30	18.651	2722	2731	2733	rBV7	12206	35331	1.09%	0.115%
31	18.821	2755	2760	2764	rBV3	45087	70900	2.18%	0.230%
32	19.080	2800	2804	2810	rVB	203438	286302	8.79%	0.930%
33	19.139	2810	2814	2818	rVB5	40839	52571	1.61%	0.171%
34	19.233	2827	2830	2835	rVB	37777	51426	1.58%	0.167%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006660.D
Acq On : 26 Jul 2016 21:34
Operator : UM/SJ
Sample : H4062-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC4

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Title : SVOA CALIBRATION

35	19.315	2839	2844	2847	rBV4	28764	51066	1.57%	0.166%
36	19.421	2856	2862	2875	rBV2	1443933	2405872	73.90%	7.815%
37	19.521	2877	2879	2886	rVB7	20475	35828	1.10%	0.116%
38	19.780	2919	2923	2924	rBV3	27495	35827	1.10%	0.116%
39	19.945	2948	2951	2960	rVB	82315	124917	3.84%	0.406%
40	20.021	2960	2964	2965	rBV4	30122	38999	1.20%	0.127%
41	20.050	2965	2969	2973	rVV2	66188	89025	2.73%	0.289%
42	20.109	2976	2979	2982	rVB	31820	35825	1.10%	0.116%
43	20.944	3117	3121	3125	rBV2	111328	180341	5.54%	0.586%
44	20.997	3126	3130	3136	rVB	232948	299998	9.21%	0.975%
45	21.215	3161	3167	3172	rBV	2294031	3255784	100.00%	10.576%
46	21.250	3172	3173	3181	rVB	170938	186057	5.71%	0.604%
47	23.280	3512	3518	3523	rBV2	1116616	1969199	60.48%	6.397%
48	23.421	3535	3542	3555	rVB	1534096	2986527	91.73%	9.701%


Sum of corrected areas: 30784389

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006660.D
Acq On : 26 Jul 2016 21:34
Operator : UM/SJ
Sample : H4062-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

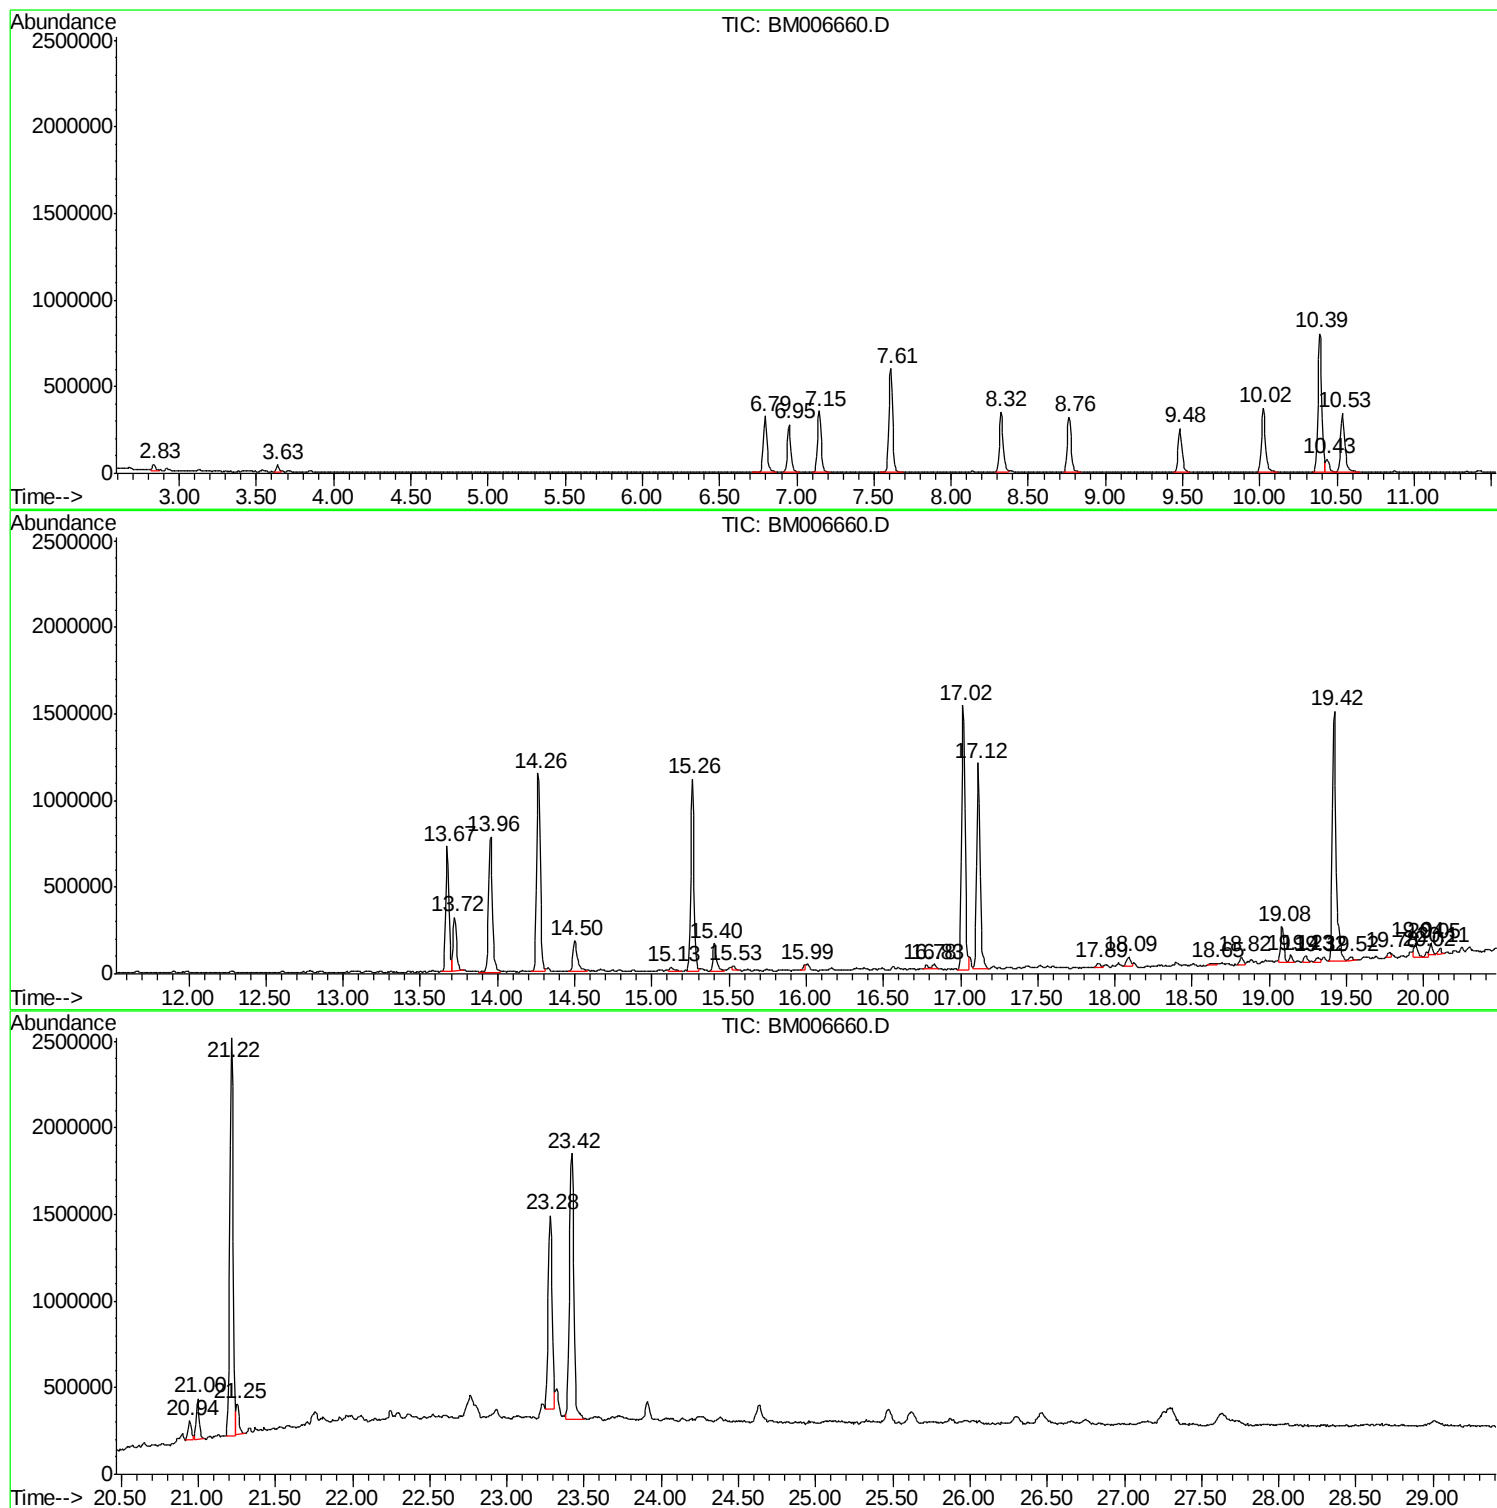

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006660.D
Acq On : 26 Jul 2016 21:34
Operator : UM/SJ
Sample : H4062-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006660.D
Acq On : 26 Jul 2016 21:34
Operator : UM/SJ
Sample : H4062-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc