

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006661.D
 Acq On : 26 Jul 2016 22:10
 Operator : UM/SJ
 Sample : H4062-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJC6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.793	709	715	732	rBV	533061	888903	26.22%	2.240%
2	6.951	732	742	755	rBV	426535	685535	20.22%	1.728%
3	7.145	767	775	789	rBV	555592	905129	26.70%	2.281%
4	7.610	847	854	864	rBV	668515	1111408	32.78%	2.801%
5	8.322	969	975	990	rBV	638595	1087534	32.08%	2.741%
6	8.763	1043	1050	1061	rBV	508666	869322	25.64%	2.191%
7	9.481	1166	1172	1186	rBV	403325	728806	21.50%	1.837%
8	10.022	1257	1264	1285	rBV	582241	1066685	31.46%	2.688%
9	10.386	1319	1326	1340	rBV	886382	1597604	47.12%	4.026%
10	10.533	1344	1351	1365	rBV	606279	1118361	32.99%	2.819%
11	13.674	1878	1885	1889	rBV	1141981	1615434	47.65%	4.071%
12	13.721	1889	1893	1911	rVB	460236	725876	21.41%	1.829%
13	13.951	1925	1932	1945	rBV	1229540	1958140	57.75%	4.935%
14	14.263	1979	1985	1998	rVB2	1288940	2087953	61.58%	5.262%
15	14.498	2018	2025	2042	rBV	352350	697490	20.57%	1.758%
16	15.121	2127	2131	2136	rBV	30166	41290	1.22%	0.104%
17	15.263	2148	2155	2165	rVB	1643737	2431610	71.72%	6.128%
18	15.404	2173	2179	2191	rBV	351377	546715	16.12%	1.378%
19	15.504	2192	2196	2204	rVB5	19820	40419	1.19%	0.102%
20	15.986	2273	2278	2287	rBV	41622	80800	2.38%	0.204%
21	16.780	2408	2413	2417	rBV	34053	52508	1.55%	0.132%
22	17.015	2447	2453	2462	rBV2	1694153	2548817	75.18%	6.424%
23	17.115	2463	2470	2479	rVB2	1736565	2653314	78.26%	6.687%
24	19.309	2839	2843	2847	rBV2	28418	37360	1.10%	0.094%
25	19.421	2855	2862	2869	rBV	2197480	3178546	93.75%	8.011%
26	20.939	3116	3120	3127	rBV2	197359	399848	11.79%	1.008%
27	20.997	3127	3130	3138	rVB	215904	291355	8.59%	0.734%
28	21.215	3162	3167	3182	rBV	2507853	3390490	100.00%	8.545%
29	23.280	3511	3518	3531	rBV2	1775843	3371116	99.43%	8.496%
30	23.421	3535	3542	3550	rVB	1683580	3265965	96.33%	8.231%
31	23.909	3622	3625	3637	rVB2	99718	204096	6.02%	0.514%


Sum of corrected areas: 39678429

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006661.D
Acq On : 26 Jul 2016 22:10
Operator : UM/SJ
Sample : H4062-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

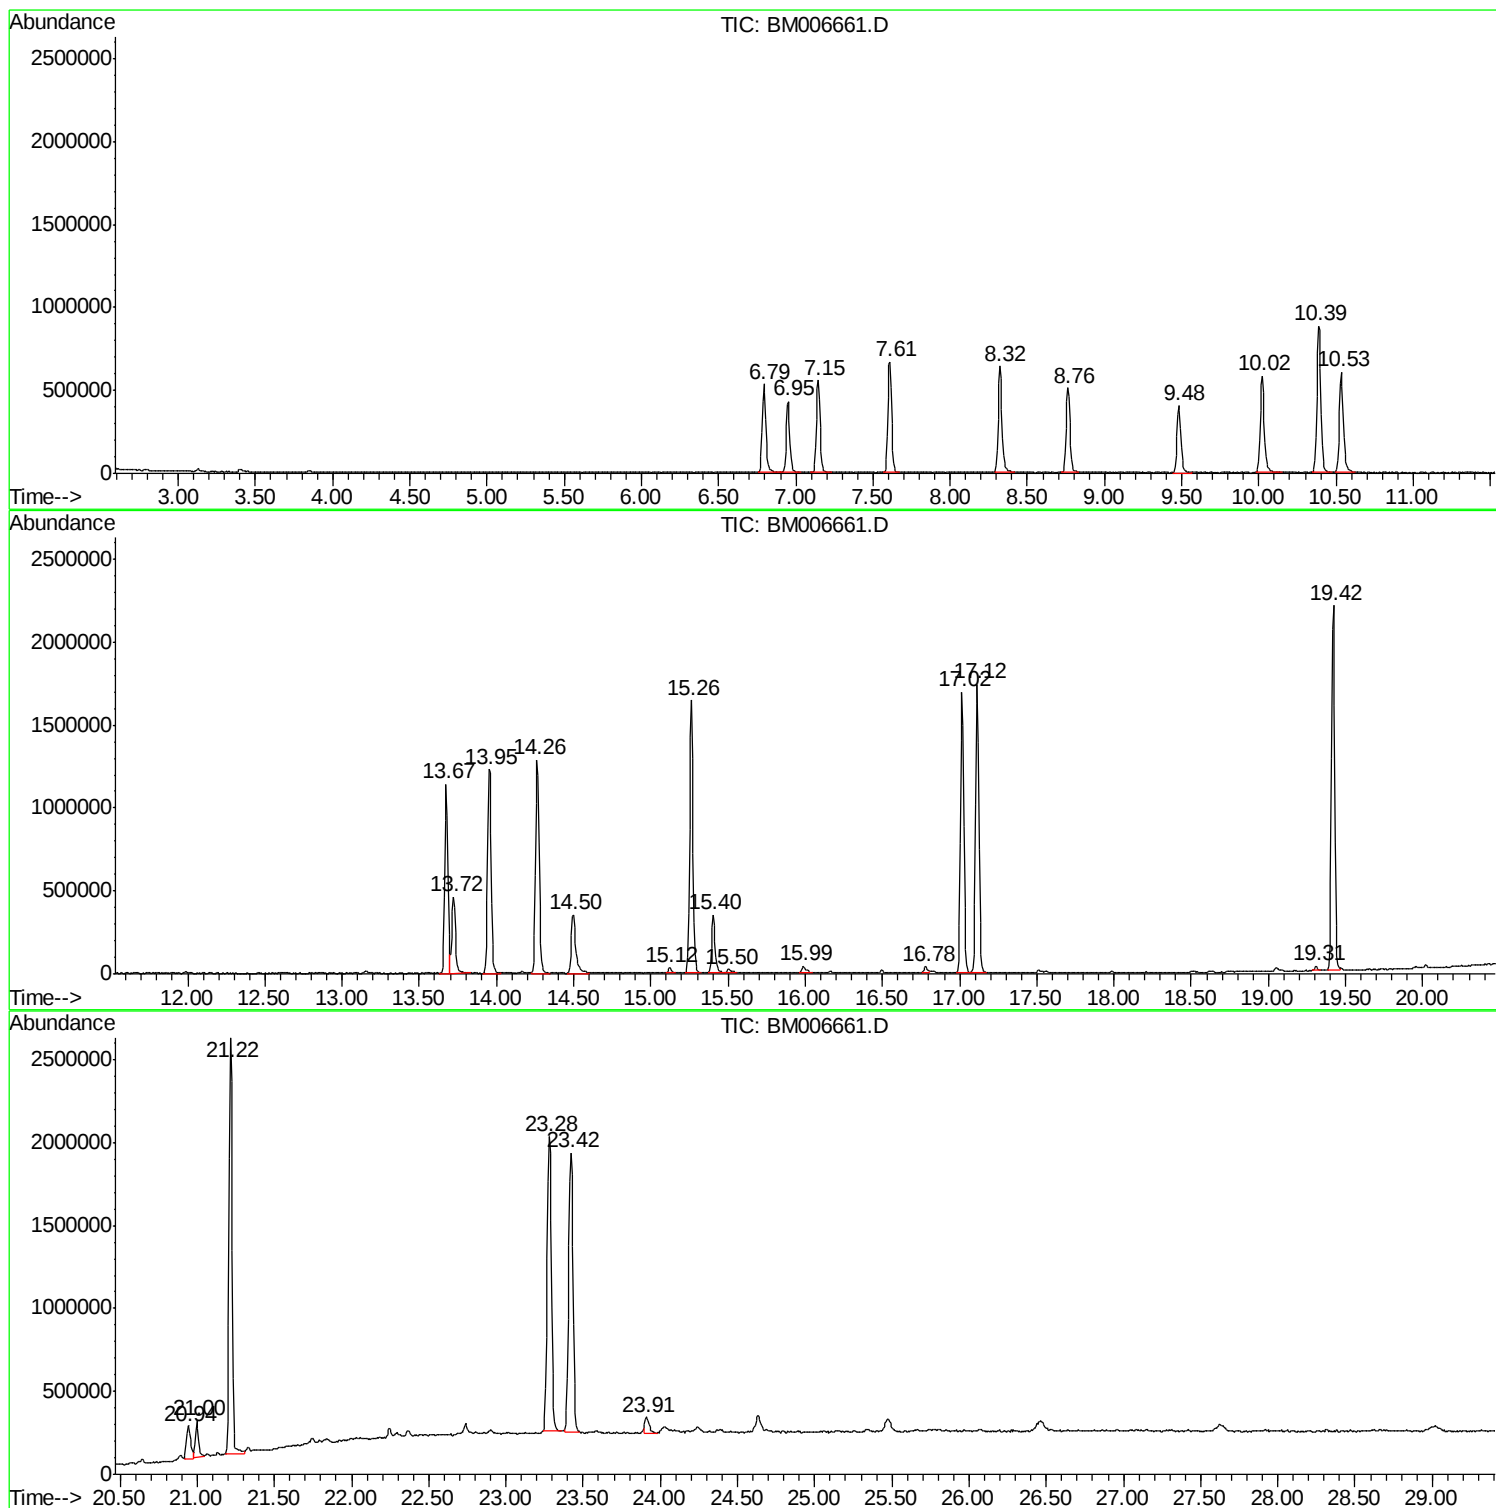

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006661.D
Acq On : 26 Jul 2016 22:10
Operator : UM/SJ
Sample : H4062-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC6










Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trichloroacetic acid, penta... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.94	2.36 ng/ul	399848	Chrysene-d12	21.22

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	93
2		1-Heneicosanol	312	C21H44O	015594-90-8	93
3		Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	93
4		n-Nonadecanol-1	284	C19H40O	001454-84-8	91
5		Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	90

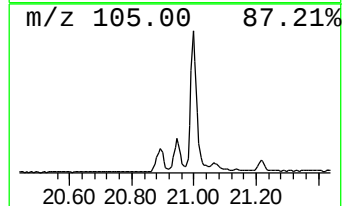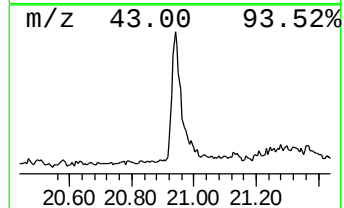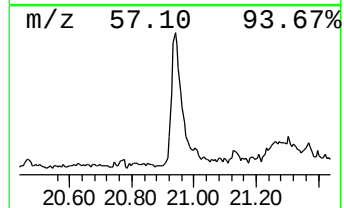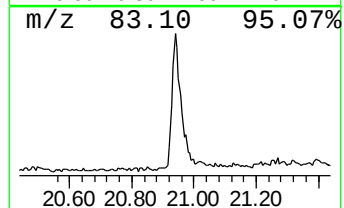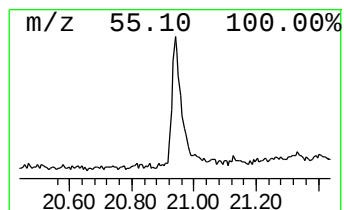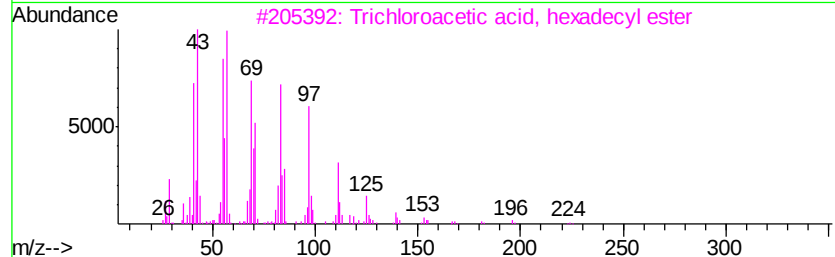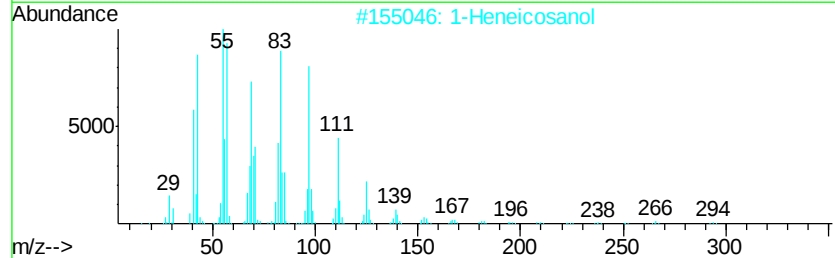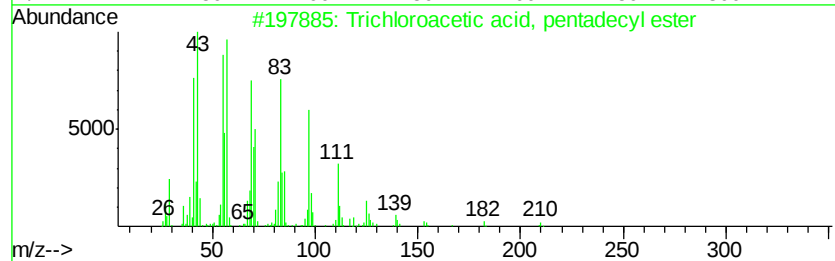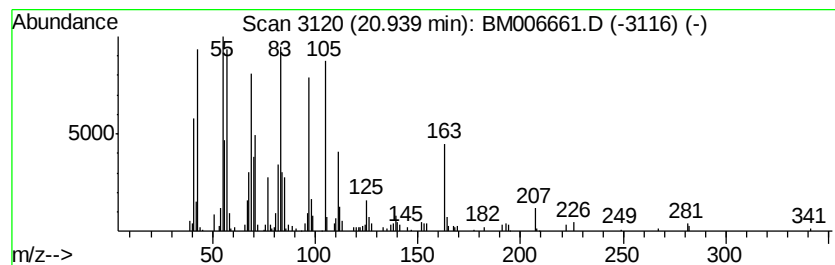

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006661.D
Acq On : 26 Jul 2016 22:10
Operator : UM/SJ
Sample : H4062-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trichloroacetic a...	20.94	2.4	ng/ul	399848	5	21.22	3390490	20.0