

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006667.D
 Acq On : 27 Jul 2016 01:47
 Operator : UM/SJ
 Sample : H4062-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJC5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.792	708	715	728	rBV	335108	570331	19.11%	2.002%
2	6.951	732	742	750	rBV	265278	434683	14.56%	1.526%
3	7.145	769	775	785	rBV	339991	568591	19.05%	1.996%
4	7.610	846	854	867	rVB	577512	974587	32.65%	3.420%
5	8.322	969	975	991	rVB	394814	672630	22.53%	2.361%
6	8.763	1043	1050	1060	rBV	313970	542562	18.18%	1.904%
7	9.480	1165	1172	1185	rBV	250808	441156	14.78%	1.548%
8	10.022	1257	1264	1278	rBV	357103	656526	22.00%	2.304%
9	10.386	1319	1326	1339	rBV	822959	1427413	47.82%	5.010%
10	10.533	1344	1351	1367	rVB	362869	687643	23.04%	2.413%
11	13.674	1878	1885	1889	rBV	693039	1010437	33.85%	3.546%
12	13.721	1889	1893	1908	rVB	287239	441449	14.79%	1.549%
13	13.951	1920	1932	1945	rBV	782534	1217724	40.80%	4.274%
14	14.262	1979	1985	1997	rBV2	1205036	1888614	63.27%	6.628%
15	14.498	2019	2025	2040	rBV	183591	389980	13.07%	1.369%
16	15.262	2148	2155	2166	rBV	1008679	1531763	51.32%	5.376%
17	15.404	2174	2179	2191	rBV	209278	317222	10.63%	1.113%
18	15.986	2274	2278	2285	rBV2	16753	30797	1.03%	0.108%
19	17.015	2447	2453	2463	rBV	1600265	2315357	77.57%	8.126%
20	17.115	2463	2470	2480	rVB	1091787	1667061	55.85%	5.851%
21	19.415	2855	2861	2877	rBV2	1359548	2020536	67.69%	7.091%
22	20.944	3116	3121	3126	rBV3	64546	116777	3.91%	0.410%
23	20.997	3126	3130	3137	rVB	123731	173467	5.81%	0.609%
24	21.215	3161	3167	3172	rBV	2270549	2984866	100.00%	10.476%
25	22.244	3340	3342	3346	rVB3	45904	44016	1.47%	0.154%
26	23.280	3511	3518	3525	rBV2	1176455	2182997	73.14%	7.661%
27	23.415	3535	3541	3552	rVB	1531165	2965447	99.35%	10.408%
28	23.909	3622	3625	3634	rVB2	120852	218484	7.32%	0.767%


Sum of corrected areas: 28493116

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006667.D
Acq On : 27 Jul 2016 01:47
Operator : UM/SJ
Sample : H4062-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

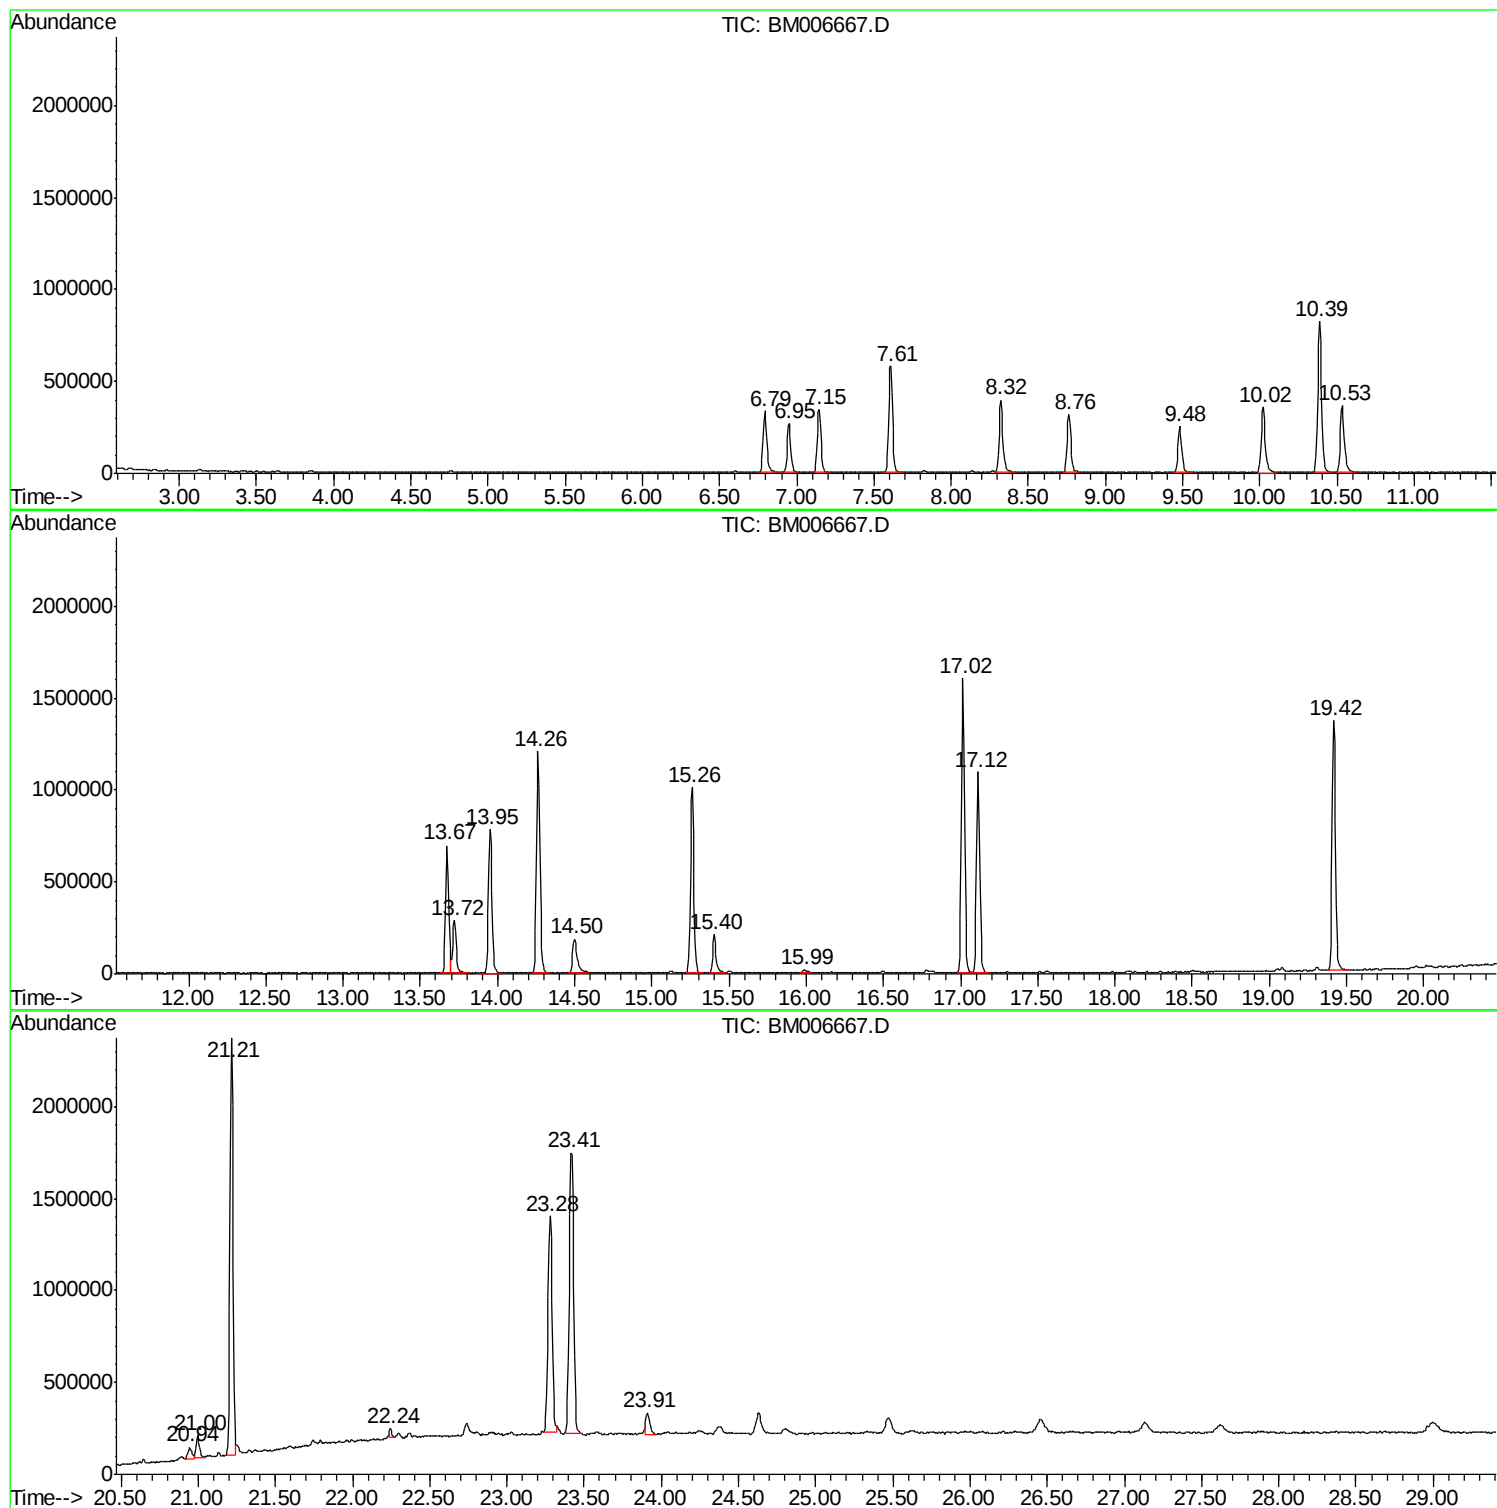

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006667.D
Acq On : 27 Jul 2016 01:47
Operator : UM/SJ
Sample : H4062-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006667.D
Acq On : 27 Jul 2016 01:47
Operator : UM/SJ
Sample : H4062-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc