

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006673.D
 Acq On : 27 Jul 2016 05:24
 Operator : UM/SJ
 Sample : H4062-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJC0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.275	453	457	466	rVB	23631	52432	1.11%	0.134%
2	6.792	710	715	727	rBV	145293	245469	5.19%	0.629%
3	6.945	735	741	755	rBV	423322	711048	15.02%	1.823%
4	7.145	768	775	787	rBV	477026	801332	16.93%	2.055%
5	7.604	847	853	864	rBV	571763	944069	19.94%	2.421%
6	8.322	969	975	992	rBV	365521	651108	13.76%	1.669%
7	8.763	1043	1050	1064	rBV	529327	918473	19.40%	2.355%
8	9.481	1164	1172	1182	rBV	439234	757439	16.00%	1.942%
9	10.016	1256	1263	1284	rBV	559004	1053074	22.25%	2.700%
10	10.386	1317	1326	1340	rBV	754472	1319655	27.88%	3.384%
11	13.674	1878	1885	1906	rBV	1135228	1713157	36.19%	4.393%
12	13.951	1925	1932	1949	rBV	1235428	1968001	41.58%	5.046%
13	14.268	1978	1986	2003	rBV2	3001434	4733584	100.00%	12.137%
14	14.498	2020	2025	2043	rBV	90551	194218	4.10%	0.498%
15	15.263	2148	2155	2166	rBV	1654766	2536934	53.59%	6.505%
16	15.404	2173	2179	2191	rBV	522482	835427	17.65%	2.142%
17	17.015	2447	2453	2463	rVV	1386839	2024967	42.78%	5.192%
18	17.115	2463	2470	2484	rVB2	1994157	3025942	63.92%	7.759%
19	19.415	2855	2861	2875	rBV	2541302	3657209	77.26%	9.377%
20	20.221	2994	2998	3004	rVB2	41262	49108	1.04%	0.126%
21	20.997	3127	3130	3138	rVB	65226	89162	1.88%	0.229%
22	21.162	3155	3158	3162	rVV	98115	113272	2.39%	0.290%
23	21.215	3162	3167	3180	rVV2	2159055	2865869	60.54%	7.348%
24	22.244	3339	3342	3346	rVB2	84082	97975	2.07%	0.251%
25	22.738	3423	3426	3431	rVB	63845	89228	1.88%	0.229%
26	23.280	3511	3518	3531	rBV2	2182282	4200621	88.74%	10.771%
27	23.421	3535	3542	3550	rVB	1516242	2914992	61.58%	7.474%
28	23.909	3621	3625	3634	rVB	107986	205233	4.34%	0.526%
29	24.633	3743	3748	3756	rVB2	109152	231659	4.89%	0.594%


Sum of corrected areas: 39000657

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006673.D
Acq On : 27 Jul 2016 05:24
Operator : UM/SJ
Sample : H4062-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

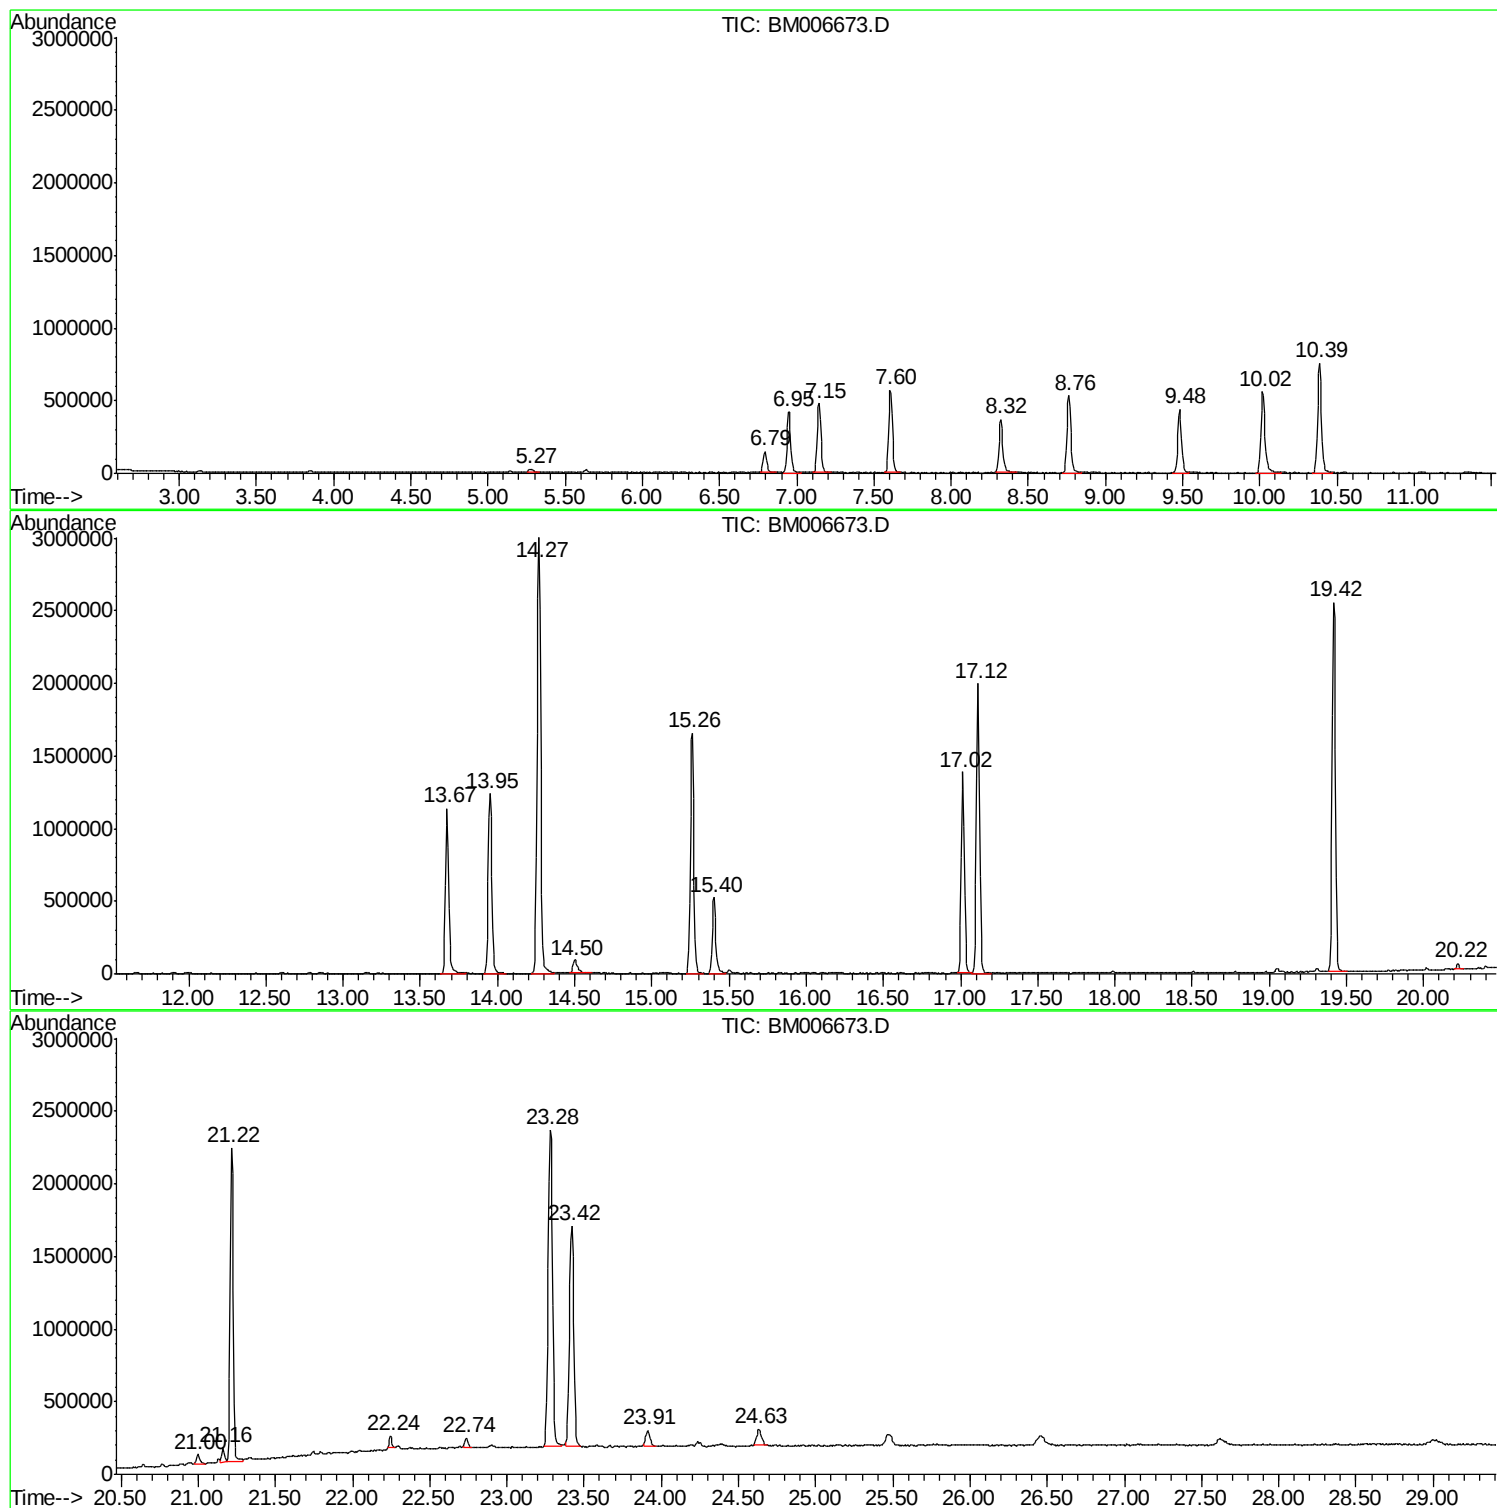

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006673.D
Acq On : 27 Jul 2016 05:24
Operator : UM/SJ
Sample : H4062-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006673.D
Acq On : 27 Jul 2016 05:24
Operator : UM/SJ
Sample : H4062-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJC0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc