

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
 Data File : BM006676.D
 Acq On : 27 Jul 2016 07:11
 Operator : UM/SJ
 Sample : H4094-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDJD6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.792	707	715	731	rBV	603266	1035269	26.20%	2.544%
2	6.945	735	741	756	rVV	480348	762813	19.31%	1.875%
3	7.139	768	774	788	rBV	615218	1021318	25.85%	2.510%
4	7.604	843	853	864	rBV	550168	913651	23.12%	2.245%
5	8.322	968	975	982	rBV	712677	1248035	31.59%	3.067%
6	8.375	982	984	994	rVB2	41065	72100	1.82%	0.177%
7	8.763	1043	1050	1069	rBV	575150	1009534	25.55%	2.481%
8	9.480	1165	1172	1188	rBV	483205	842369	21.32%	2.070%
9	10.016	1256	1263	1284	rBV	671052	1241963	31.43%	3.052%
10	10.386	1318	1326	1343	rBV	767975	1337468	33.85%	3.287%
11	10.533	1343	1351	1365	rBV	676957	1303956	33.00%	3.205%
12	13.674	1878	1885	1889	rBV	1279760	1869633	47.32%	4.595%
13	13.721	1889	1893	1906	rVB	608895	928300	23.50%	2.281%
14	13.951	1925	1932	1945	rVB	1385036	2236247	56.60%	5.496%
15	14.262	1978	1985	2001	rVB2	1059019	1748316	44.25%	4.297%
16	14.492	2018	2024	2040	rBV	369057	714147	18.07%	1.755%
17	15.257	2148	2154	2164	rBV	1843646	2798347	70.83%	6.877%
18	15.404	2173	2179	2192	rBV	425722	673399	17.04%	1.655%
19	16.774	2408	2412	2426	rBV3	23555	50225	1.27%	0.123%
20	17.015	2446	2453	2463	rBV	1435071	2151473	54.45%	5.287%
21	17.109	2463	2469	2481	rVB2	2029459	3068437	77.66%	7.541%
22	19.415	2855	2861	2876	rBV2	2598714	3692904	93.47%	9.076%
23	20.944	3116	3121	3126	rBV4	49866	105182	2.66%	0.258%
24	20.997	3126	3130	3136	rVB	63595	99204	2.51%	0.244%
25	21.215	3161	3167	3178	rBV	2175992	2877226	72.82%	7.071%
26	23.280	3510	3518	3529	rBV2	2056663	3951037	100.00%	9.710%
27	23.415	3534	3541	3549	rVB	1483662	2767960	70.06%	6.802%
28	23.903	3621	3624	3631	rVB3	89575	170249	4.31%	0.418%


Sum of corrected areas: 40690762

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006676.D
Acq On : 27 Jul 2016 07:11
Operator : UM/SJ
Sample : H4094-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJD6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

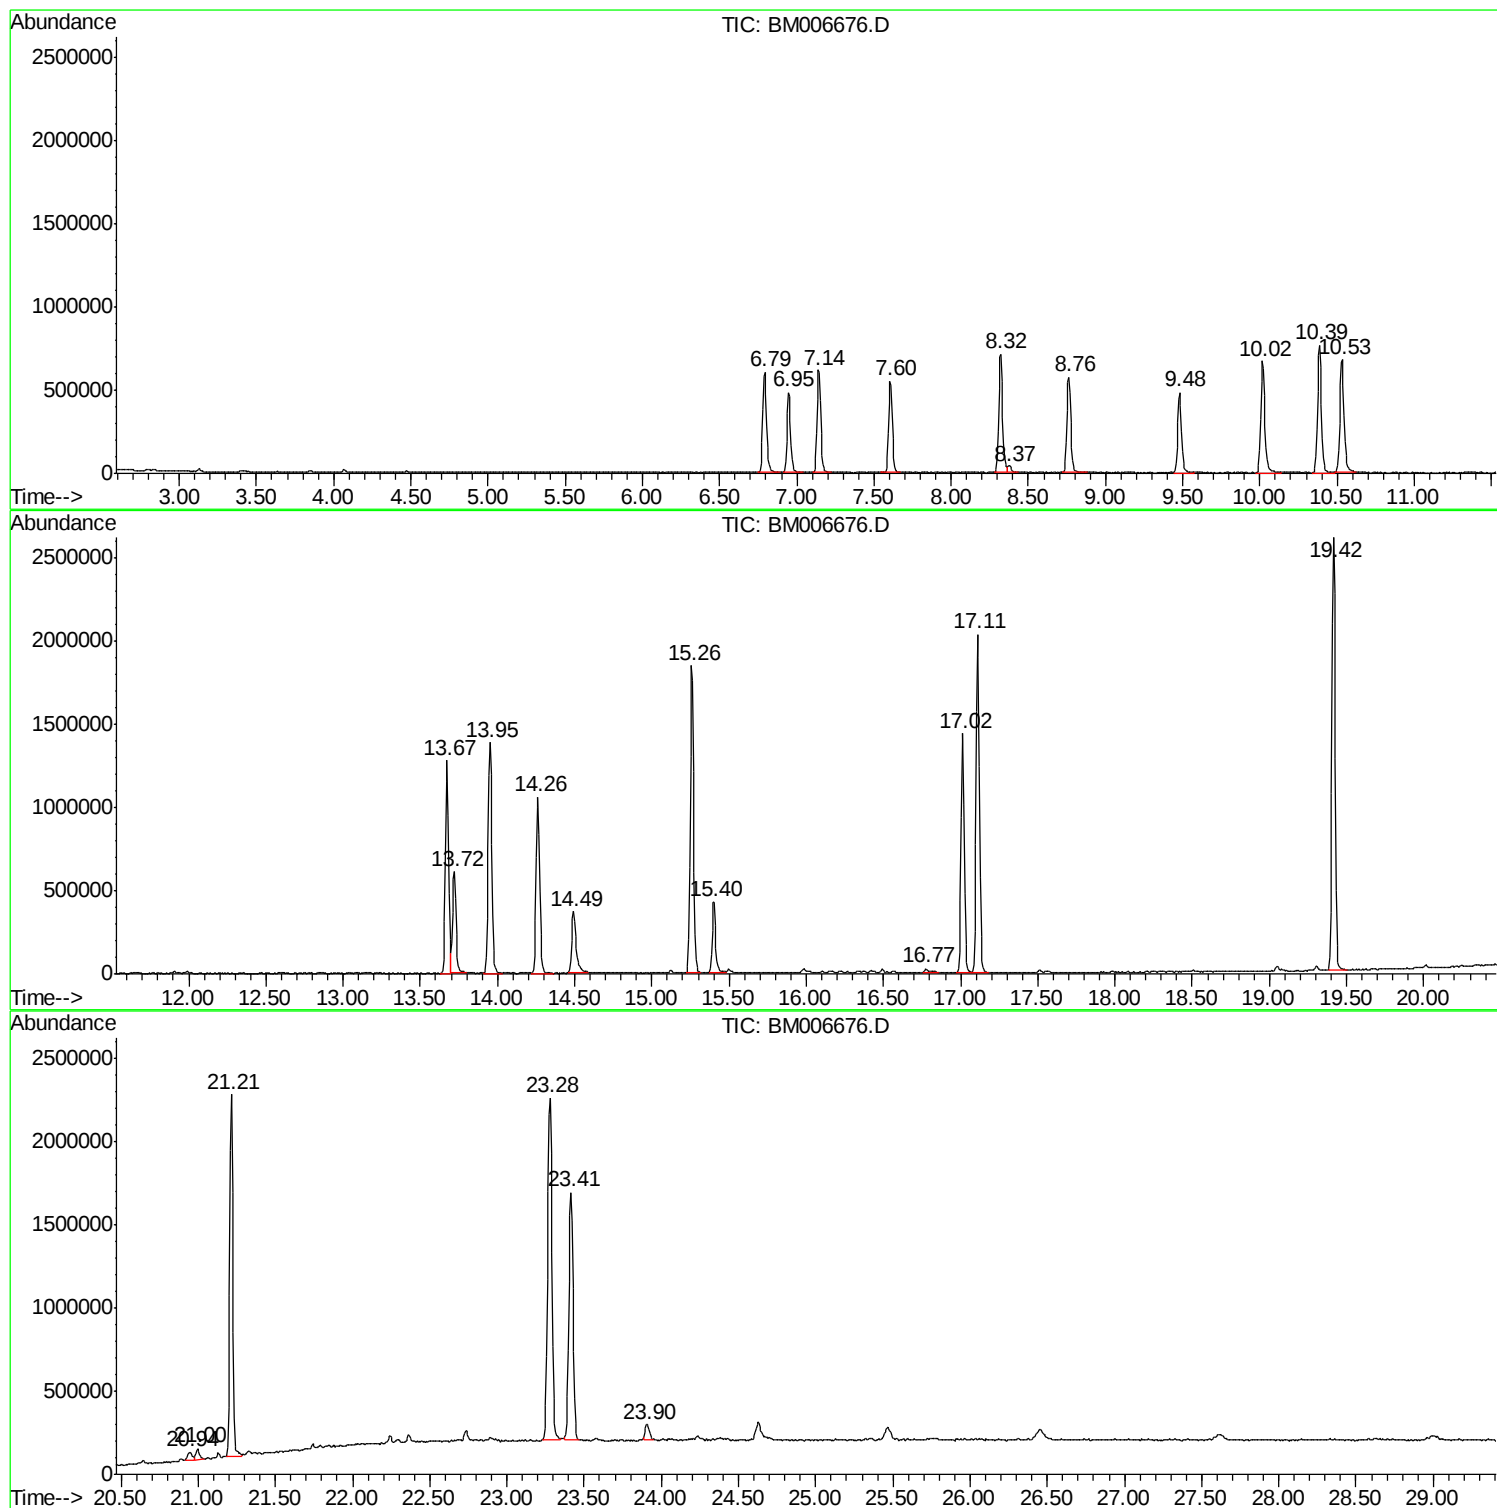

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006676.D
Acq On : 27 Jul 2016 07:11
Operator : UM/SJ
Sample : H4094-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJD6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM072616\
Data File : BM006676.D
Acq On : 27 Jul 2016 07:11
Operator : UM/SJ
Sample : H4094-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDJD6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM072616.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc