


Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM072617\  
 Data File : BM010963.D  
 Acq On : 26 Jul 2017 10:17  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampled :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_M\METHODS\8270-BM072617.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Jul 26 15:23:06 2017

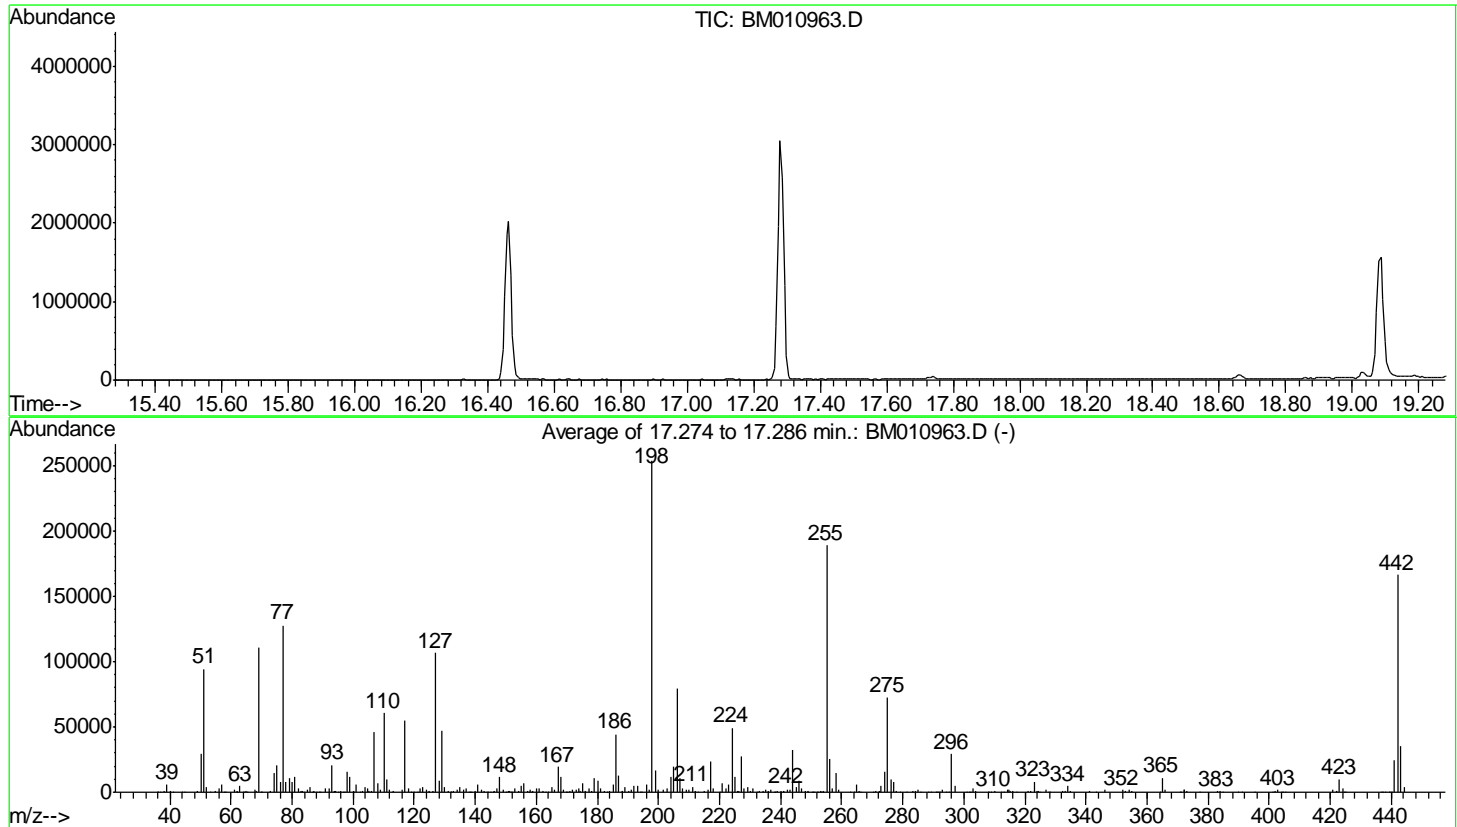

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	94413	PASS
68	69	0.00	2	1.7	1922	PASS
69	198	0.00	100	43.7	110832	PASS
70	69	0.00	2	0.2	263	PASS
127	198	10	80	42.0	106602	PASS
197	198	0.00	2	1.0	2439	PASS
198	198	100	100	100.0	253824	PASS
199	198	5	9	6.7	16940	PASS
275	198	10	60	28.4	72128	PASS
365	198	1	100	4.3	10960	PASS
441	443	0.01	100	71.4	25011	PASS
442	198	50	100	65.6	166448	PASS
443	442	15	24	21.0	35013	PASS