


Data Path : Z:\HPCHEM1\BNA M\DATA\BM072617\
 Data File : BM010981.D
 Acq On : 26 Jul 2017 21:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM072617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 26 17:29:06 2017

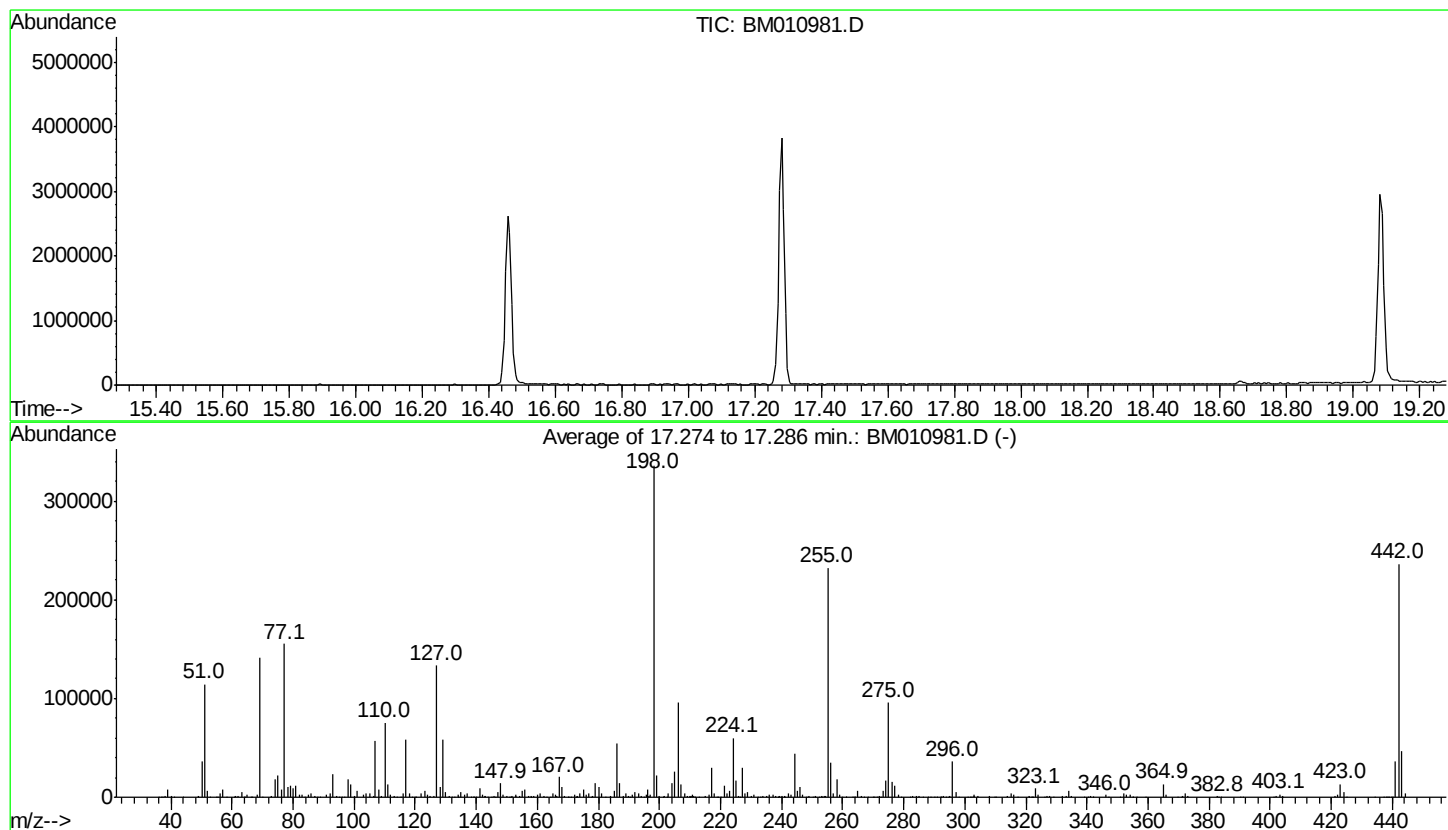

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	114290	PASS
68	69	0.00	2	1.7	2366	PASS
69	198	0.00	100	41.9	140856	PASS
70	69	0.00	2	0.5	670	PASS
127	198	10	80	39.6	133042	PASS
197	198	0.00	2	0.6	2039	PASS
198	198	100	100	100.0	335893	PASS
199	198	5	9	6.7	22357	PASS
275	198	10	60	28.5	95738	PASS
365	198	1	100	3.9	13094	PASS
441	443	0.01	100	76.9	35874	PASS
442	198	50	100	70.3	236266	PASS
443	442	15	24	19.7	46653	PASS