


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072618\
Data File : BM016074.D
Acq On : 26 Jul 2018 15:38
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 23 16:08:38 2018

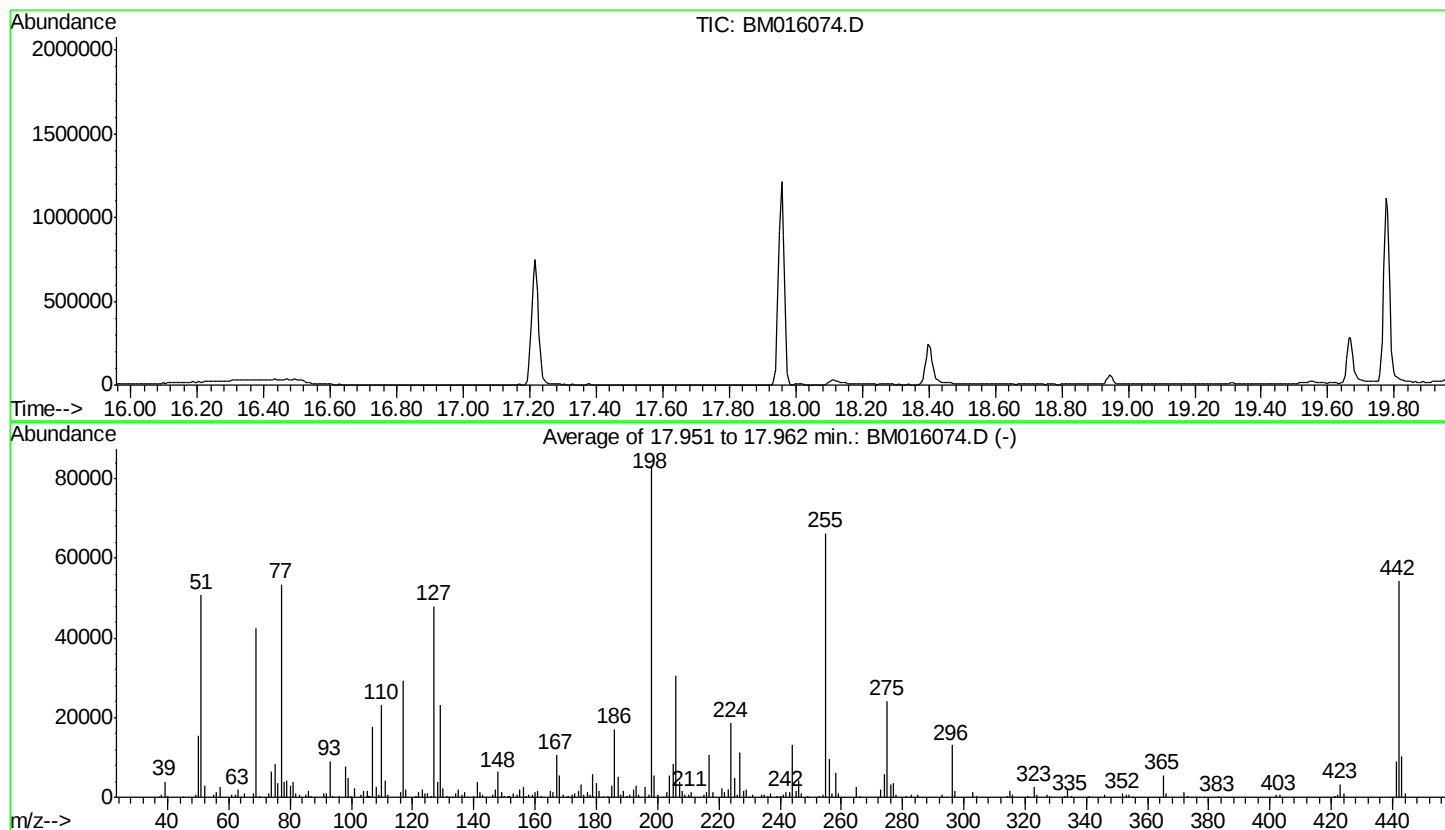

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.1	50824	PASS
68	69	0.00	2	1.9	825	PASS
69	198	0.00	100	51.0	42405	PASS
70	69	0.00	2	0.6	272	PASS
127	198	10	80	57.6	47949	PASS
197	198	0.00	2	0.8	658	PASS
198	198	100	100	100.0	83210	PASS
199	198	5	9	6.5	5368	PASS
275	198	10	60	29.1	24186	PASS
365	198	1	100	6.7	5552	PASS
441	198	0.01	100	10.8	9004	PASS
442	198	50	100	65.3	54306	PASS
443	442	15	24	19.2	10449	PASS