

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035923.D
 Acq On : 26 Jul 2022 13:22
 Operator : CG/JU
 Sample : N3801-21
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBHY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	21	26	30	rBV	434967	632970	5.07%	0.581%
2	3.699	101	104	127	rBV	484487	763740	6.11%	0.701%
3	3.940	139	145	153	rVV	45579	72006	0.58%	0.066%
4	4.034	156	161	167	rVB	34228	48118	0.39%	0.044%
5	4.569	247	252	257	rBV2	17705	28696	0.23%	0.026%
6	4.969	316	320	326	rBV2	8434	12917	0.10%	0.012%
7	5.152	346	351	357	rVB	13906	21737	0.17%	0.020%
8	5.575	418	423	429	rVB	9134	18222	0.15%	0.017%
9	7.046	664	673	681	rBV	399054	641168	5.13%	0.589%
10	7.216	693	702	716	rBV	1616241	2465751	19.73%	2.264%
11	7.410	728	735	747	rBV	1387498	2183923	17.48%	2.005%
12	7.887	807	816	823	rBV	1279503	2034764	16.28%	1.868%
13	8.593	928	936	946	rBV	1126263	1783290	14.27%	1.638%
14	9.052	1006	1014	1025	rBV	1919544	2965409	23.73%	2.723%
15	9.469	1081	1085	1089	rVB2	16292	19986	0.16%	0.018%
16	9.775	1128	1137	1152	rBV	1298314	2142561	17.14%	1.967%
17	10.310	1220	1228	1238	rBV	1944937	3156873	25.26%	2.899%
18	10.469	1250	1255	1268	rBV	125000	222355	1.78%	0.204%
19	10.693	1285	1293	1301	rBV	1853143	3107891	24.87%	2.854%
20	10.828	1307	1316	1332	rBV	1988860	3371626	26.98%	3.096%
21	11.345	1400	1404	1409	rVB2	13547	21890	0.18%	0.020%
22	11.481	1421	1427	1438	rBV3	26719	65129	0.52%	0.060%
23	11.963	1504	1509	1517	rVB2	13856	23357	0.19%	0.021%
24	12.275	1551	1562	1567	rBV2	42635	74592	0.60%	0.068%
25	12.351	1570	1575	1580	rVB6	7253	14667	0.12%	0.013%
26	12.887	1662	1666	1672	rVB2	17073	27675	0.22%	0.025%
27	13.139	1702	1709	1715	rBV	21047	31767	0.25%	0.029%
28	13.428	1753	1758	1762	rVV4	12902	20682	0.17%	0.019%
29	13.492	1766	1769	1776	rVB6	10304	15587	0.12%	0.014%
30	13.939	1838	1845	1856	rBV	4558906	6065452	48.54%	5.570%
31	14.034	1856	1861	1874	rVB3	21774	49782	0.40%	0.046%
32	14.216	1881	1892	1902	rBV	5129912	7289620	58.33%	6.694%
33	14.398	1918	1923	1927	rBV	8383	12611	0.10%	0.012%
34	14.522	1935	1944	1952	rBV	3029474	4280528	34.25%	3.931%
35	14.716	1969	1977	1986	rBV	385797	612950	4.90%	0.563%
36	14.875	1997	2004	2008	rBV6	16653	29284	0.23%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035923.D
 Acq On : 26 Jul 2022 13:22
 Operator : CG/JU
 Sample : N3801-21
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBHY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	14.939	2011	2015	2019	rVB6	13680	20383	0.16%	0.019%
38	15.322	2074	2080	2088	rBV2	69173	116549	0.93%	0.107%
39	15.510	2105	2112	2123	rBV	6988844	9432812	75.48%	8.662%
40	15.622	2125	2131	2147	rVV	1893157	2589356	20.72%	2.378%
41	15.745	2147	2152	2158	rVB2	75465	113307	0.91%	0.104%
42	16.069	2204	2207	2213	rVB8	7786	13482	0.11%	0.012%
43	16.192	2221	2228	2233	rBV4	23849	47649	0.38%	0.044%
44	16.292	2240	2245	2255	rBV6	24844	49753	0.40%	0.046%
45	16.398	2255	2263	2269	rBV10	6295	17515	0.14%	0.016%
46	16.751	2315	2323	2325	rBV7	8756	18923	0.15%	0.017%
47	16.804	2328	2332	2338	rBV9	9092	13639	0.11%	0.013%
48	16.939	2351	2355	2359	rVB5	12770	18901	0.15%	0.017%
49	17.022	2366	2369	2371	rBV4	15374	18414	0.15%	0.017%
50	17.186	2393	2397	2401	rVB6	11190	12971	0.10%	0.012%
51	17.257	2403	2409	2416	rBV	3804577	5151794	41.22%	4.731%
52	17.357	2419	2426	2438	rBV	7443164	10293531	82.37%	9.452%
53	17.545	2455	2458	2464	rVB	19198	29777	0.24%	0.027%
54	17.880	2511	2515	2518	rBV5	13072	16454	0.13%	0.015%
55	17.933	2521	2524	2526	rBV4	11315	12730	0.10%	0.012%
56	18.151	2557	2561	2568	rBV3	47352	69751	0.56%	0.064%
57	18.233	2570	2575	2579	rVV	45650	61963	0.50%	0.057%
58	18.639	2640	2644	2650	rBV6	12310	20452	0.16%	0.019%
59	19.051	2711	2714	2719	rBV7	14900	23099	0.18%	0.021%
60	19.210	2736	2741	2748	rBV	89442	131337	1.05%	0.121%
61	19.280	2748	2753	2757	rBV	97865	142948	1.14%	0.131%
62	19.433	2775	2779	2783	rBV4	32291	47335	0.38%	0.043%
63	19.586	2802	2805	2808	rVB3	24696	24626	0.20%	0.023%
64	19.651	2809	2816	2830	rBV	9604982	12496799	100.00%	11.475%
65	21.433	3114	3119	3127	rBV	4528011	5722496	45.79%	5.255%
66	23.656	3489	3497	3505	rBV2	6453302	12215516	97.75%	11.217%
67	23.809	3515	3523	3534	rVB	2888061	5627846	45.03%	5.168%




Sum of corrected areas: 108901684

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035923.D
Acq On : 26 Jul 2022 13:22
Operator : CG/JU
Sample : N3801-21
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBHY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

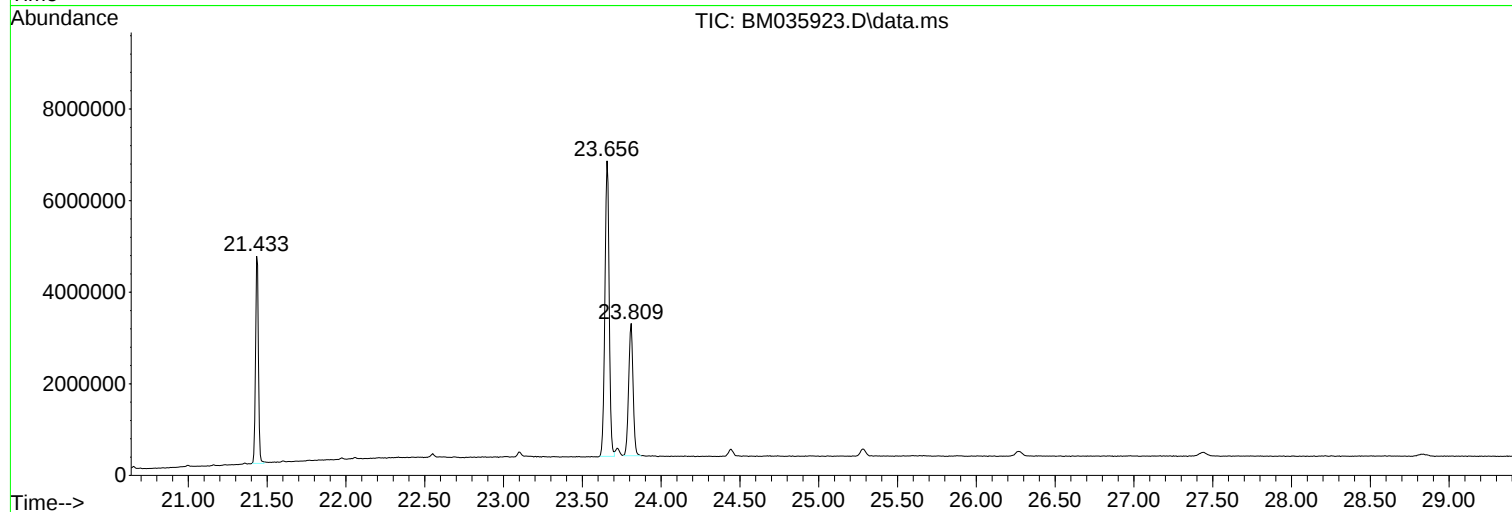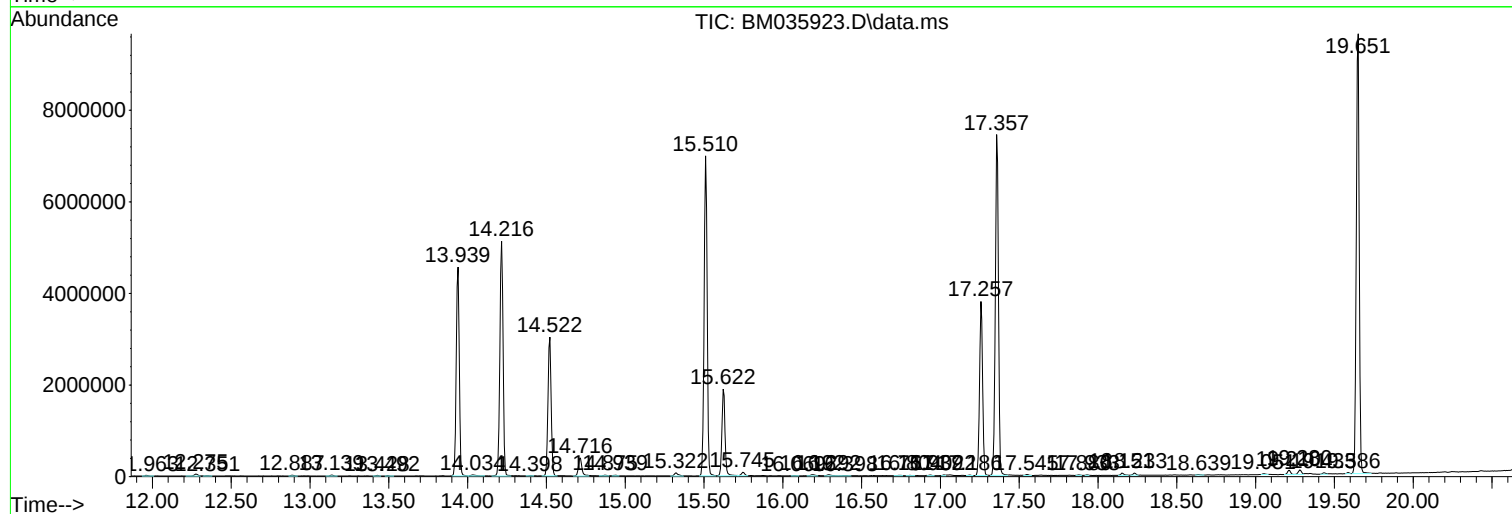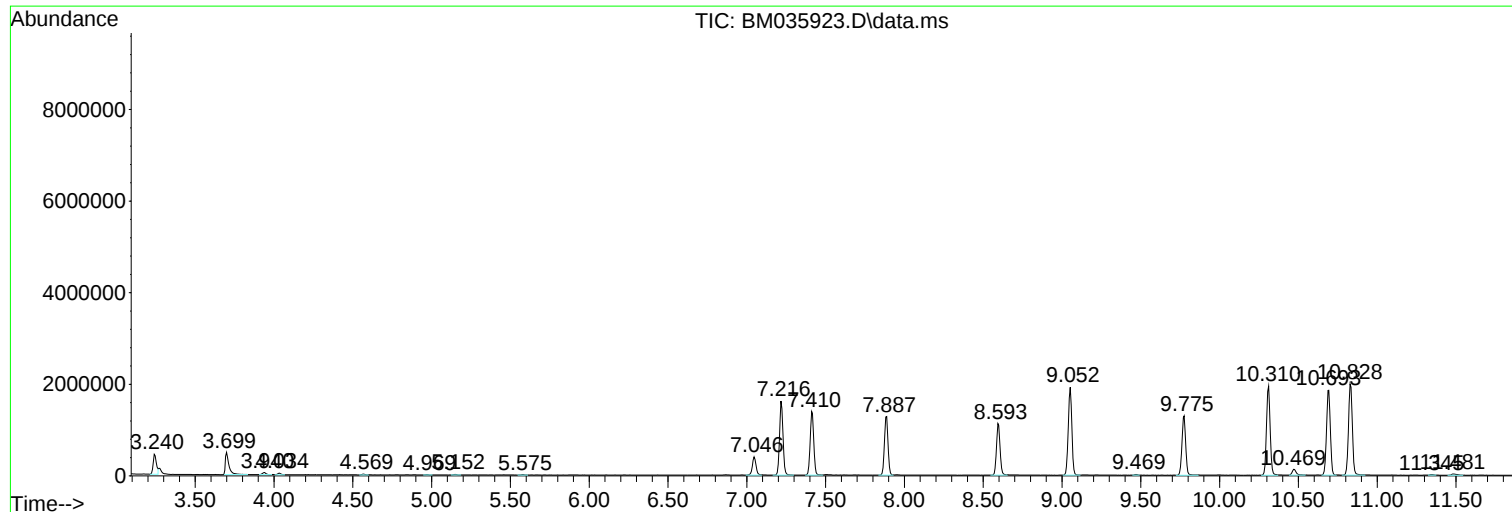

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035923.D
Acq On : 26 Jul 2022 13:22
Operator : CG/JU
Sample : N3801-21
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBHY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035923.D
Acq On : 26 Jul 2022 13:22
Operator : CG/JU
Sample : N3801-21
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBHY6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc