

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035927.D
 Acq On : 26 Jul 2022 15:51
 Operator : CG/JU
 Sample : PB146324BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK324

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	40	rVB	111307	149001	1.41%	0.143%
2	3.693	99	103	123	rBV	1427751	2111564	20.00%	2.030%
3	4.034	156	161	166	rVB	28912	40616	0.38%	0.039%
4	7.045	666	673	688	rBV	1572953	2450763	23.21%	2.356%
5	7.216	696	702	714	rVB	1386056	2186951	20.71%	2.102%
6	7.410	727	735	746	rBV	1621277	2554564	24.19%	2.455%
7	7.887	806	816	826	rBV	1217937	1906177	18.05%	1.832%
8	8.598	929	937	951	rBV	1990819	3160052	29.93%	3.037%
9	9.051	1004	1014	1024	rBV	1634342	2584243	24.47%	2.484%
10	9.775	1129	1137	1150	rBV	1208610	1955010	18.51%	1.879%
11	10.310	1220	1228	1246	rBV	1919926	3091589	29.28%	2.971%
12	10.692	1281	1293	1302	rBV	1779577	2930964	27.76%	2.817%
13	10.828	1308	1316	1330	rBV	2117184	3619499	34.28%	3.479%
14	12.274	1557	1562	1569	rBV	38599	63635	0.60%	0.061%
15	13.939	1838	1845	1856	rBV	4093566	5447173	51.59%	5.235%
16	14.216	1885	1892	1904	rBV	4558529	6367685	60.30%	6.120%
17	14.521	1937	1944	1957	rBV	2931057	4085383	38.69%	3.927%
18	14.716	1971	1977	1992	rBV	1917982	2709006	25.66%	2.604%
19	14.945	2011	2016	2024	rVB10	7988	15997	0.15%	0.015%
20	15.510	2105	2112	2125	rBV	5946557	8143552	77.12%	7.827%
21	15.627	2125	2132	2145	rVV	1615938	2286189	21.65%	2.197%
22	15.751	2147	2153	2158	rVB	63117	100973	0.96%	0.097%
23	16.292	2241	2245	2254	rVB4	21246	31751	0.30%	0.031%
24	16.939	2350	2355	2359	rBV7	10306	13292	0.13%	0.013%
25	17.027	2366	2370	2372	rBV4	7933	11712	0.11%	0.011%
26	17.256	2403	2409	2419	rBV	3545325	4908012	46.48%	4.717%
27	17.357	2419	2426	2440	rBV	6326906	8892477	84.22%	8.547%
28	17.633	2469	2473	2483	rVB4	5695	11348	0.11%	0.011%
29	18.162	2558	2563	2565	rBV6	8121	13138	0.12%	0.013%
30	19.051	2711	2714	2717	rBV5	8647	12062	0.11%	0.012%
31	19.215	2737	2742	2748	rBV	74170	107299	1.02%	0.103%
32	19.280	2749	2753	2758	rVV	67797	93189	0.88%	0.090%
33	19.439	2776	2780	2782	rBV4	8530	11995	0.11%	0.012%
34	19.650	2809	2816	2822	rBV	8272614	10559174	100.00%	10.149%
35	20.650	2984	2986	2990	rVB2	41409	41524	0.39%	0.040%
36	21.433	3114	3119	3130	rBV	4444608	5469509	51.80%	5.257%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035927.D
Acq On : 26 Jul 2022 15:51
Operator : CG/JU
Sample : PB146324BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK324

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION

37	23.656	3489	3497	3505	rBV2	5477432	10362553	98.14%	9.960%
38	23.809	3516	3523	3531	rVB2	2735679	5216401	49.40%	5.014%
39	24.444	3627	3631	3637	rVB2	179178	327293	3.10%	0.315%




Sum of corrected areas: 104043315

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035927.D
Acq On : 26 Jul 2022 15:51
Operator : CG/JU
Sample : PB146324BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

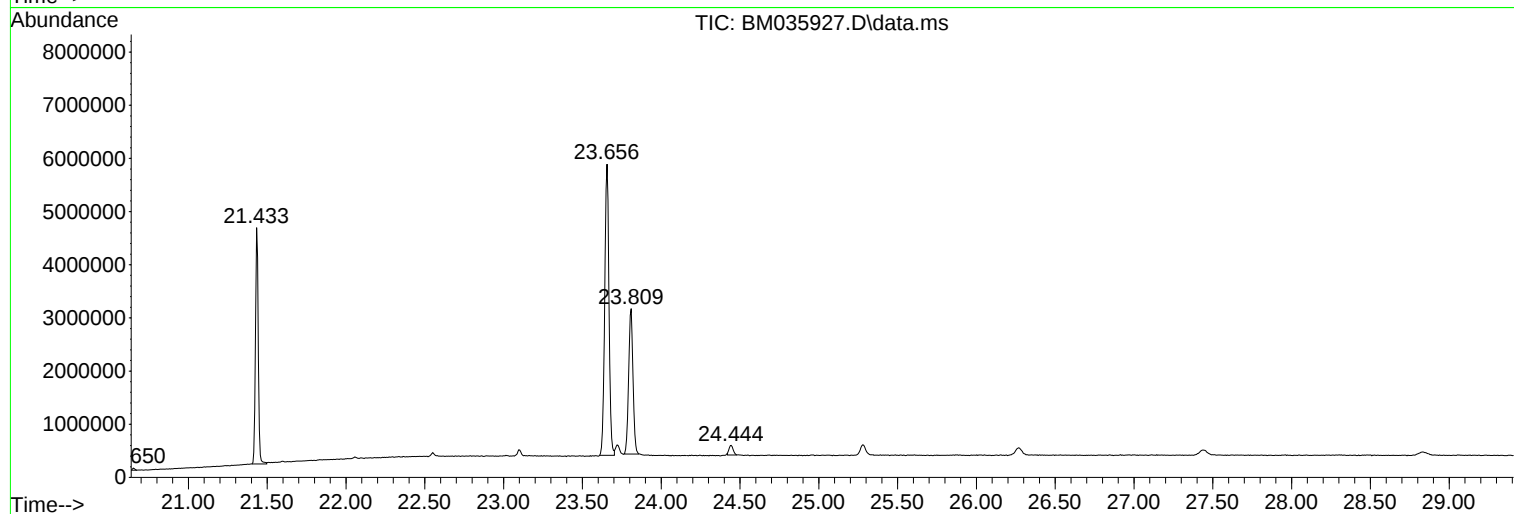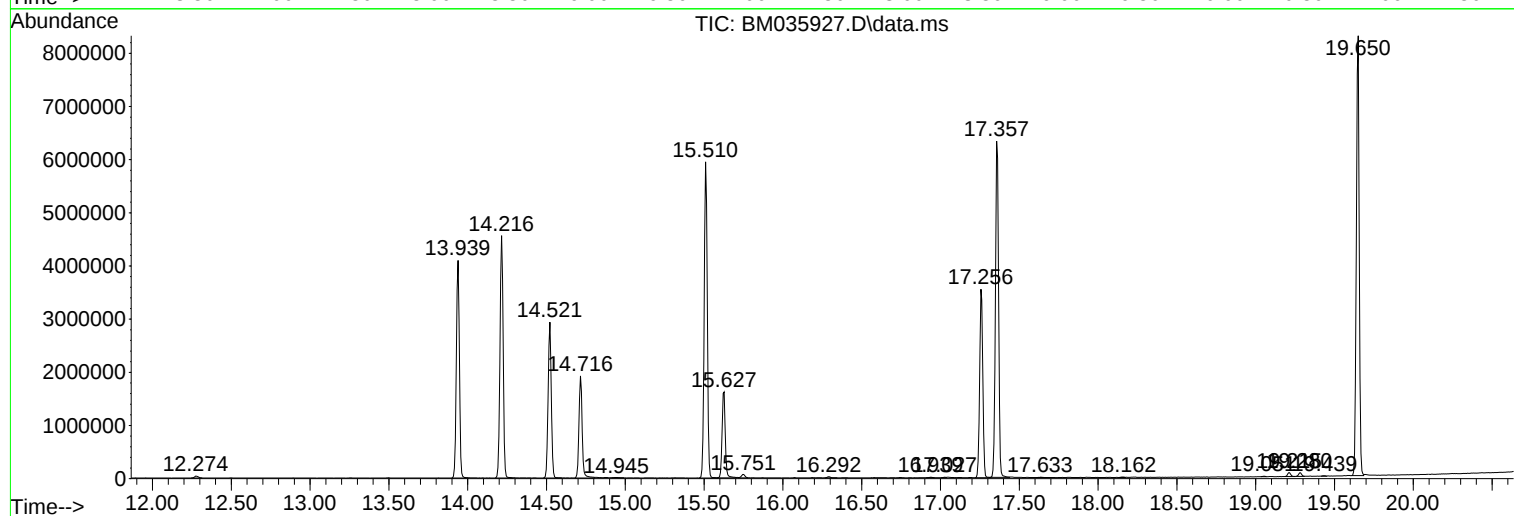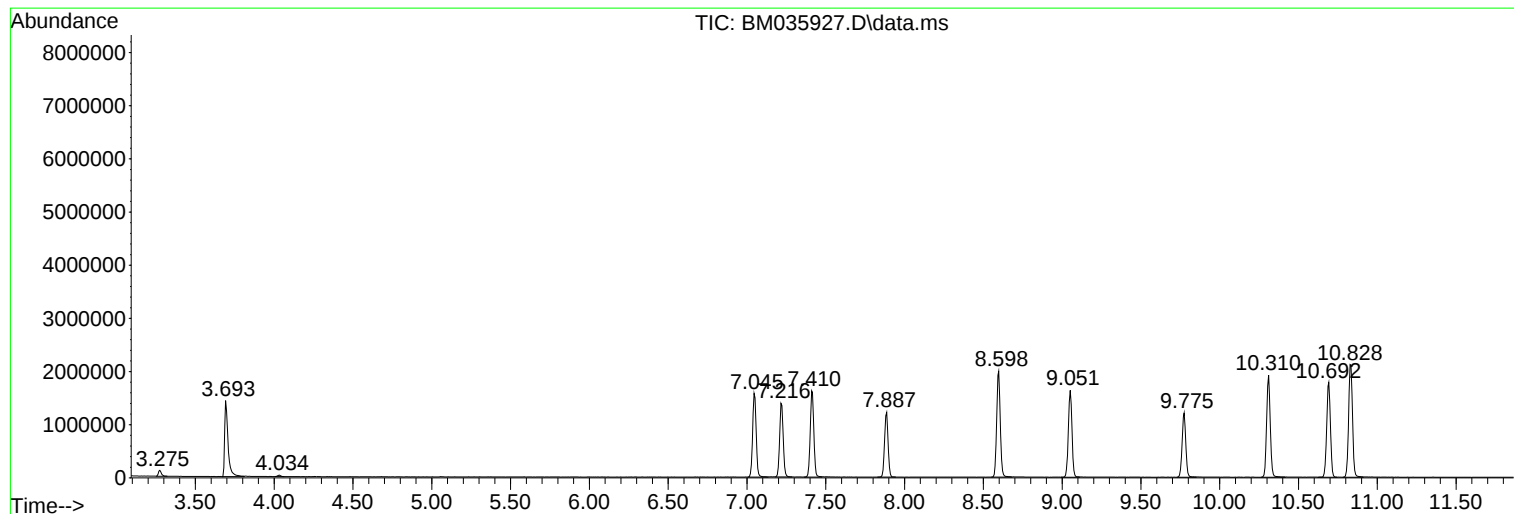

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035927.D
Acq On : 26 Jul 2022 15:51
Operator : CG/JU
Sample : PB146324BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035927.D
Acq On : 26 Jul 2022 15:51
Operator : CG/JU
Sample : PB146324BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc