

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035928.D
 Acq On : 26 Jul 2022 16:28
 Operator : CG/JU
 Sample : PB146365BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK365

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	41	rVB	120591	161707	1.41%	0.147%
2	3.693	99	103	123	rBV	1559738	2317861	20.16%	2.103%
3	4.034	156	161	167	rVB	26359	39512	0.34%	0.036%
4	7.045	667	673	689	rBV	1723580	2664403	23.17%	2.417%
5	7.216	696	702	715	rVB	1496085	2371307	20.62%	2.151%
6	7.416	727	736	748	rBV	1741033	2771093	24.10%	2.514%
7	7.887	809	816	826	rBV	1202523	1883541	16.38%	1.709%
8	8.598	929	937	952	rBV	2142037	3416335	29.71%	3.099%
9	9.051	1005	1014	1026	rBV	1811638	2812500	24.46%	2.551%
10	9.775	1129	1137	1149	rBV	1323681	2115686	18.40%	1.919%
11	10.310	1220	1228	1240	rBV	2044604	3307774	28.76%	3.001%
12	10.692	1285	1293	1304	rVB	1792595	2893072	25.16%	2.625%
13	10.833	1308	1317	1334	rBV	2322689	3925724	34.14%	3.561%
14	12.280	1558	1563	1568	rBV	38275	64300	0.56%	0.058%
15	13.939	1838	1845	1857	rBV	4411430	5854830	50.91%	5.311%
16	14.216	1884	1892	1901	rBV	4936630	6831086	59.40%	6.197%
17	14.521	1937	1944	1956	rBV	2936152	4034291	35.08%	3.660%
18	14.715	1971	1977	1997	rBV	2063458	2958877	25.73%	2.684%
19	15.510	2105	2112	2125	rBV	6407077	8776810	76.32%	7.962%
20	15.627	2125	2132	2146	rVV	1770252	2477482	21.54%	2.248%
21	15.751	2148	2153	2158	rVB	70101	104257	0.91%	0.095%
22	16.292	2241	2245	2252	rVB4	22336	32630	0.28%	0.030%
23	16.939	2352	2355	2359	rBV4	11417	13157	0.11%	0.012%
24	17.027	2364	2370	2371	rBV5	9226	13712	0.12%	0.012%
25	17.256	2403	2409	2419	rBV	3397748	4853601	42.21%	4.403%
26	17.362	2419	2427	2438	rBV	6763865	9601742	83.49%	8.711%
27	19.050	2711	2714	2718	rBV5	8135	12747	0.11%	0.012%
28	19.215	2737	2742	2747	rBV2	77366	107691	0.94%	0.098%
29	19.280	2749	2753	2761	rVV	72614	104048	0.90%	0.094%
30	19.650	2809	2816	2822	rBV	8662758	11317609	98.42%	10.267%
31	20.650	2984	2986	2990	rVB2	39551	44065	0.38%	0.040%
32	21.439	3114	3120	3129	rBV	4310293	5406394	47.01%	4.905%
33	23.656	3489	3497	3506	rBV2	6049466	11499807	100.00%	10.432%
34	23.809	3516	3523	3536	rVB2	2764753	5441932	47.32%	4.937%

Sum of corrected areas: 110231583

Instrument :

BNA_M

ClientSampleId :




SBLK365

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035928.D
Acq On : 26 Jul 2022 16:28
Operator : CG/JU
Sample : PB146365BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK365

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

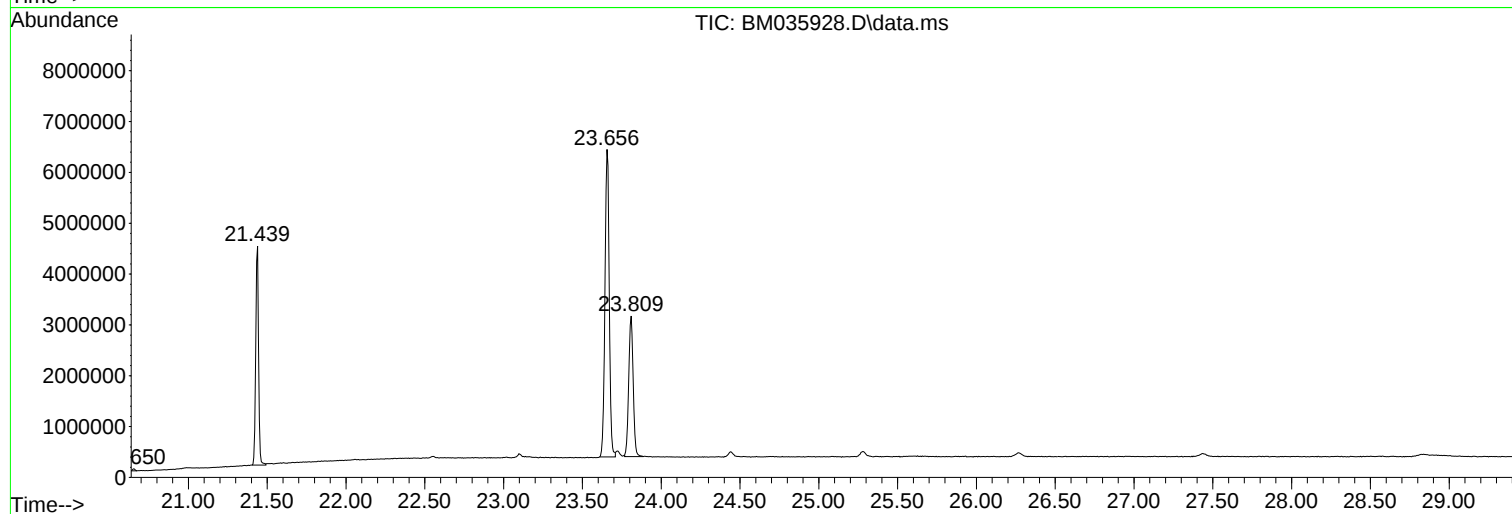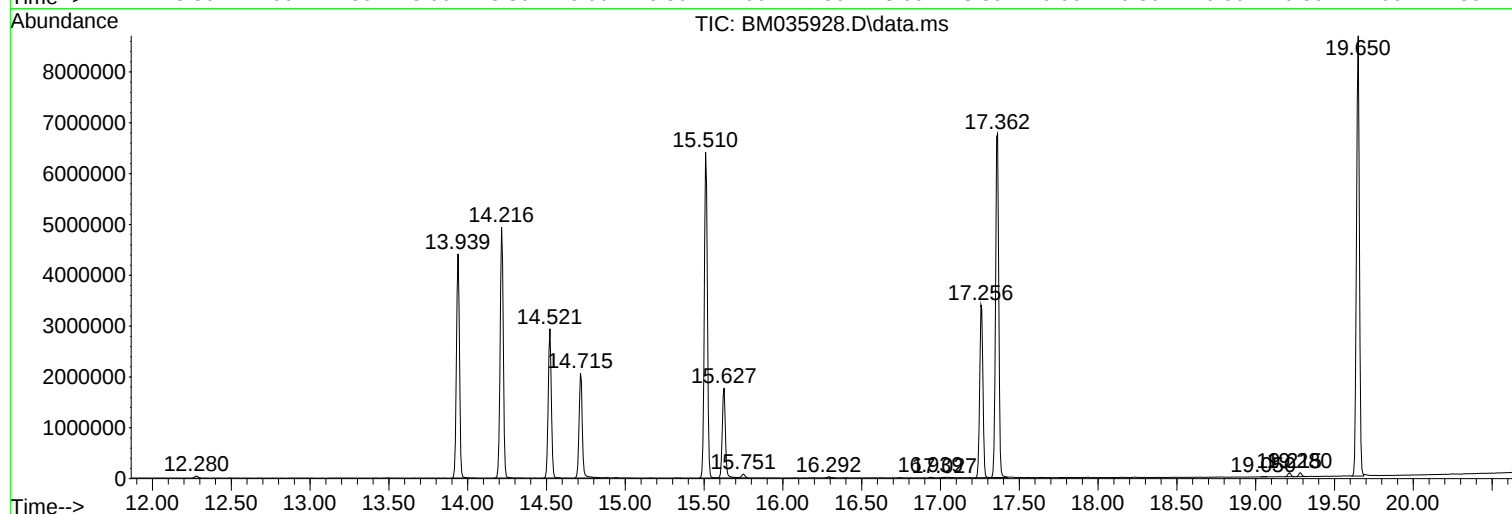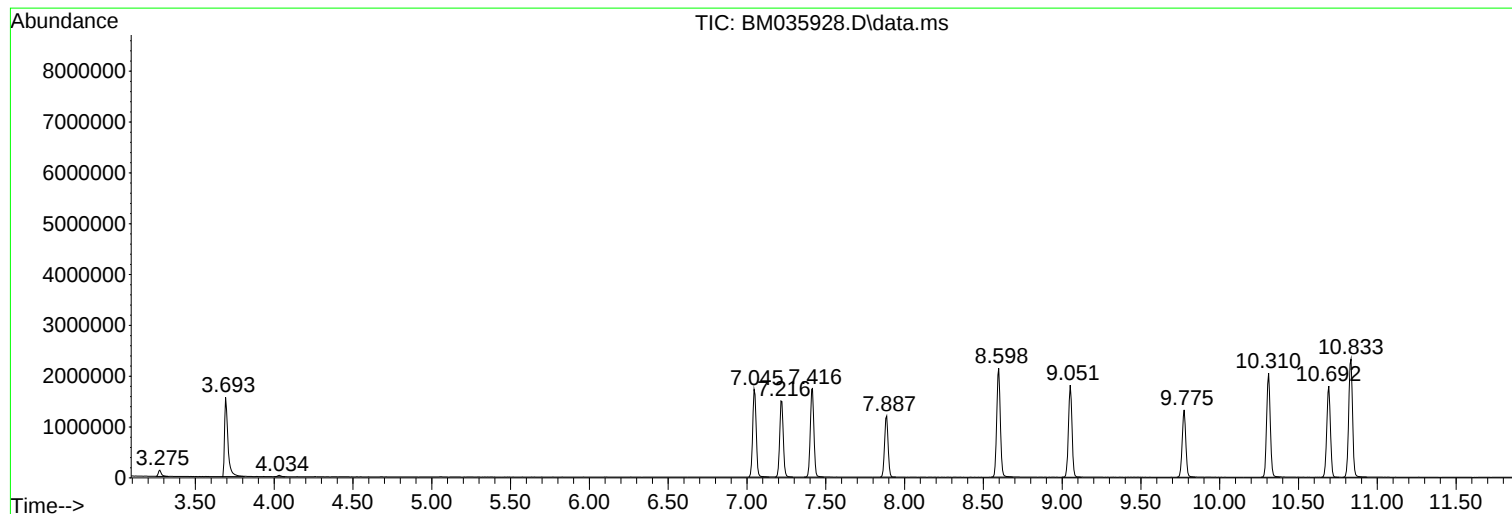

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035928.D
Acq On : 26 Jul 2022 16:28
Operator : CG/JU
Sample : PB146365BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK365

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035928.D
Acq On : 26 Jul 2022 16:28
Operator : CG/JU
Sample : PB146365BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK365

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc