

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035929.D
 Acq On : 26 Jul 2022 17:05
 Operator : CG/JU
 Sample : PB146343BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK343

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035929.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	27	32	40	rBV	111305	149421	1.49%	0.150%
2	3.693	100	103	124	rBV	1438529	2138398	21.33%	2.140%
3	4.034	156	161	168	rBV	24235	35150	0.35%	0.035%
4	4.264	197	200	207	rVB4	8236	12018	0.12%	0.012%
5	7.046	666	673	687	rBV	1618911	2481799	24.75%	2.484%
6	7.216	695	702	712	rBV	1412355	2182913	21.77%	2.184%
7	7.410	728	735	755	rBV	1627457	2563969	25.57%	2.566%
8	7.887	808	816	825	rBV	1145537	1839273	18.34%	1.841%
9	8.599	929	937	950	rBV	1991159	3148431	31.40%	3.151%
10	9.052	1006	1014	1027	rBV	1640993	2569422	25.63%	2.571%
11	9.775	1129	1137	1146	rBV	1170600	1914257	19.09%	1.916%
12	10.310	1219	1228	1244	rBV	1839679	3033953	30.26%	3.036%
13	10.693	1285	1293	1301	rBV	1688870	2806910	27.99%	2.809%
14	10.828	1308	1316	1329	rBV	2135882	3584371	35.75%	3.587%
15	12.281	1555	1563	1569	rBV2	35135	60726	0.61%	0.061%
16	13.492	1764	1769	1777	rVB6	5738	11208	0.11%	0.011%
17	13.939	1838	1845	1859	rBV	3867741	5131420	51.18%	5.135%
18	14.216	1884	1892	1901	rBV	4426496	6148150	61.32%	6.152%
19	14.522	1937	1944	1953	rBV	2777349	3892513	38.82%	3.895%
20	14.716	1970	1977	1992	rBV	1830841	2568972	25.62%	2.571%
21	15.510	2105	2112	2124	rBV	5678436	7842851	78.22%	7.848%
22	15.628	2125	2132	2148	rVV	1523763	2110597	21.05%	2.112%
23	15.751	2148	2153	2160	rVB	63725	96428	0.96%	0.096%
24	16.292	2239	2245	2255	rVB3	19419	32478	0.32%	0.033%
25	16.939	2350	2355	2359	rVB5	10481	13956	0.14%	0.014%
26	17.257	2403	2409	2418	rBV	3359169	4638444	46.26%	4.642%
27	17.357	2419	2426	2439	rVV	6161682	8416614	83.94%	8.422%
28	18.233	2570	2575	2579	rBV3	8982	11985	0.12%	0.012%
29	19.216	2737	2742	2747	rBV	69787	101930	1.02%	0.102%
30	19.280	2749	2753	2762	rVV	63739	95618	0.95%	0.096%
31	19.651	2809	2816	2822	rBV	7471447	9918613	98.92%	9.925%
32	20.651	2984	2986	2990	rVB2	35585	36571	0.36%	0.037%
33	21.433	3114	3119	3128	rBV	4066244	5155068	51.41%	5.159%
34	23.656	3489	3497	3504	rBV2	5324208	10026933	100.00%	10.034%
35	23.809	3516	3523	3535	rVB2	2602697	5159669	51.46%	5.163%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035929.D
Acq On : 26 Jul 2022 17:05
Operator : CG/JU
Sample : PB146343BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK343

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 99931029

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035929.D
Acq On : 26 Jul 2022 17:05
Operator : CG/JU
Sample : PB146343BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK343

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

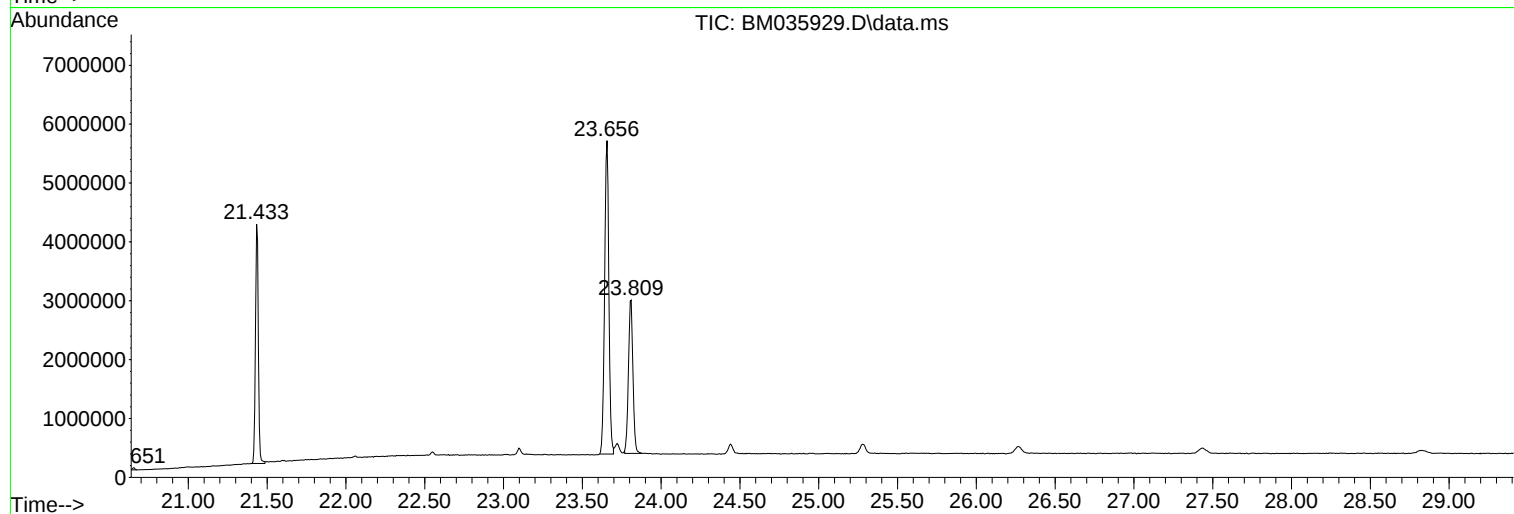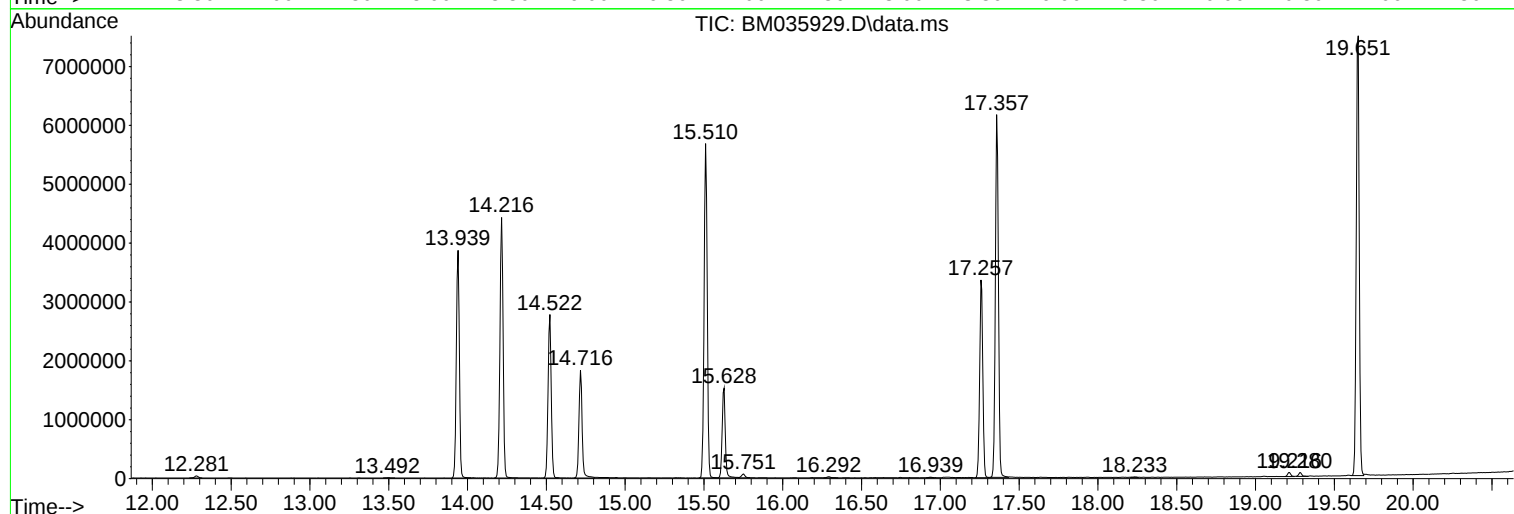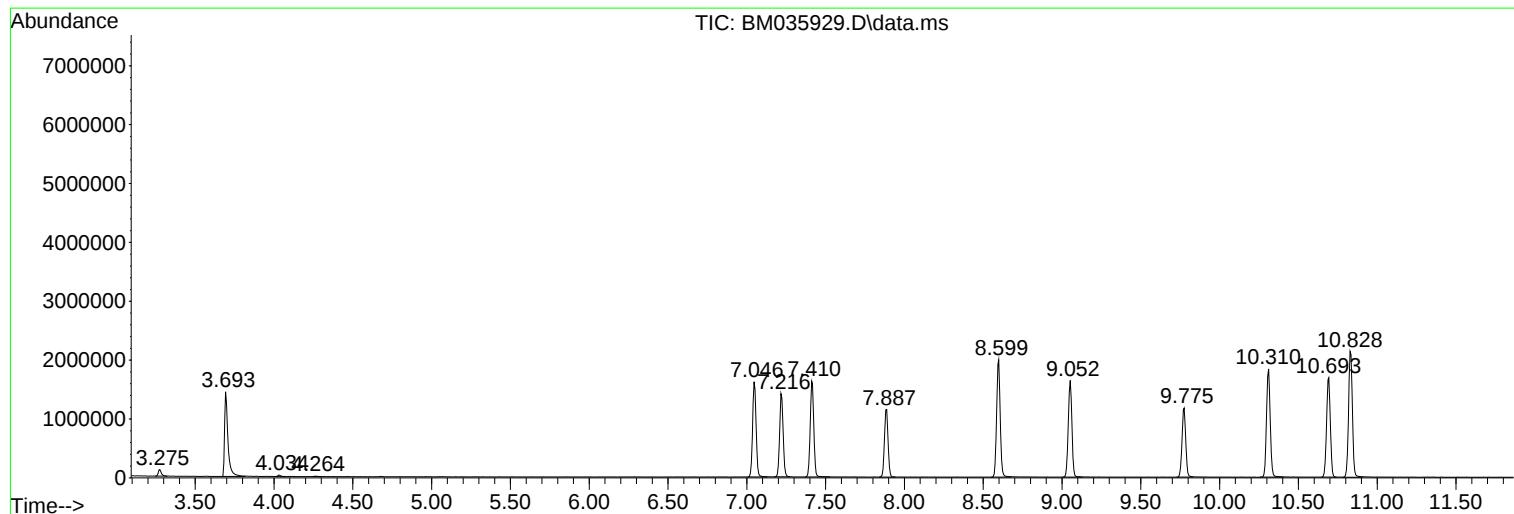

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035929.D
Acq On : 26 Jul 2022 17:05
Operator : CG/JU
Sample : PB146343BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK343

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035929.D
Acq On : 26 Jul 2022 17:05
Operator : CG/JU
Sample : PB146343BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK343

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------