

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035930.D
 Acq On : 26 Jul 2022 17:42
 Operator : CG/JU
 Sample : PB146378BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK378

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035930.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	27	32	40	rVB	106499	142610	1.44%	0.148%
2	3.693	99	103	127	rBV	1368901	2046661	20.60%	2.127%
3	4.034	156	161	168	rVB	22533	33635	0.34%	0.035%
4	4.263	196	200	205	rVB7	9620	13631	0.14%	0.014%
5	7.045	667	673	685	rBV	1537362	2372030	23.87%	2.465%
6	7.216	695	702	713	rBV	1357133	2090710	21.04%	2.173%
7	7.410	728	735	747	rBV	1542108	2434510	24.50%	2.530%
8	7.887	809	816	826	rVB	1080257	1706630	17.18%	1.774%
9	8.598	929	937	950	rBV	1937535	3029877	30.49%	3.149%
10	9.051	1005	1014	1023	rBV	1560097	2445581	24.61%	2.542%
11	9.775	1126	1137	1150	rBV	1143117	1834987	18.47%	1.907%
12	10.310	1220	1228	1245	rBV	1786614	2933488	29.52%	3.049%
13	10.692	1284	1293	1301	rBV	1624571	2642179	26.59%	2.746%
14	10.833	1309	1317	1329	rBV	2027782	3421300	34.43%	3.556%
15	12.275	1557	1562	1569	rVB2	33606	54686	0.55%	0.057%
16	13.939	1838	1845	1857	rBV	3602816	4906709	49.38%	5.100%
17	14.216	1885	1892	1905	rBV	4275023	5871518	59.09%	6.102%
18	14.521	1937	1944	1954	rBV	2636379	3658754	36.82%	3.803%
19	14.716	1970	1977	1997	rBV	1789806	2472501	24.88%	2.570%
20	14.874	2002	2004	2011	rVB8	5402	10994	0.11%	0.011%
21	15.510	2105	2112	2125	rBV	5526274	7504801	75.53%	7.800%
22	15.627	2125	2132	2148	rVV	1394858	2013434	20.26%	2.093%
23	15.751	2148	2153	2163	rVB	61319	97557	0.98%	0.101%
24	16.292	2240	2245	2250	rBV4	17827	28046	0.28%	0.029%
25	16.939	2351	2355	2360	rVB6	8138	10862	0.11%	0.011%
26	17.021	2365	2369	2371	rBV3	8909	12122	0.12%	0.013%
27	17.257	2403	2409	2419	rBV	3191865	4389817	44.18%	4.562%
28	17.357	2419	2426	2440	rBV	5839177	8132596	81.85%	8.452%
29	17.933	2520	2524	2528	rVB7	8151	12194	0.12%	0.013%
30	19.215	2737	2742	2748	rVB	66127	91034	0.92%	0.095%
31	19.280	2748	2753	2759	rBV	61873	93852	0.94%	0.098%
32	19.645	2809	2815	2828	rBV	7218399	9731622	97.94%	10.114%
33	20.650	2983	2986	2990	rBV	39660	46163	0.46%	0.048%
34	21.433	3114	3119	3129	rBV	4097225	4997881	50.30%	5.194%
35	23.656	3489	3497	3504	rBV	5203872	9936576	100.00%	10.327%
36	23.803	3515	3522	3532	rVB2	2567193	4996552	50.28%	5.193%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035930.D
Acq On : 26 Jul 2022 17:42
Operator : CG/JU
Sample : PB146378BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 96218100

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035930.D
Acq On : 26 Jul 2022 17:42
Operator : CG/JU
Sample : PB146378BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

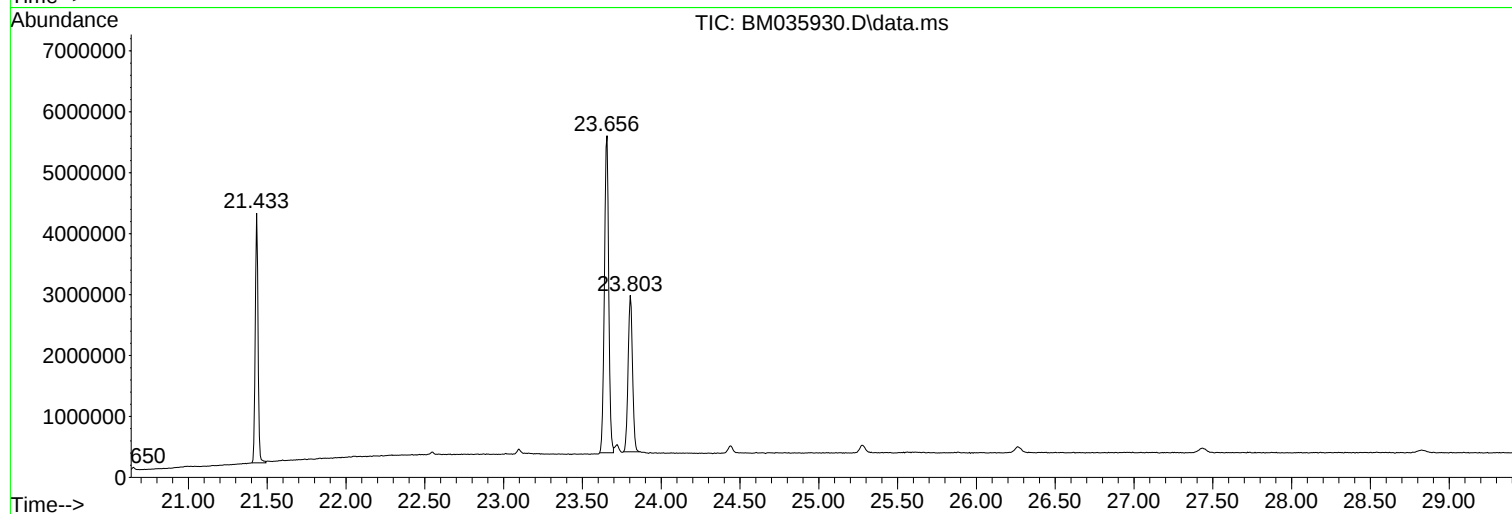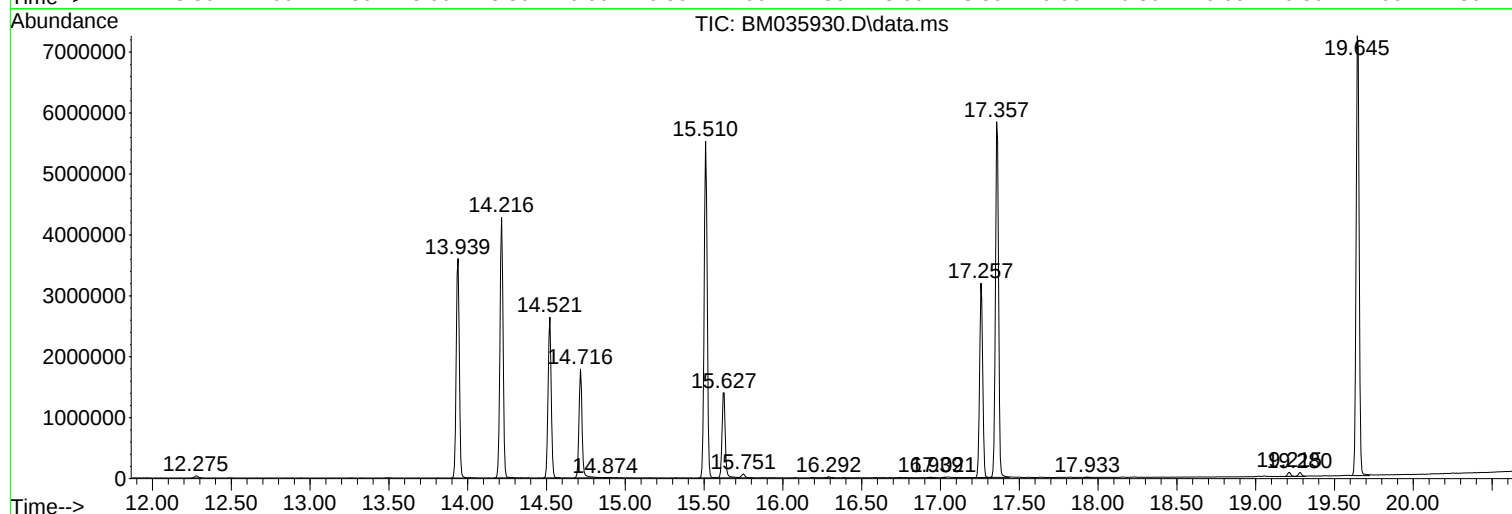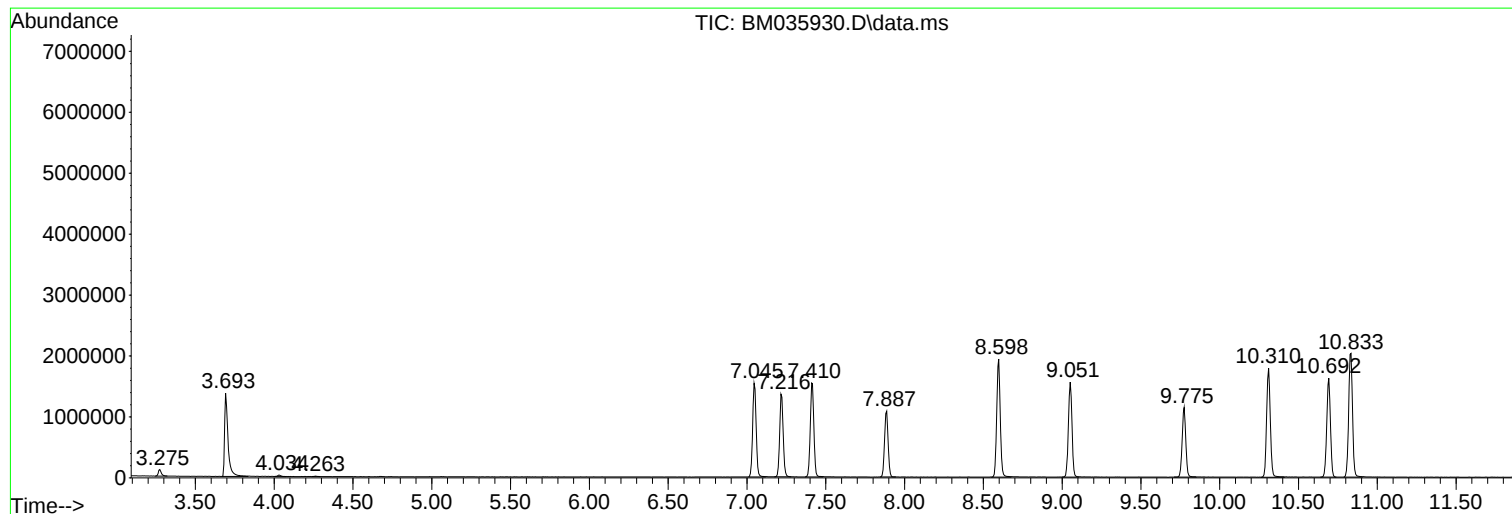

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035930.D
Acq On : 26 Jul 2022 17:42
Operator : CG/JU
Sample : PB146378BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035930.D
Acq On : 26 Jul 2022 17:42
Operator : CG/JU
Sample : PB146378BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK378

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------