

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035931.D
 Acq On : 26 Jul 2022 18:19
 Operator : CG/JU
 Sample : N3792-15
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	38	rVB	76117	97517	0.88%	0.108%
2	3.569	79	82	89	rVB3	8552	15467	0.14%	0.017%
3	3.699	101	104	121	rBV	295919	468568	4.21%	0.518%
4	3.934	139	144	150	rVB	33189	50948	0.46%	0.056%
5	4.028	157	160	165	rVB	22031	29971	0.27%	0.033%
6	5.575	419	423	427	rBV	8840	13381	0.12%	0.015%
7	6.875	638	644	654	rBV2	34257	61983	0.56%	0.068%
8	7.045	665	673	682	rBV	305758	485845	4.36%	0.537%
9	7.216	695	702	712	rBV	1390676	2156268	19.36%	2.382%
10	7.410	727	735	747	rBV	1188792	1888174	16.95%	2.086%
11	7.886	809	816	823	rBV	991448	1536833	13.80%	1.698%
12	8.457	906	913	922	rBV7	10679	25088	0.23%	0.028%
13	8.598	929	937	949	rBV	914651	1489416	13.37%	1.646%
14	9.051	1006	1014	1025	rBV	1658305	2556068	22.94%	2.824%
15	9.169	1028	1034	1039	rVV2	36585	61491	0.55%	0.068%
16	9.216	1039	1042	1051	rVB9	6901	12838	0.12%	0.014%
17	9.775	1129	1137	1150	rBV	1149412	1830493	16.43%	2.022%
18	9.916	1156	1161	1166	rBV3	17338	32549	0.29%	0.036%
19	10.004	1171	1176	1182	rBV2	24345	41246	0.37%	0.046%
20	10.310	1219	1228	1241	rBV	1707271	2746412	24.65%	3.034%
21	10.486	1251	1258	1261	rBV7	7237	14713	0.13%	0.016%
22	10.692	1285	1293	1301	rBV	1459427	2363748	21.22%	2.611%
23	10.833	1306	1317	1329	rBV	1498507	2566887	23.04%	2.836%
24	11.345	1401	1404	1410	rVB2	7418	11281	0.10%	0.012%
25	11.486	1422	1428	1436	rBV	35091	67069	0.60%	0.074%
26	12.280	1557	1563	1570	rVB	33249	55165	0.50%	0.061%
27	12.886	1660	1666	1671	rBV	18700	28016	0.25%	0.031%
28	13.139	1703	1709	1714	rVB4	16838	26282	0.24%	0.029%
29	13.492	1765	1769	1775	rVB6	8304	12855	0.12%	0.014%
30	13.939	1838	1845	1857	rVV	3894484	5180994	46.51%	5.724%
31	14.215	1885	1892	1899	rBV	4516105	6089897	54.67%	6.728%
32	14.521	1936	1944	1956	rBV	2312580	3257707	29.24%	3.599%
33	14.715	1968	1977	1987	rBV	272928	443281	3.98%	0.490%
34	14.933	2010	2014	2020	rVB7	15309	25153	0.23%	0.028%
35	15.321	2075	2080	2087	rBV2	55339	86402	0.78%	0.095%
36	15.510	2105	2112	2122	rBV	6015613	8080633	72.54%	8.928%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035931.D
 Acq On : 26 Jul 2022 18:19
 Operator : CG/JU
 Sample : N3792-15
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUN8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.627	2125	2132	2147	rVV	1494913	2111252	18.95%	2.333%
38	15.751	2148	2153	2161	rVB	64905	100951	0.91%	0.112%
39	16.198	2223	2229	2231	rBV5	7124	12714	0.11%	0.014%
40	16.292	2241	2245	2254	rVB4	21607	36574	0.33%	0.040%
41	16.392	2257	2262	2270	rBV10	6895	17891	0.16%	0.020%
42	16.939	2352	2355	2361	rVB8	8625	11256	0.10%	0.012%
43	17.021	2364	2369	2373	rBV5	15313	25955	0.23%	0.029%
44	17.139	2385	2389	2394	rBV3	13398	20797	0.19%	0.023%
45	17.256	2402	2409	2417	rBV	2843973	3923371	35.22%	4.335%
46	17.356	2420	2426	2437	rBV	6105553	8333659	74.81%	9.207%
47	17.821	2500	2505	2510	rVB8	6630	13587	0.12%	0.015%
48	17.939	2520	2525	2531	rVB	54371	68038	0.61%	0.075%
49	18.156	2558	2562	2565	rBV	94769	119889	1.08%	0.132%
50	18.192	2565	2568	2571	rVV	41411	57566	0.52%	0.064%
51	18.233	2571	2575	2580	rVB	35629	50446	0.45%	0.056%
52	18.486	2614	2618	2621	rVB4	11700	15980	0.14%	0.018%
53	18.639	2640	2644	2649	rBV2	21038	31269	0.28%	0.035%
54	19.050	2710	2714	2719	rBV8	13069	22282	0.20%	0.025%
55	19.209	2737	2741	2746	rBV	75648	100587	0.90%	0.111%
56	19.280	2749	2753	2757	rBV	84058	113925	1.02%	0.126%
57	19.350	2762	2765	2770	rVB5	14625	19378	0.17%	0.021%
58	19.433	2775	2779	2784	rBV3	42041	58741	0.53%	0.065%
59	19.586	2802	2805	2809	rVB4	19197	18133	0.16%	0.020%
60	19.650	2809	2816	2822	rBV	8035769	10711287	96.15%	11.834%
61	20.650	2984	2986	2989	rVB2	41470	37803	0.34%	0.042%
62	21.150	3068	3071	3079	rBV3	112547	159991	1.44%	0.177%
63	21.433	3114	3119	3128	rBV	3844724	4525252	40.62%	5.000%
64	23.656	3489	3497	3504	rBV2	5869171	11140316	100.00%	12.308%
65	23.803	3515	3522	3540	rVB2	2426179	4743597	42.58%	5.241%




Sum of corrected areas: 90513126

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035931.D
Acq On : 26 Jul 2022 18:19
Operator : CG/JU
Sample : N3792-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

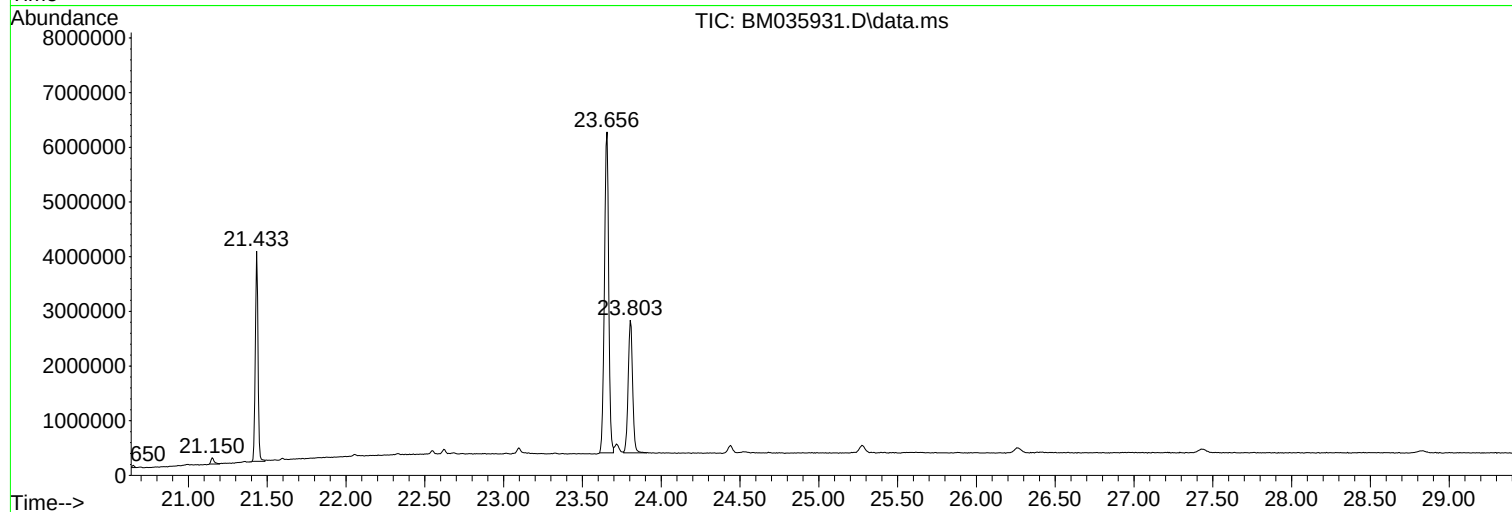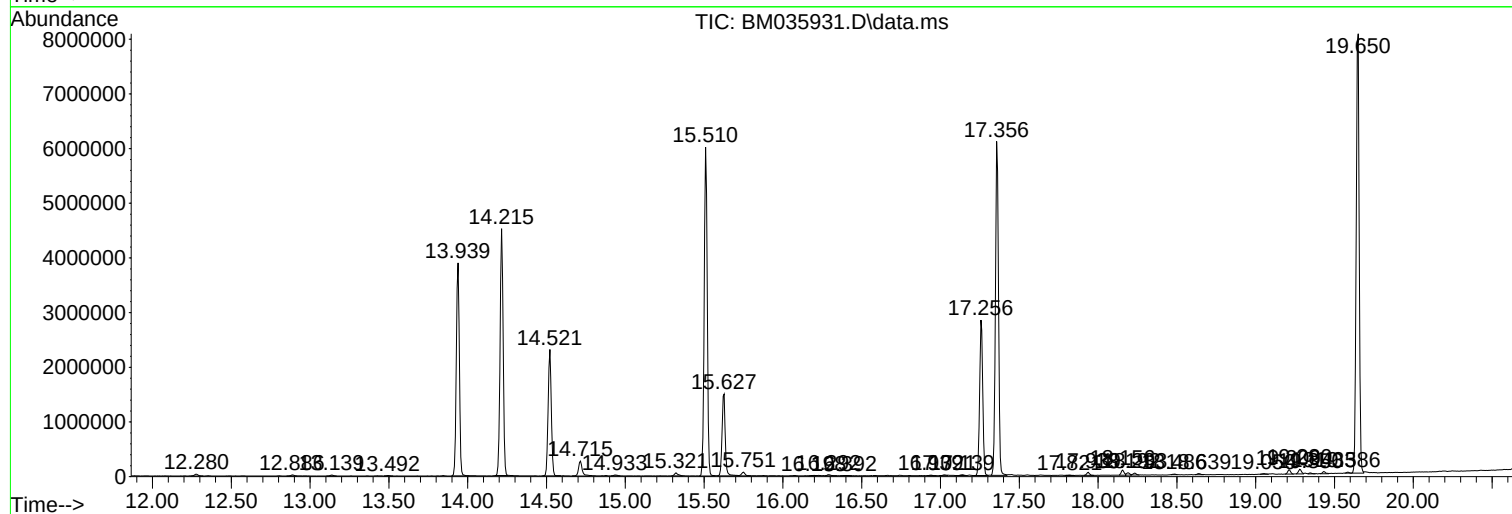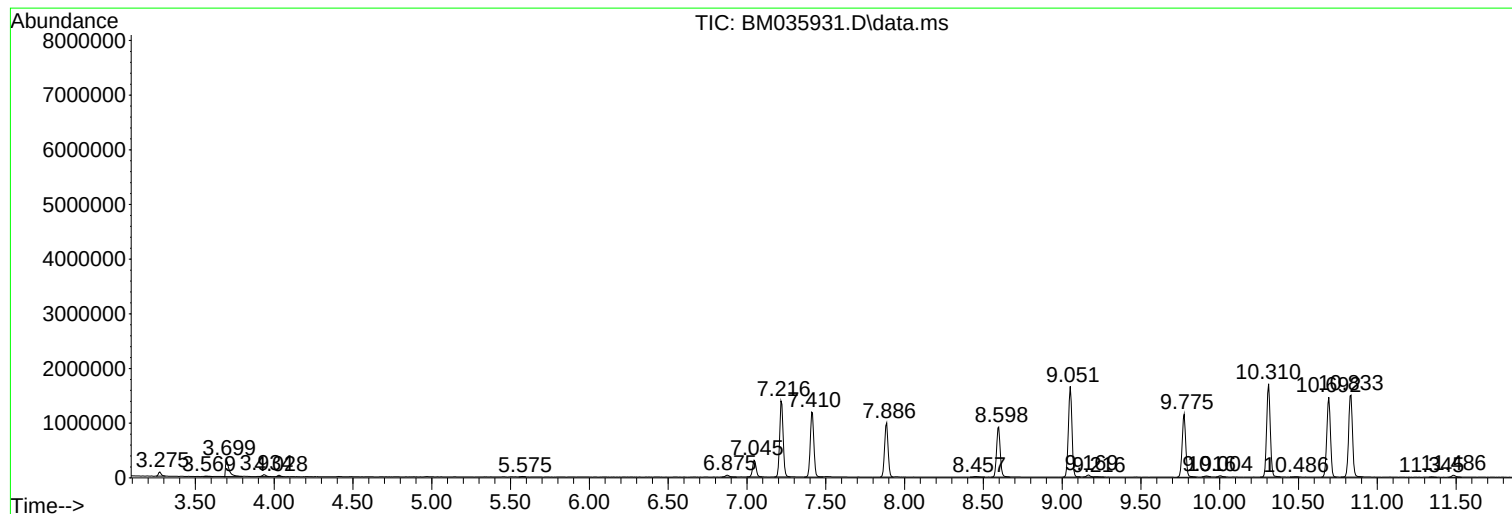

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035931.D
Acq On : 26 Jul 2022 18:19
Operator : CG/JU
Sample : N3792-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035931.D
Acq On : 26 Jul 2022 18:19
Operator : CG/JU
Sample : N3792-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUN8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc