

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035932.D
 Acq On : 26 Jul 2022 18:56
 Operator : CG/JU
 Sample : N3792-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUN0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035932.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	39	rVB	97947	126566	0.95%	0.112%
2	3.569	79	82	86	rVB2	12064	15208	0.11%	0.013%
3	3.699	102	104	122	rBV	237766	381084	2.85%	0.337%
4	3.940	138	145	149	rBV	36384	57817	0.43%	0.051%
5	4.034	157	161	167	rVB	30882	44140	0.33%	0.039%
6	4.263	196	200	208	rVB	26169	34768	0.26%	0.031%
7	4.428	223	228	235	rBV7	11852	25229	0.19%	0.022%
8	4.681	267	271	276	rBV3	16015	20422	0.15%	0.018%
9	7.046	666	673	686	rBV	463890	716996	5.36%	0.635%
10	7.216	694	702	712	rBV	1736714	2664028	19.91%	2.358%
11	7.293	712	715	719	rVB	11513	17543	0.13%	0.016%
12	7.410	728	735	747	rBV	1604476	2460204	18.38%	2.177%
13	7.881	808	815	823	rBV	1436878	2293854	17.14%	2.030%
14	8.593	928	936	947	rBV	1250062	2012013	15.04%	1.781%
15	9.051	1006	1014	1022	rBV	2006966	3184115	23.79%	2.818%
16	9.216	1037	1042	1048	rVB7	9052	17915	0.13%	0.016%
17	9.769	1128	1136	1148	rBV	1364107	2253453	16.84%	1.994%
18	9.934	1157	1164	1173	rVB5	7930	19707	0.15%	0.017%
19	10.310	1220	1228	1241	rBV	2139537	3519014	26.30%	3.115%
20	10.481	1253	1257	1266	rVB5	13234	25742	0.19%	0.023%
21	10.692	1285	1293	1300	rBV	2131157	3551640	26.54%	3.144%
22	10.828	1305	1316	1328	rBV	1045590	1740831	13.01%	1.541%
23	12.275	1556	1562	1565	rBV2	44527	70491	0.53%	0.062%
24	12.316	1565	1569	1579	rVB	100788	154642	1.16%	0.137%
25	12.886	1662	1666	1670	rBV6	7886	13855	0.10%	0.012%
26	13.139	1704	1709	1715	rBV7	8714	13608	0.10%	0.012%
27	13.492	1762	1769	1773	rBV7	11732	22805	0.17%	0.020%
28	13.939	1838	1845	1854	rBV	4734579	6351498	47.46%	5.622%
29	14.216	1880	1892	1901	rBV	5389650	7495389	56.01%	6.634%
30	14.522	1932	1944	1958	rBV	3482674	4965566	37.11%	4.395%
31	14.716	1970	1977	1996	rVB	400948	626680	4.68%	0.555%
32	14.869	2001	2003	2010	rVV7	10609	19427	0.15%	0.017%
33	14.939	2010	2015	2019	rVB8	8923	14715	0.11%	0.013%
34	15.321	2075	2080	2082	rBV2	13152	17645	0.13%	0.016%
35	15.510	2104	2112	2125	rBV	7101298	9800504	73.24%	8.674%
36	15.621	2125	2131	2145	rVV	854663	1190227	8.89%	1.053%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035932.D
 Acq On : 26 Jul 2022 18:56
 Operator : CG/JU
 Sample : N3792-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBUN0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.751	2148	2153	2160	rVB	79326	116653	0.87%	0.103%
38	15.869	2169	2173	2177	rBV7	9315	15688	0.12%	0.014%
39	16.074	2202	2208	2212	rVB8	7008	15201	0.11%	0.013%
40	16.174	2222	2225	2231	rBV5	16509	26522	0.20%	0.023%
41	16.233	2231	2235	2239	rVV4	12649	17908	0.13%	0.016%
42	16.292	2240	2245	2252	rVB4	29879	51661	0.39%	0.046%
43	16.751	2319	2323	2328	rBV3	16084	27830	0.21%	0.025%
44	16.939	2352	2355	2359	rVB6	13280	17084	0.13%	0.015%
45	17.021	2365	2369	2372	rBV3	19704	30197	0.23%	0.027%
46	17.133	2386	2388	2392	rVB2	14228	15433	0.12%	0.014%
47	17.180	2392	2396	2401	rVB7	13721	22469	0.17%	0.020%
48	17.257	2403	2409	2416	rBV	4344593	6008072	44.90%	5.318%
49	17.310	2416	2418	2420	rVV2	17579	16961	0.13%	0.015%
50	17.357	2420	2426	2439	rVB	7522130	10556339	78.88%	9.343%
51	17.551	2456	2459	2466	rVB2	14875	27477	0.21%	0.024%
52	17.633	2469	2473	2478	rVB5	13643	23779	0.18%	0.021%
53	17.939	2520	2525	2531	rVB	95454	116261	0.87%	0.103%
54	18.157	2558	2562	2567	rBV3	28551	40954	0.31%	0.036%
55	18.233	2571	2575	2579	rVB	43931	52222	0.39%	0.046%
56	18.486	2616	2618	2626	rVB9	13682	23828	0.18%	0.021%
57	18.639	2640	2644	2648	rVB3	34240	48189	0.36%	0.043%
58	19.051	2710	2714	2718	rBV2	58546	86146	0.64%	0.076%
59	19.209	2737	2741	2746	rVB2	100660	129454	0.97%	0.115%
60	19.280	2749	2753	2757	rBV	106934	138702	1.04%	0.123%
61	19.345	2762	2764	2768	rVB4	19689	21012	0.16%	0.019%
62	19.586	2802	2805	2809	rVB3	26392	29388	0.22%	0.026%
63	19.645	2809	2815	2822	rBV	9715072	13382111	100.00%	11.844%
64	20.651	2984	2986	2989	rVB2	46056	43913	0.33%	0.039%
65	21.151	3067	3071	3078	rBV	200972	313008	2.34%	0.277%
66	21.433	3114	3119	3130	rBV	5625747	6717502	50.20%	5.946%
67	23.097	3398	3402	3407	rVB	157342	217757	1.63%	0.193%
68	23.656	3488	3497	3504	rBV2	6173010	12059910	90.12%	10.674%
69	23.803	3515	3522	3538	rVB2	3192349	6184484	46.21%	5.474%
70	24.433	3625	3629	3637	rVB	222895	450113	3.36%	0.398%




Sum of corrected areas: 112983569

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035932.D
Acq On : 26 Jul 2022 18:56
Operator : CG/JU
Sample : N3792-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUN0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

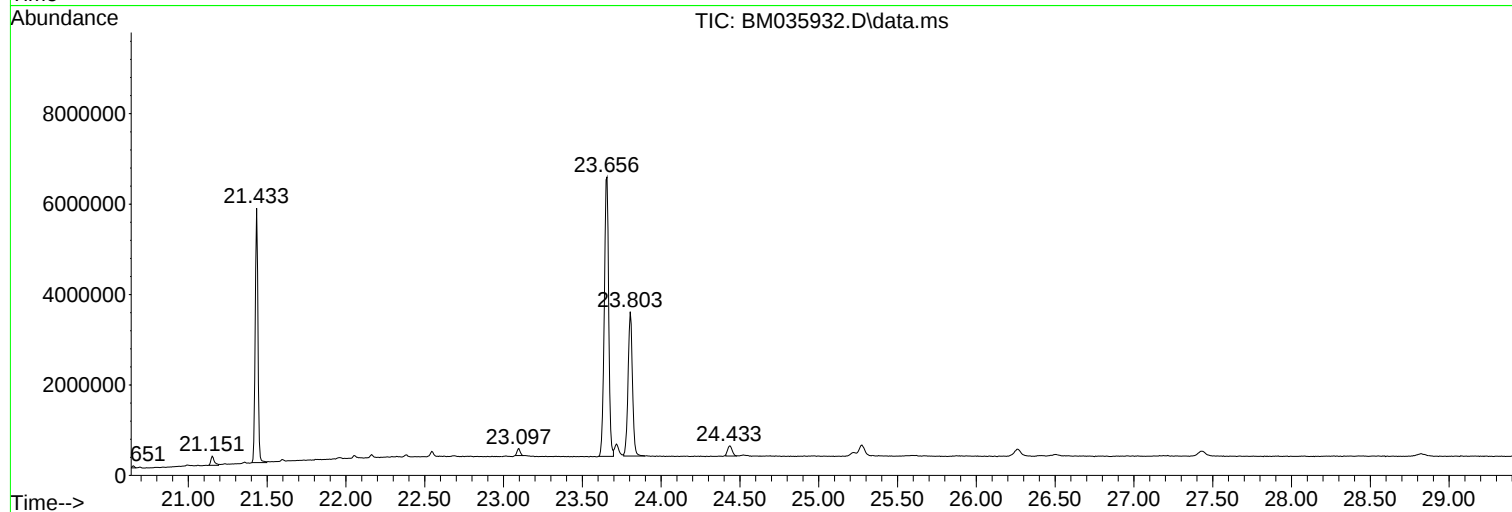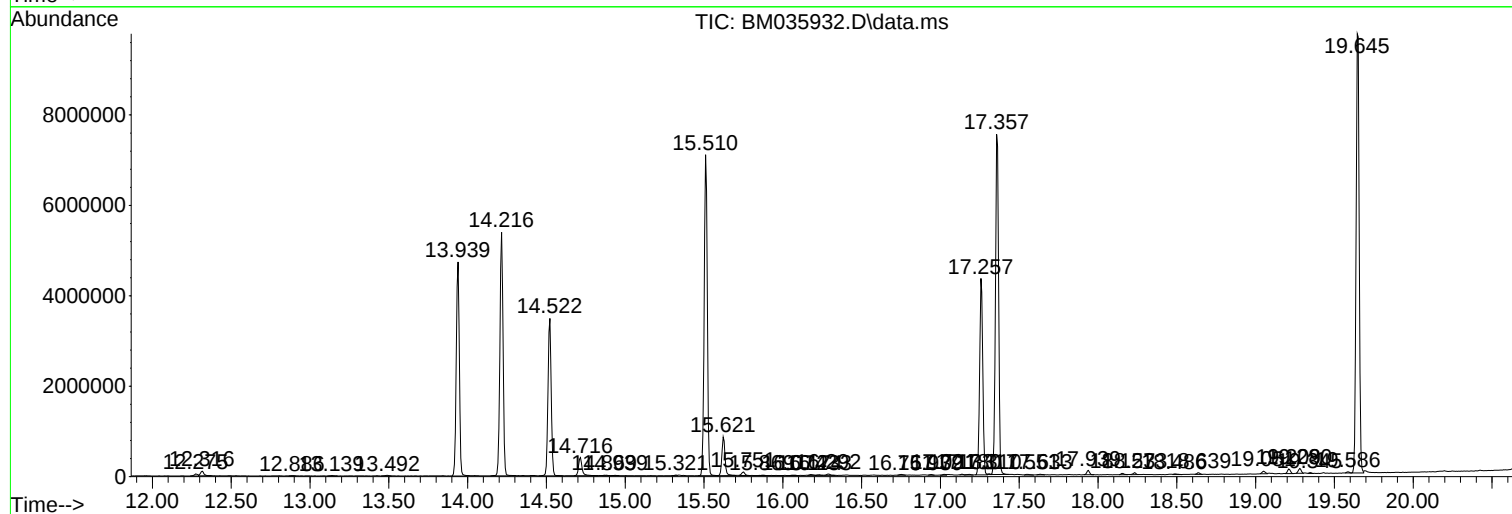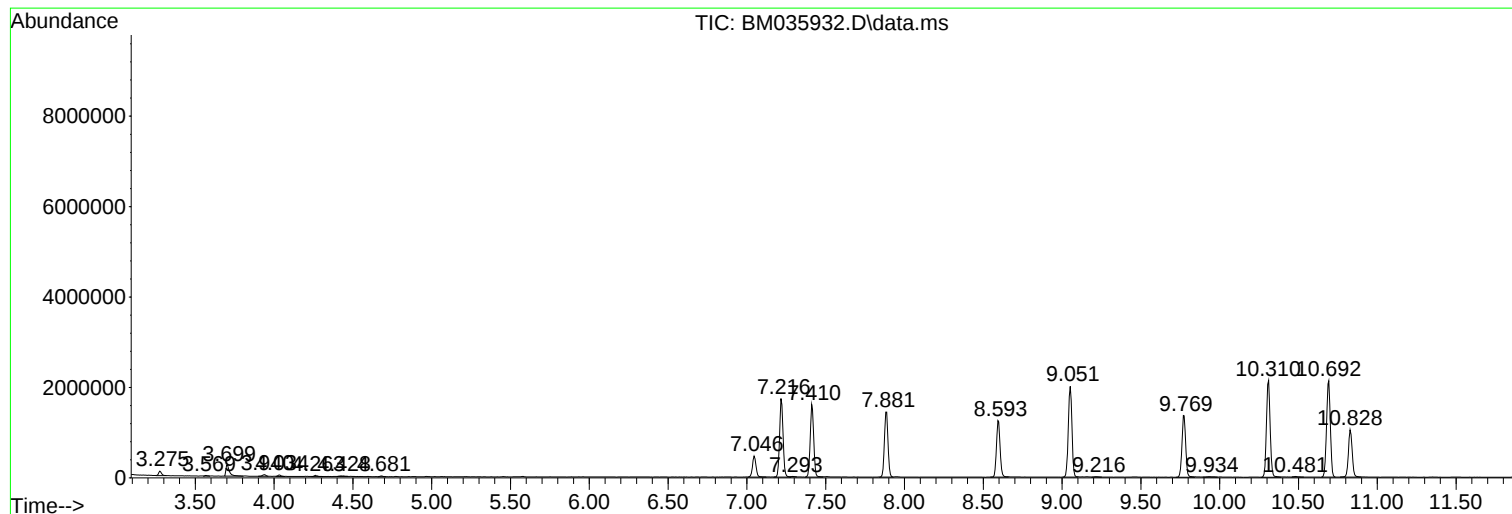

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035932.D
Acq On : 26 Jul 2022 18:56
Operator : CG/JU
Sample : N3792-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUN0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035932.D
Acq On : 26 Jul 2022 18:56
Operator : CG/JU
Sample : N3792-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBUN0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------