

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035933.D
 Acq On : 26 Jul 2022 19:32
 Operator : CG/JU
 Sample : N3704-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035933.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	42	rVB	109297	152094	1.51%	0.161%
2	3.558	77	80	94	rBV	67249	106411	1.05%	0.113%
3	3.693	100	103	119	rBV	696110	1115716	11.04%	1.181%
4	3.934	140	144	149	rVB2	17463	27967	0.28%	0.030%
5	4.034	156	161	168	rVB	20232	30295	0.30%	0.032%
6	4.963	315	319	324	rBV4	9700	18069	0.18%	0.019%
7	5.010	324	327	334	rVB	10096	15755	0.16%	0.017%
8	5.210	358	361	367	rBV5	5731	10503	0.10%	0.011%
9	5.575	417	423	427	rBV5	7557	11753	0.12%	0.012%
10	7.046	665	673	690	rBV	1299483	1991589	19.71%	2.107%
11	7.216	696	702	711	rBV	1144639	1737414	17.19%	1.838%
12	7.293	711	715	720	rVB	19860	31946	0.32%	0.034%
13	7.410	727	735	745	rBV	1286923	2004369	19.83%	2.121%
14	7.887	809	816	823	rBV	1063448	1686508	16.69%	1.785%
15	7.951	823	827	832	rVB3	9675	16606	0.16%	0.018%
16	8.598	929	937	952	rBV	1615918	2635957	26.08%	2.789%
17	9.051	1006	1014	1026	rBV	1329114	2085018	20.63%	2.206%
18	9.216	1038	1042	1048	rBV9	8378	16226	0.16%	0.017%
19	9.469	1078	1085	1091	rVB7	6917	18692	0.18%	0.020%
20	9.775	1128	1137	1148	rBV	953408	1574498	15.58%	1.666%
21	10.310	1220	1228	1239	rBV	1568987	2536975	25.11%	2.685%
22	10.481	1253	1257	1263	rBV5	9634	14685	0.15%	0.016%
23	10.692	1285	1293	1302	rBV	1569582	2641125	26.14%	2.795%
24	10.828	1306	1316	1331	rBV	1751063	2961817	29.31%	3.134%
25	12.275	1555	1562	1570	rVB	31962	55281	0.55%	0.058%
26	12.886	1662	1666	1672	rBV8	7454	12546	0.12%	0.013%
27	13.139	1704	1709	1713	rBV4	8378	12677	0.13%	0.013%
28	13.492	1764	1769	1775	rBV7	8730	14989	0.15%	0.016%
29	13.939	1837	1845	1856	rBV	3416479	4590916	45.43%	4.858%
30	14.216	1885	1892	1902	rVB	3794574	5332157	52.77%	5.642%
31	14.422	1923	1927	1932	rVB4	8326	12312	0.12%	0.013%
32	14.522	1936	1944	1955	rBV	2496077	3647543	36.09%	3.860%
33	14.716	1968	1977	1995	rBV	1538621	2269949	22.46%	2.402%
34	14.939	2008	2015	2020	rBV3	23528	35467	0.35%	0.038%
35	15.322	2075	2080	2083	rBV2	12503	20525	0.20%	0.022%
36	15.369	2085	2088	2095	rVB5	9062	14646	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035933.D
 Acq On : 26 Jul 2022 19:32
 Operator : CG/JU
 Sample : N3704-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	15.510	2101	2112	2125	rBV	5048858	7011780	69.39%	7.420%
38	15.622	2125	2131	2144	rVV	1300428	1735147	17.17%	1.836%
39	15.751	2147	2153	2157	rVB	55214	77272	0.76%	0.082%
40	16.292	2241	2245	2248	rBV4	18533	22733	0.22%	0.024%
41	16.398	2257	2263	2268	rBV10	7721	17747	0.18%	0.019%
42	16.516	2277	2283	2289	rBV6	6417	14298	0.14%	0.015%
43	16.745	2318	2322	2326	rBV5	7605	12344	0.12%	0.013%
44	16.939	2350	2355	2361	rBV9	7896	13111	0.13%	0.014%
45	17.027	2366	2370	2371	rBV3	11351	14809	0.15%	0.016%
46	17.257	2403	2409	2418	rVV	3035328	4351499	43.06%	4.605%
47	17.357	2419	2426	2438	rVV	5657330	7753302	76.72%	8.204%
48	17.451	2438	2442	2447	rVB	61619	86304	0.85%	0.091%
49	17.557	2456	2460	2466	rVB6	7843	13106	0.13%	0.014%
50	17.639	2469	2474	2480	rBV7	7766	15208	0.15%	0.016%
51	17.933	2521	2524	2529	rVB2	24583	32176	0.32%	0.034%
52	18.157	2557	2562	2569	rBV	138196	197882	1.96%	0.209%
53	18.233	2572	2575	2580	rVB	14989	22808	0.23%	0.024%
54	19.045	2708	2713	2718	rBV9	20180	41051	0.41%	0.043%
55	19.210	2737	2741	2745	rBV2	72465	94302	0.93%	0.100%
56	19.280	2749	2753	2762	rVV	70574	103131	1.02%	0.109%
57	19.433	2776	2779	2783	rBV3	46442	56467	0.56%	0.060%
58	19.586	2802	2805	2809	rBV	38875	45997	0.46%	0.049%
59	19.645	2809	2815	2822	rBV	7318934	9515592	94.16%	10.069%
60	20.198	2906	2909	2914	rVB	67029	74424	0.74%	0.079%
61	20.574	2970	2973	2977	rBV2	98480	131131	1.30%	0.139%
62	20.692	2989	2993	2997	rVB2	159741	193085	1.91%	0.204%
63	21.151	3067	3071	3081	rBV2	518893	768477	7.60%	0.813%
64	21.433	3113	3119	3126	rBV	4124604	5100073	50.47%	5.397%
65	21.592	3143	3146	3154	rBV	218124	245473	2.43%	0.260%
66	22.050	3221	3224	3231	rBV	203546	250468	2.48%	0.265%
67	22.545	3304	3308	3316	rVB2	251671	365150	3.61%	0.386%
68	23.092	3398	3401	3408	rVB	219660	311313	3.08%	0.329%
69	23.650	3488	3496	3503	rBV2	5482369	10105420	100.00%	10.693%
70	23.715	3504	3507	3514	rVV	281566	488959	4.84%	0.517%
71	23.803	3515	3522	3538	rVB2	2609985	5288735	52.34%	5.596%
72	24.433	3625	3629	3638	rVB	239201	472080	4.67%	0.500%




Sum of corrected areas: 94503850

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035933.D
Acq On : 26 Jul 2022 19:32
Operator : CG/JU
Sample : N3704-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COAH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

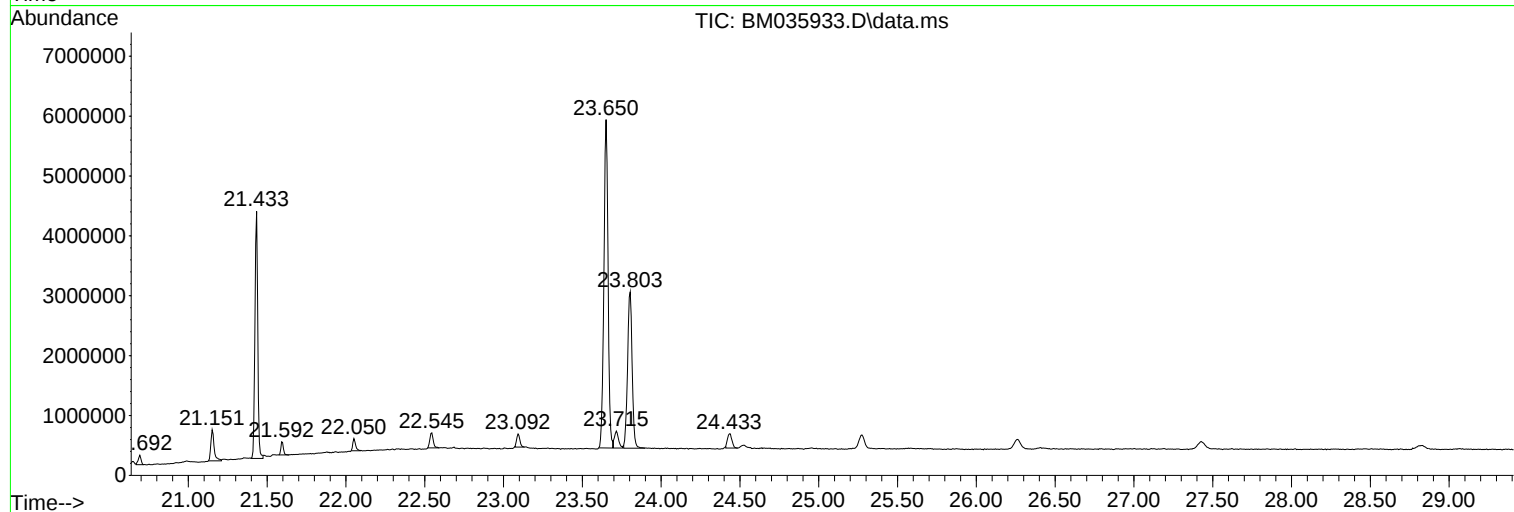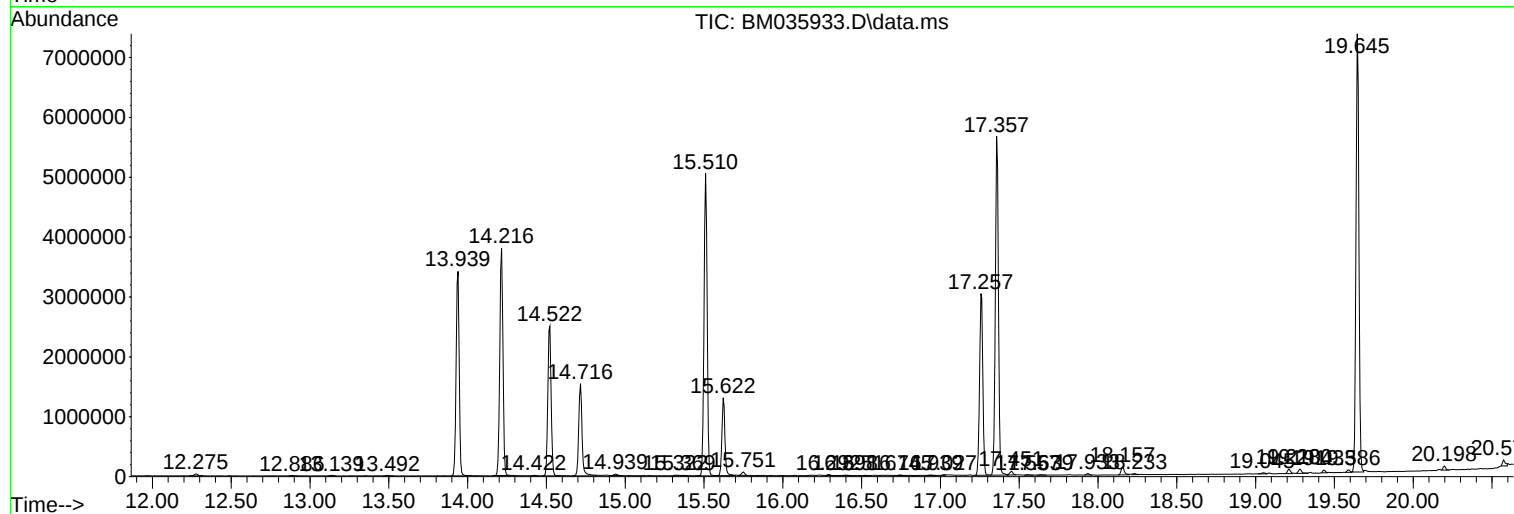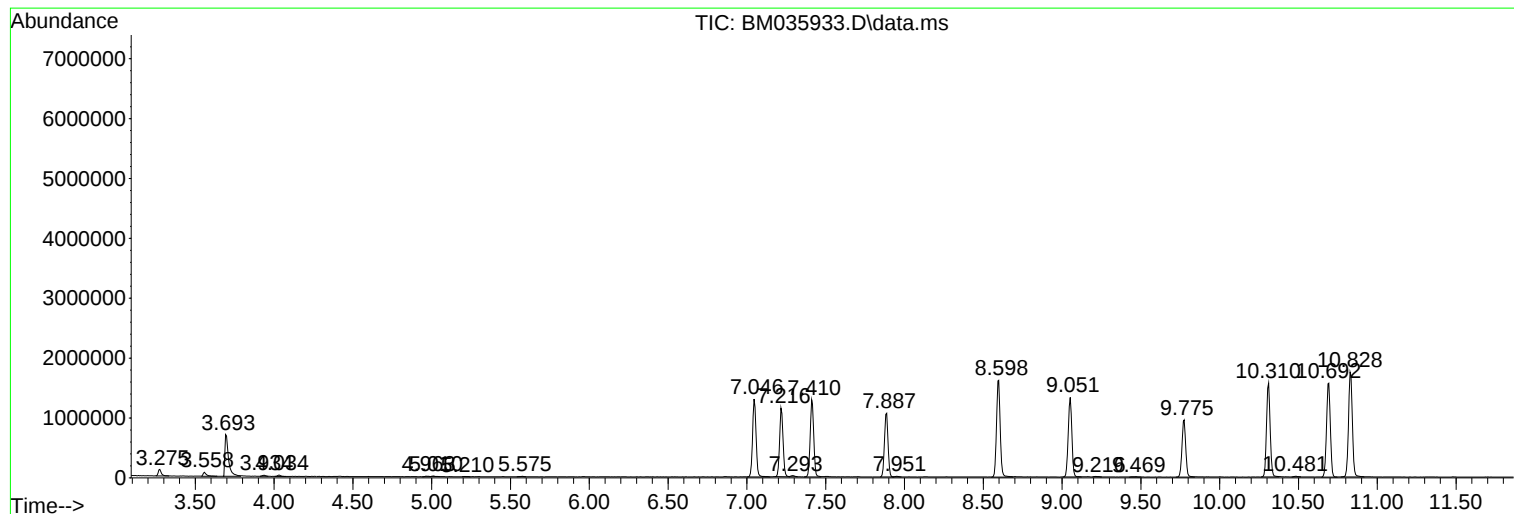

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035933.D
Acq On : 26 Jul 2022 19:32
Operator : CG/JU
Sample : N3704-01
Misc :
ALS Vial : 17 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
C0AH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentadecafluorooctanoic aci... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.151	3.01 ng/ul	768477	Chrysene-d12	21.433	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	91
2	Oxalic acid, isobutyl hexadecyl ...	370	C22H42O4	1000309-38-1	91
3	Ethanol, 2-(tetradecyloxy)-	258	C16H34O2	002136-70-1	90
4	Pentafluoropropionic acid, hepta...	402	C20H35F5O2	959218-78-1	76
5	Heptafluorobutyric acid, hexadec...	438	C20H33F7O2	006385-15-5	76

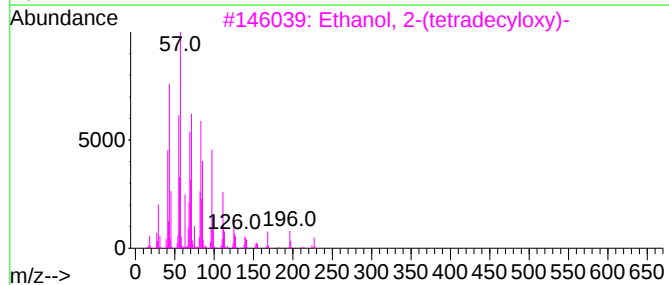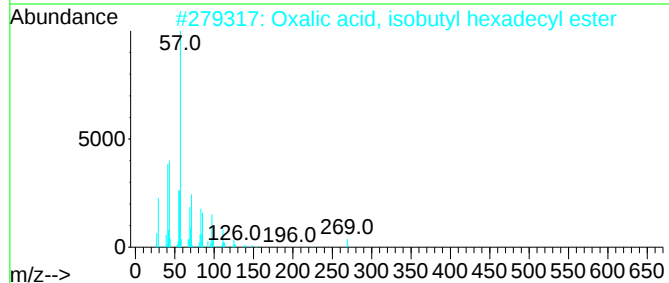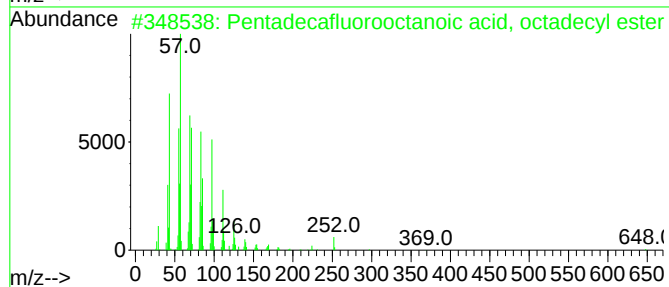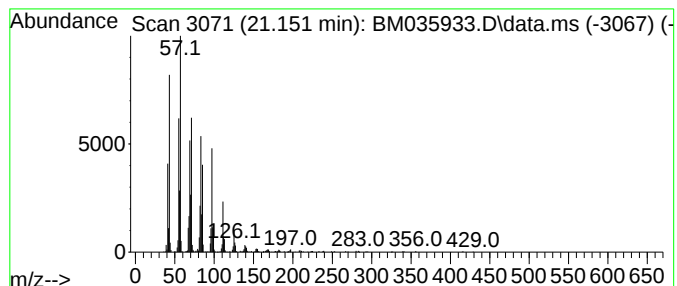

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035933.D
Acq On : 26 Jul 2022 19:32
Operator : CG/JU
Sample : N3704-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentadecafluoro...	21.151	3.0	ng/ul	768477	5	21.433	5100070	20.0