

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035938.D
 Acq On : 26 Jul 2022 22:35
 Operator : CG/JU
 Sample : N3831-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VNJ-237

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	37	rVB	44138	53714	0.99%	0.095%
2	3.716	103	107	113	rVB	37150	47972	0.88%	0.085%
3	3.816	119	124	132	rVV	192752	254453	4.67%	0.449%
4	3.887	132	136	140	rVV	23814	31383	0.58%	0.055%
5	3.940	140	145	151	rVB	84650	132812	2.44%	0.234%
6	4.034	157	161	166	rVB	29699	42173	0.77%	0.074%
7	4.204	187	190	195	rVB5	8873	12459	0.23%	0.022%
8	4.269	197	201	205	rVB6	6206	8734	0.16%	0.015%
9	4.416	222	226	232	rVB5	13416	19918	0.37%	0.035%
10	4.487	234	238	244	rVB5	5998	8545	0.16%	0.015%
11	4.599	253	257	262	rVB2	25306	36192	0.66%	0.064%
12	4.675	267	270	276	rBV6	5895	10106	0.19%	0.018%
13	4.775	281	287	295	rVB2	10412	24945	0.46%	0.044%
14	4.869	298	303	304	rBV5	5128	8232	0.15%	0.015%
15	4.963	314	319	324	rBV	32130	49498	0.91%	0.087%
16	5.069	332	337	342	rBV	25897	41289	0.76%	0.073%
17	5.457	398	403	407	rVB	9598	14328	0.26%	0.025%
18	5.575	419	423	429	rVB	20446	27481	0.50%	0.049%
19	6.104	510	513	516	rBV5	5911	9274	0.17%	0.016%
20	6.740	617	621	626	rBV3	10552	15796	0.29%	0.028%
21	6.869	640	643	648	rVB4	8407	10965	0.20%	0.019%
22	7.045	664	673	689	rBV	501096	811174	14.90%	1.432%
23	7.216	695	702	713	rBV	717261	1088601	20.00%	1.922%
24	7.298	713	716	721	rVB6	6352	9508	0.17%	0.017%
25	7.410	729	735	746	rBV	493213	771203	14.17%	1.362%
26	7.504	747	751	755	rBV	13860	18511	0.34%	0.033%
27	7.704	780	785	792	rVB5	7852	14262	0.26%	0.025%
28	7.881	804	815	823	rBV	1443026	2279544	41.88%	4.025%
29	7.951	823	827	833	rVB4	9634	17194	0.32%	0.030%
30	8.110	850	854	861	rBV6	5603	11135	0.20%	0.020%
31	8.422	900	907	913	rBV7	6805	16287	0.30%	0.029%
32	8.592	928	936	944	rBV	371878	597740	10.98%	1.055%
33	8.716	951	957	962	rBV	36096	57607	1.06%	0.102%
34	9.051	1007	1014	1022	rBV	768263	1260580	23.16%	2.226%
35	9.216	1037	1042	1047	rBV7	9739	14889	0.27%	0.026%
36	9.469	1077	1085	1089	rBV	14685	23721	0.44%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035938.D
 Acq On : 26 Jul 2022 22:35
 Operator : CG/JU
 Sample : N3831-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VNJ-237

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	9.769	1127	1136	1142	rBV2	101084	175094	3.22%	0.309%
38	10.133	1191	1198	1203	rBV10	5575	11029	0.20%	0.019%
39	10.304	1220	1227	1236	rBV	437029	738294	13.56%	1.304%
40	10.475	1250	1256	1259	rBV7	4720	8977	0.16%	0.016%

41	10.686	1284	1292	1306	rBV	2139840	3527313	64.80%	6.228%
42	10.828	1306	1316	1336	rVV	707759	1243428	22.84%	2.195%
43	11.228	1380	1384	1390	rBV9	4681	9534	0.18%	0.017%
44	11.304	1392	1397	1400	rBV6	4312	8681	0.16%	0.015%
45	11.963	1503	1509	1513	rBV4	5302	11377	0.21%	0.020%

46	12.275	1554	1562	1569	rVB2	20747	42374	0.78%	0.075%
47	12.886	1660	1666	1671	rVB4	12958	18609	0.34%	0.033%
48	13.133	1704	1708	1716	rVB2	13845	19721	0.36%	0.035%
49	13.351	1742	1745	1750	rVB6	6694	8656	0.16%	0.015%
50	13.486	1765	1768	1774	rVB4	7261	10705	0.20%	0.019%

51	13.845	1824	1829	1834	rVB7	11775	17499	0.32%	0.031%
52	13.933	1838	1844	1853	rVV	1347115	1788063	32.85%	3.157%
53	14.169	1881	1884	1885	rBV2	8403	8281	0.15%	0.015%
54	14.210	1885	1891	1899	rVV	2096487	3012127	55.34%	5.318%
55	14.421	1924	1927	1932	rVB4	9629	11433	0.21%	0.020%

56	14.521	1935	1944	1950	rBV	3178575	4698846	86.33%	8.296%
57	14.574	1951	1953	1961	rVB4	14931	23037	0.42%	0.041%
58	14.745	1975	1982	1983	rVV6	6868	14337	0.26%	0.025%
59	14.768	1983	1986	1989	rVB5	6662	8154	0.15%	0.014%
60	14.868	1999	2003	2008	rBV3	28337	47606	0.87%	0.084%

61	14.939	2011	2015	2020	rVB4	23241	34310	0.63%	0.061%
62	15.286	2070	2074	2075	rBV3	6040	8013	0.15%	0.014%
63	15.316	2075	2079	2081	rVV	15364	25104	0.46%	0.044%
64	15.368	2085	2088	2092	rVB4	10087	13304	0.24%	0.023%
65	15.510	2105	2112	2119	rBV	2818128	3950340	72.58%	6.975%

66	15.557	2119	2120	2126	rVV5	19455	28259	0.52%	0.050%
67	15.615	2128	2130	2136	rVB7	7809	12071	0.22%	0.021%
68	15.745	2146	2152	2161	rBV3	31386	53826	0.99%	0.095%
69	15.998	2191	2195	2198	rBV6	5450	8525	0.16%	0.015%
70	16.233	2227	2235	2242	rBV3	29058	69836	1.28%	0.123%

71	16.292	2242	2245	2252	rVB7	13863	20095	0.37%	0.035%
72	16.392	2257	2262	2263	rBV5	7360	9293	0.17%	0.016%
73	16.574	2289	2293	2296	rVV6	4698	8289	0.15%	0.015%
74	16.739	2318	2321	2326	rVB4	8970	12088	0.22%	0.021%
75	16.804	2327	2332	2336	rBV	45731	61373	1.13%	0.108%

76	17.021	2362	2369	2376	rBV8	25471	57081	1.05%	0.101%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035938.D
 Acq On : 26 Jul 2022 22:35
 Operator : CG/JU
 Sample : N3831-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 VNJ-237

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

77	17.068	2376	2377	2382	rVB3	10974	11914	0.22%	0.021%
78	17.180	2393	2396	2400	rBV6	11745	14183	0.26%	0.025%
79	17.257	2402	2409	2414	rBV	3992411	5443086	100.00%	9.610%
80	17.298	2414	2416	2420	rVV	88792	112911	2.07%	0.199%
81	17.357	2420	2426	2437	rVV	2786449	3846703	70.67%	6.792%
82	17.445	2439	2441	2446	rVB6	15010	21700	0.40%	0.038%
83	17.551	2456	2459	2464	rVB4	9625	14758	0.27%	0.026%
84	17.657	2472	2477	2481	rVB6	19521	35142	0.65%	0.062%
85	17.762	2491	2495	2499	rBV6	10706	16102	0.30%	0.028%
86	17.933	2520	2524	2529	rVB2	83395	112073	2.06%	0.198%
87	18.151	2554	2561	2564	rBV6	29048	54963	1.01%	0.097%
88	18.227	2570	2574	2578	rBV	43818	51985	0.96%	0.092%
89	18.327	2589	2591	2594	rVB2	15420	14248	0.26%	0.025%
90	18.456	2610	2613	2616	rBV3	12057	13998	0.26%	0.025%
91	19.045	2710	2713	2718	rBV2	54551	81865	1.50%	0.145%
92	19.209	2738	2741	2745	rVB3	37873	47558	0.87%	0.084%
93	19.280	2750	2753	2755	rVV2	34703	48536	0.89%	0.086%
94	19.309	2755	2758	2763	rVB	152744	189707	3.49%	0.335%
95	19.645	2809	2815	2829	rBV	3629339	4951275	90.96%	8.742%
96	20.650	2983	2986	2989	rVB	67233	68430	1.26%	0.121%
97	21.150	3067	3071	3080	rBV	526620	782331	14.37%	1.381%
98	21.433	3113	3119	3123	rBV	4076003	5349675	98.28%	9.445%
99	23.644	3489	3495	3503	rBV2	1686451	3181268	58.45%	5.617%
100	23.797	3515	3521	3542	rVB2	2178298	4486945	82.43%	7.922%




Sum of corrected areas: 56638563

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035938.D
Acq On : 26 Jul 2022 22:35
Operator : CG/JU
Sample : N3831-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-237

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

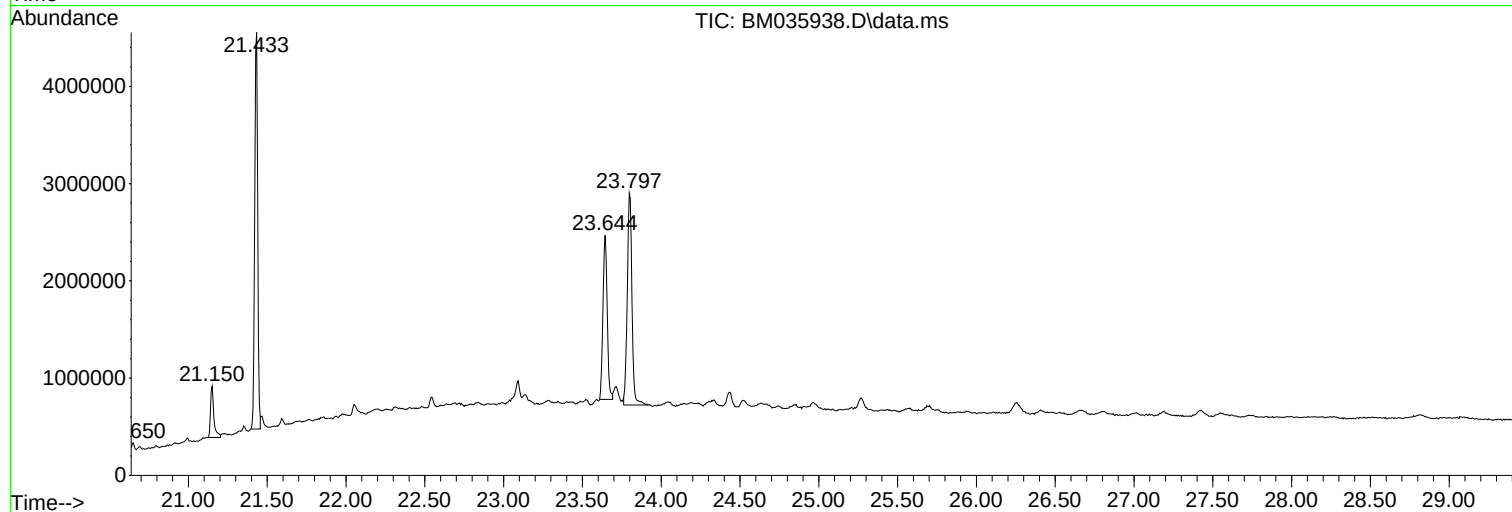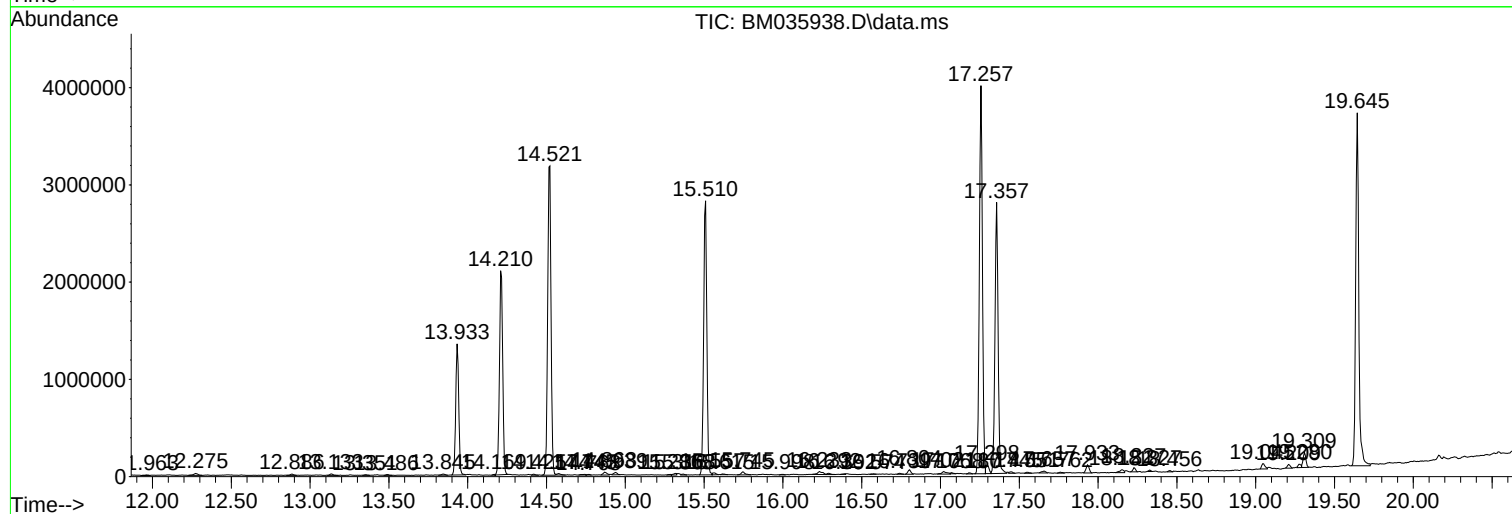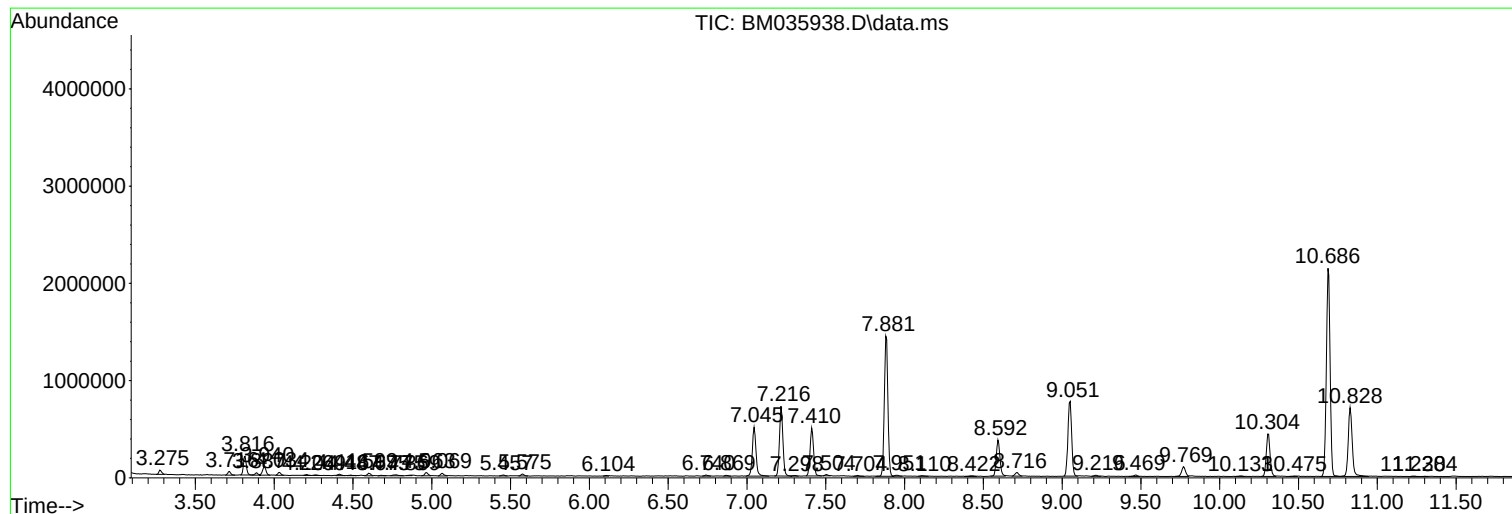

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035938.D
Acq On : 26 Jul 2022 22:35
Operator : CG/JU
Sample : N3831-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-237










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.816	2.23 ng/ul	254453	1,4-Dichlorobenzene-d4	7.887

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Thiazole	85	C3H3NS	000288-47-1	43
2			Thiazole	85	C3H3NS	000288-47-1	43
3			2H-Pyran, tetrahydro-2-methyl-	100	C6H12O	010141-72-7	39
4			2,2'-Bi-2H-pyran, octahydro-	170	C10H18O2	016282-29-4	25
5			2-Pyrrolidinone	85	C4H7NO	000616-45-5	9

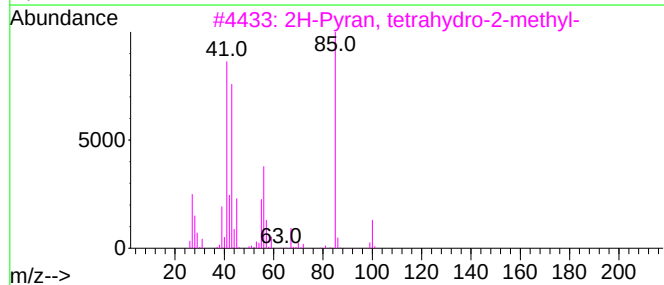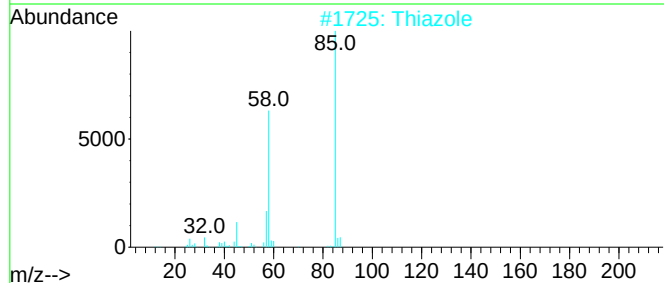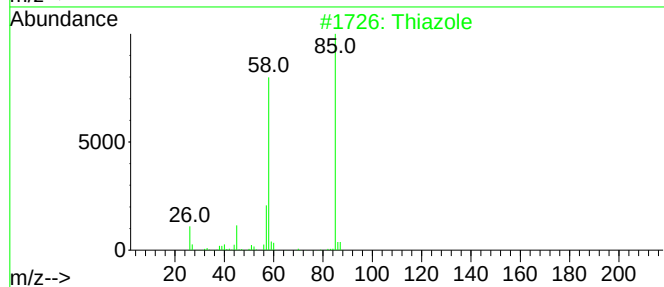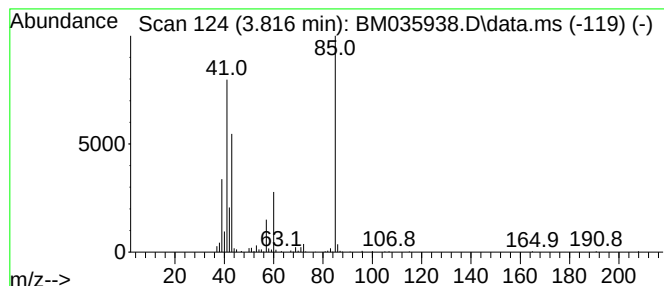

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035938.D
Acq On : 26 Jul 2022 22:35
Operator : CG/JU
Sample : N3831-01
Misc :
ALS Vial : 22 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
VNJ-237

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.150	2.92 ng/ul	782331	Chrysene-d12	21.433	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	5-Eicosene, (E)-	280	C20H40	074685-30-6	96
2	Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	94
3	Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
4	Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94
5	Cyclohexadecane	224	C16H32	000295-65-8	93

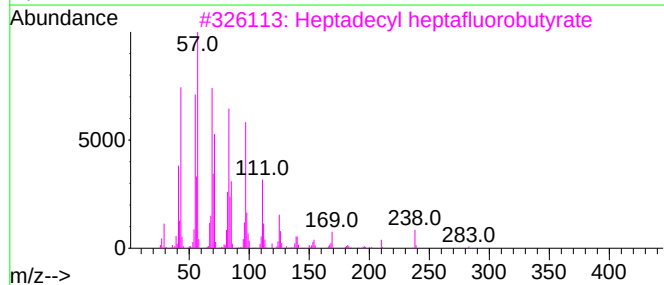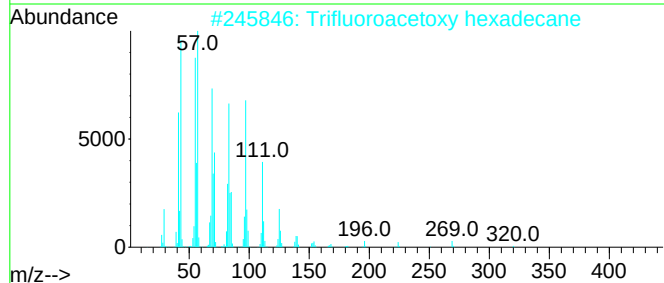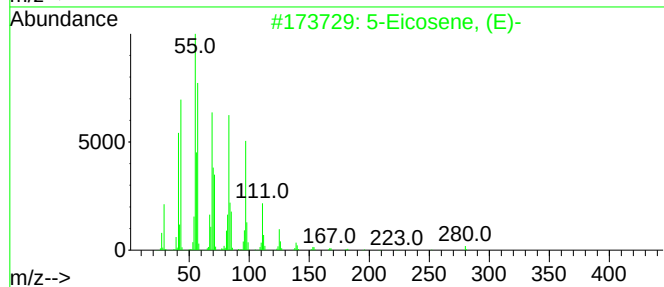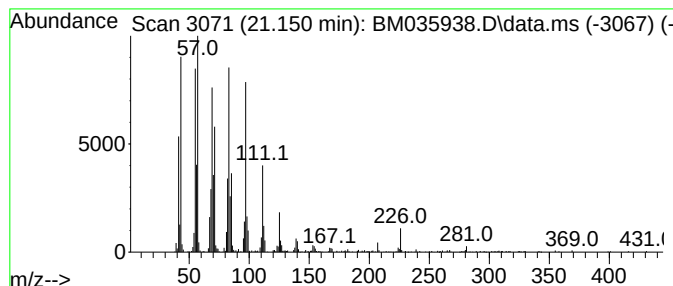

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035938.D
Acq On : 26 Jul 2022 22:35
Operator : CG/JU
Sample : N3831-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
VNJ-237

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.816	2.2	ng/u1	254453	1	7.887	2279540	20.0
(DEL) Alkane: S...	21.150	2.9	ng/u1	782331	5	21.433	5349680	20.0