

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035941.D
 Acq On : 27 Jul 2022 00:23
 Operator : CG/JU
 Sample : N3709-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0B28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	40	rVB	42337	76224	1.27%	0.119%
2	3.740	108	111	117	rBV8	9860	18001	0.30%	0.028%
3	3.822	122	125	134	rVB	23330	34028	0.57%	0.053%
4	3.940	139	145	153	rBV	75172	144836	2.41%	0.227%
5	4.040	159	162	168	rVB	27255	43995	0.73%	0.069%
6	4.416	222	226	232	rVB2	35803	60509	1.01%	0.095%
7	4.610	255	259	264	rVB6	13568	18052	0.30%	0.028%
8	4.969	315	320	327	rBV	40340	74981	1.25%	0.117%
9	5.069	333	337	342	rBV4	22959	40974	0.68%	0.064%
10	5.328	375	381	388	rBV6	17513	48170	0.80%	0.075%
11	5.457	399	403	407	rVB2	13417	21553	0.36%	0.034%
12	5.581	418	424	430	rVB	32419	51547	0.86%	0.081%
13	5.728	445	449	452	rBV	13692	17690	0.29%	0.028%
14	5.769	452	456	461	rVB8	11003	21636	0.36%	0.034%
15	5.934	480	484	495	rVB3	48987	97955	1.63%	0.153%
16	6.763	619	625	629	rBV	26115	48389	0.81%	0.076%
17	6.875	639	644	648	rBV6	14470	30292	0.50%	0.047%
18	7.016	663	668	670	rBV	59534	83337	1.39%	0.130%
19	7.063	670	676	689	rVB	1463627	2344497	39.08%	3.669%
20	7.228	697	704	712	rBV	1225968	1953099	32.56%	3.056%
21	7.293	712	715	719	rVB2	9693	17694	0.29%	0.028%
22	7.422	730	737	748	rVB	1568450	2435060	40.59%	3.810%
23	7.510	748	752	759	rVB3	23608	38270	0.64%	0.060%
24	7.587	760	765	769	rBV3	37086	55825	0.93%	0.087%
25	7.892	808	817	823	rBV	1807309	2763970	46.07%	4.325%
26	7.951	823	827	834	rVB3	29163	62966	1.05%	0.099%
27	8.287	881	884	887	rBV2	12991	17584	0.29%	0.028%
28	8.334	887	892	898	rVB6	10808	21440	0.36%	0.034%
29	8.498	914	920	925	rVB5	17167	35522	0.59%	0.056%
30	8.610	932	939	951	rBV	1935807	3050510	50.85%	4.773%
31	8.722	954	958	963	rVV	27726	44739	0.75%	0.070%
32	8.804	966	972	974	rVB6	10161	17723	0.30%	0.028%
33	8.992	999	1004	1008	rBV7	18015	31098	0.52%	0.049%
34	9.057	1008	1015	1023	rVV	1501208	2479072	41.32%	3.879%
35	9.122	1023	1026	1030	rVB4	15709	25871	0.43%	0.040%
36	9.222	1038	1043	1052	rVB2	55749	91123	1.52%	0.143%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
 Data File : BM035941.D
 Acq On : 27 Jul 2022 00:23
 Operator : CG/JU
 Sample : N3709-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0B28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
 Title : SVOA CALIBRATION

37	9.469	1076	1085	1094	rVB	221750	357009	5.95%	0.559%
38	9.598	1102	1107	1116	rBV2	26549	53468	0.89%	0.084%
39	9.781	1129	1138	1148	rBV	935447	1584367	26.41%	2.479%
40	10.028	1174	1180	1186	rBV7	14390	32323	0.54%	0.051%
41	10.322	1223	1230	1241	rBV	1817527	2939744	49.00%	4.600%
42	10.410	1241	1245	1252	rVB6	15621	34176	0.57%	0.053%
43	10.557	1266	1270	1274	rBV6	17824	28662	0.48%	0.045%
44	10.698	1286	1294	1302	rBV	2447298	4019695	67.00%	6.290%
45	10.792	1306	1310	1313	rVV2	42094	63119	1.05%	0.099%
46	10.839	1313	1318	1335	rVB	231539	470181	7.84%	0.736%
47	11.116	1360	1365	1371	rVB9	18772	37454	0.62%	0.059%
48	11.498	1421	1430	1436	rBV8	21439	51023	0.85%	0.080%
49	11.563	1436	1441	1444	rVB5	15317	25439	0.42%	0.040%
50	11.963	1503	1509	1514	rBV	100017	151903	2.53%	0.238%
51	12.028	1516	1520	1527	rVB9	18206	34525	0.58%	0.054%
52	12.116	1527	1535	1541	rBV5	25209	50423	0.84%	0.079%
53	12.251	1554	1558	1561	rBV4	41804	65762	1.10%	0.103%
54	12.280	1561	1563	1568	rVB	29810	45476	0.76%	0.071%
55	12.586	1610	1615	1620	rBV9	12013	17911	0.30%	0.028%
56	13.145	1706	1710	1714	rBV4	12657	18162	0.30%	0.028%
57	13.357	1742	1746	1750	rBV	34297	49863	0.83%	0.078%
58	13.404	1751	1754	1760	rVB2	27382	33350	0.56%	0.052%
59	13.498	1766	1770	1777	rBV5	49457	74285	1.24%	0.116%
60	13.580	1780	1784	1789	rVB8	11352	19991	0.33%	0.031%
61	13.663	1795	1798	1801	rBV5	16087	24275	0.40%	0.038%
62	13.704	1802	1805	1811	rVB7	15879	24358	0.41%	0.038%
63	13.774	1814	1817	1821	rBV4	23764	32641	0.54%	0.051%
64	13.945	1840	1846	1851	rBV	2784084	3709541	61.83%	5.805%
65	14.057	1861	1865	1869	rBV7	17078	30192	0.50%	0.047%
66	14.180	1882	1886	1887	rBV3	49184	64084	1.07%	0.100%
67	14.221	1887	1893	1903	rVB	3524530	5304953	88.43%	8.301%
68	14.427	1925	1928	1932	rVB2	44539	44927	0.75%	0.070%
69	14.527	1939	1945	1951	rBV	3092131	4477914	74.64%	7.007%
70	14.733	1975	1980	1991	rBV	667407	1047117	17.45%	1.639%
71	14.886	2002	2006	2010	rBV	78964	105943	1.77%	0.166%
72	14.945	2014	2016	2021	rVB4	38975	45904	0.77%	0.072%
73	15.321	2077	2080	2085	rVB	82342	106721	1.78%	0.167%
74	15.374	2085	2089	2093	rVB	177918	201920	3.37%	0.316%
75	15.521	2108	2114	2121	rBV	4287747	5999201	100.00%	9.388%
76	15.645	2131	2135	2141	rBV2	126415	171873	2.86%	0.269%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035941.D
Acq On : 27 Jul 2022 00:23
Operator : CG/JU
Sample : N3709-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0B28

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Title : SVOA CALIBRATION

77	16.239	2233	2236	2237	rBV2	71713	77929	1.30%	0.122%
78	17.268	2406	2411	2417	rBV	3078654	4228984	70.49%	6.618%
79	17.368	2422	2428	2437	rVV	3986665	5576705	92.96%	8.726%
80	18.168	2561	2564	2567	rBV3	202685	266529	4.44%	0.417%
81	19.656	2813	2817	2822	rBV	4188893	5687664	94.81%	8.900%




Sum of corrected areas: 63905918

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035941.D
Acq On : 27 Jul 2022 00:23
Operator : CG/JU
Sample : N3709-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0B28

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

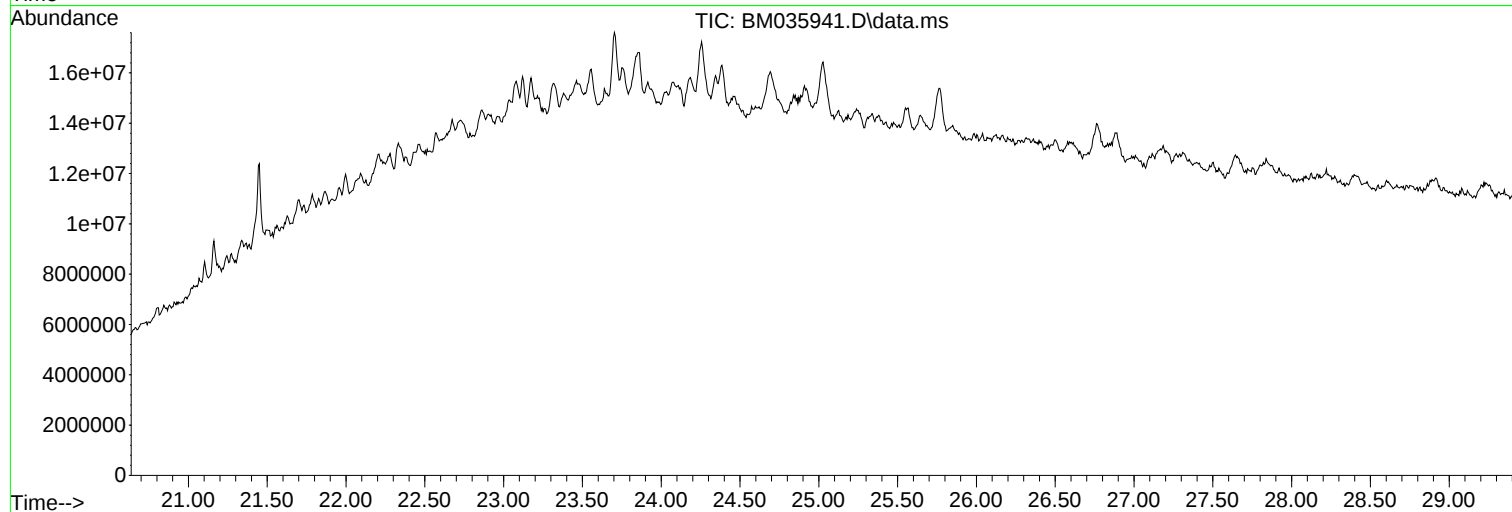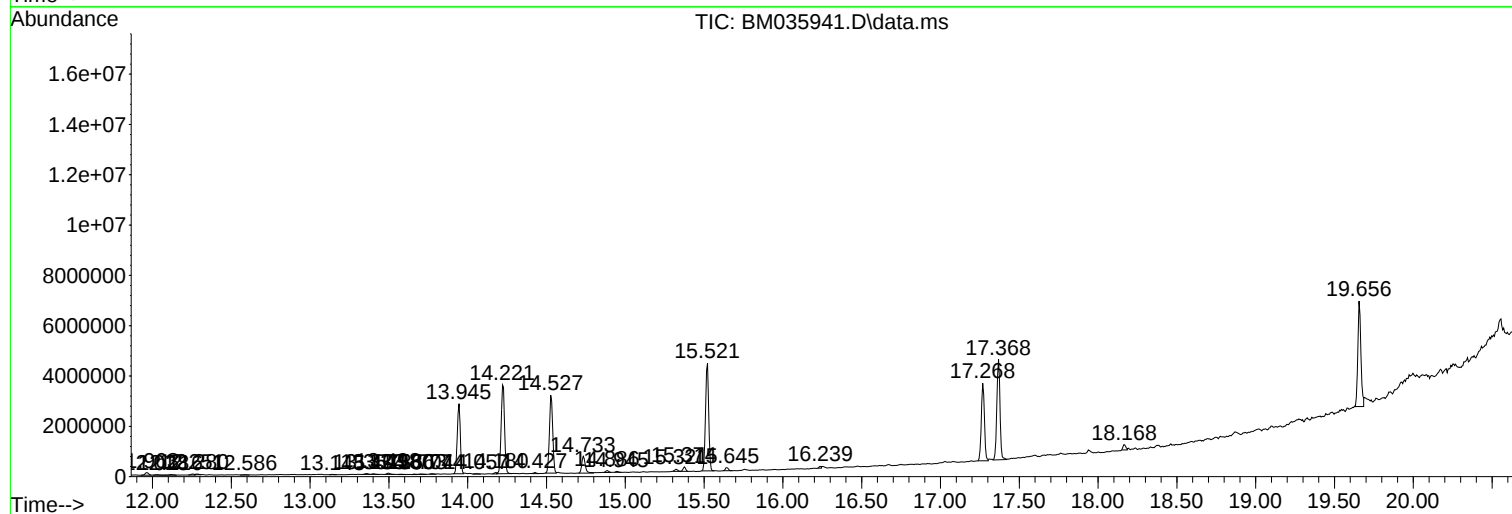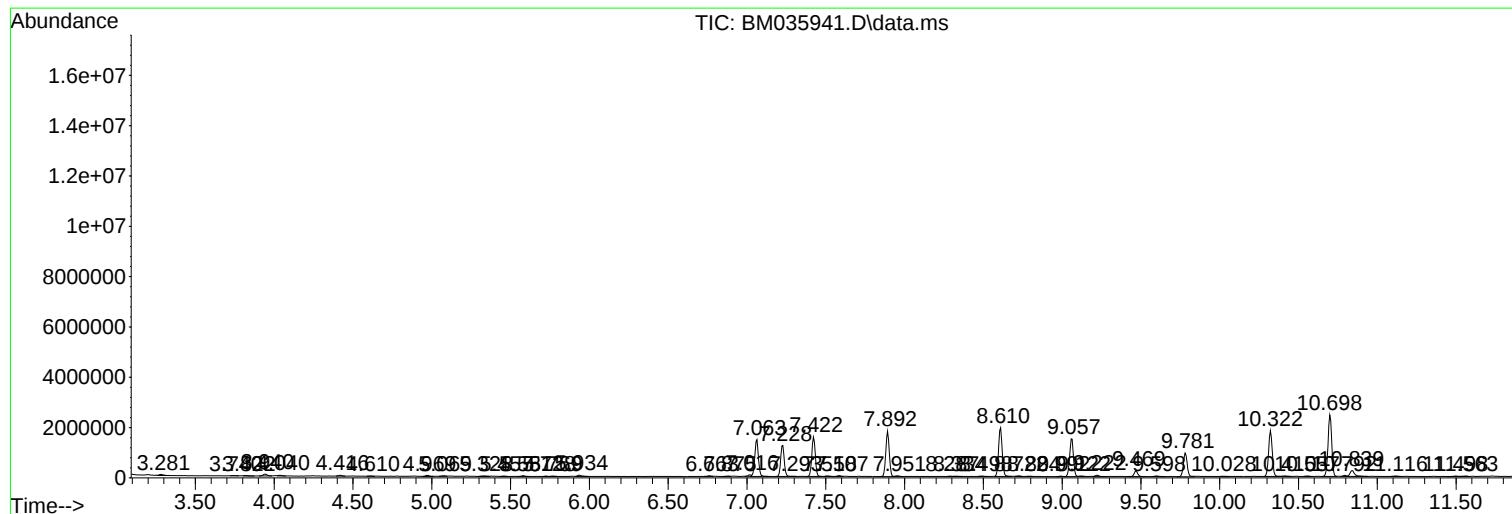

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035941.D
Acq On : 27 Jul 2022 00:23
Operator : CG/JU
Sample : N3709-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0B28

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072622\
Data File : BM035941.D
Acq On : 27 Jul 2022 00:23
Operator : CG/JU
Sample : N3709-14
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0B28

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM072522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc