




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
Data File : BM046849.D
Acq On : 27 Jul 2024 03:06
Operator : MA/JU
Sample : PB162152BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Manual IntegrationsAPPROVED

Quant Time: Jul 27 03:38:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 08/05/2024

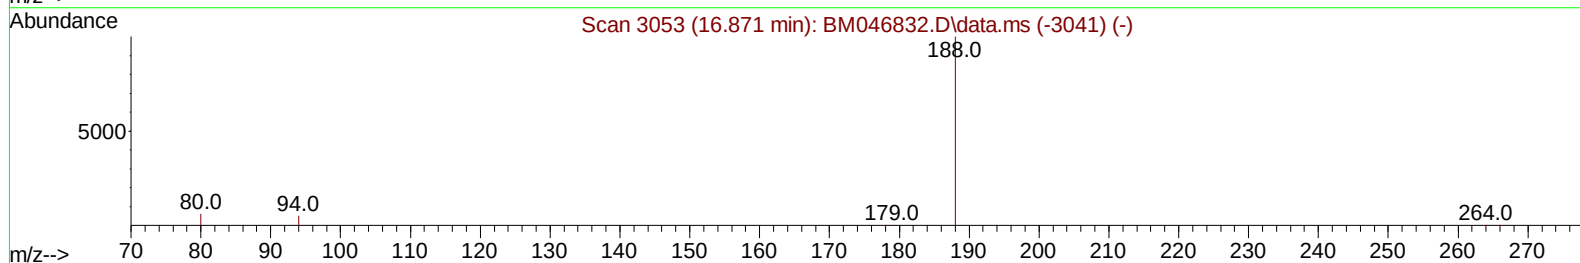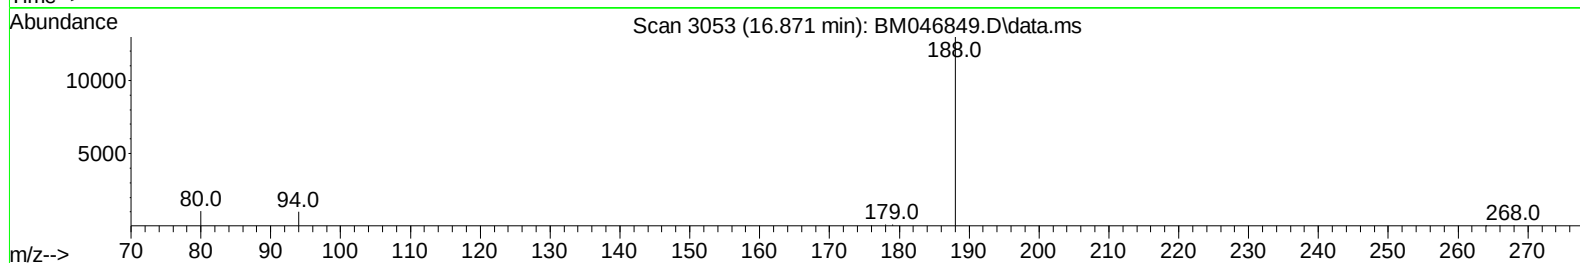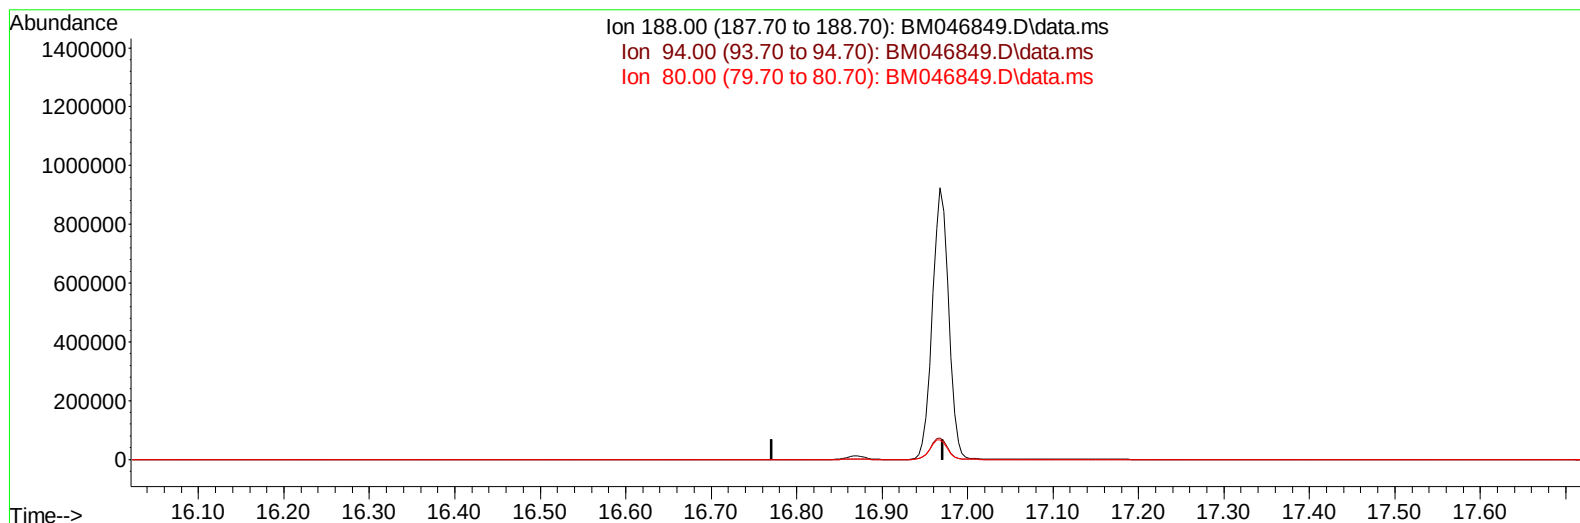

TIC: BM046849.D\data.ms

(13) Phenanthrene-d10 (I)

16.871min (-16.871) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.60	0.00#
80.00	6.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
Data File : BM046849.D
Acq On : 27 Jul 2024 03:06
Operator : MA/JU
Sample : PB162152BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Manual IntegrationsAPPROVED

Quant Time: Jul 27 03:38:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 08/05/2024

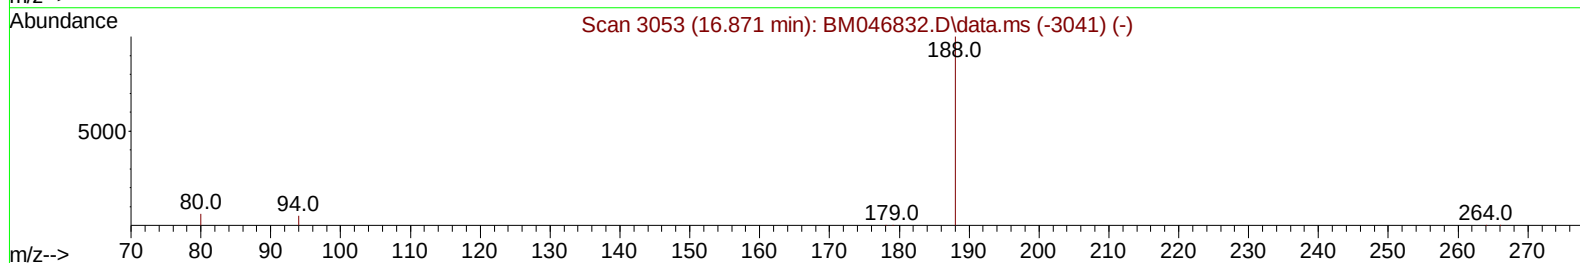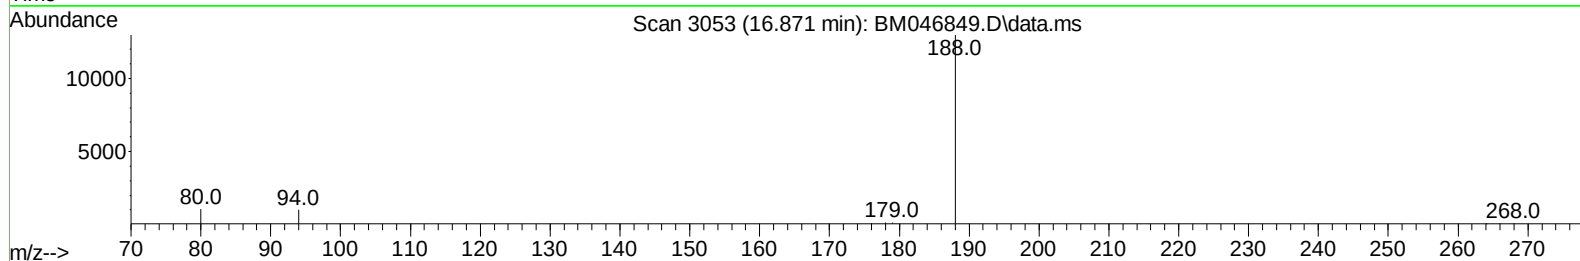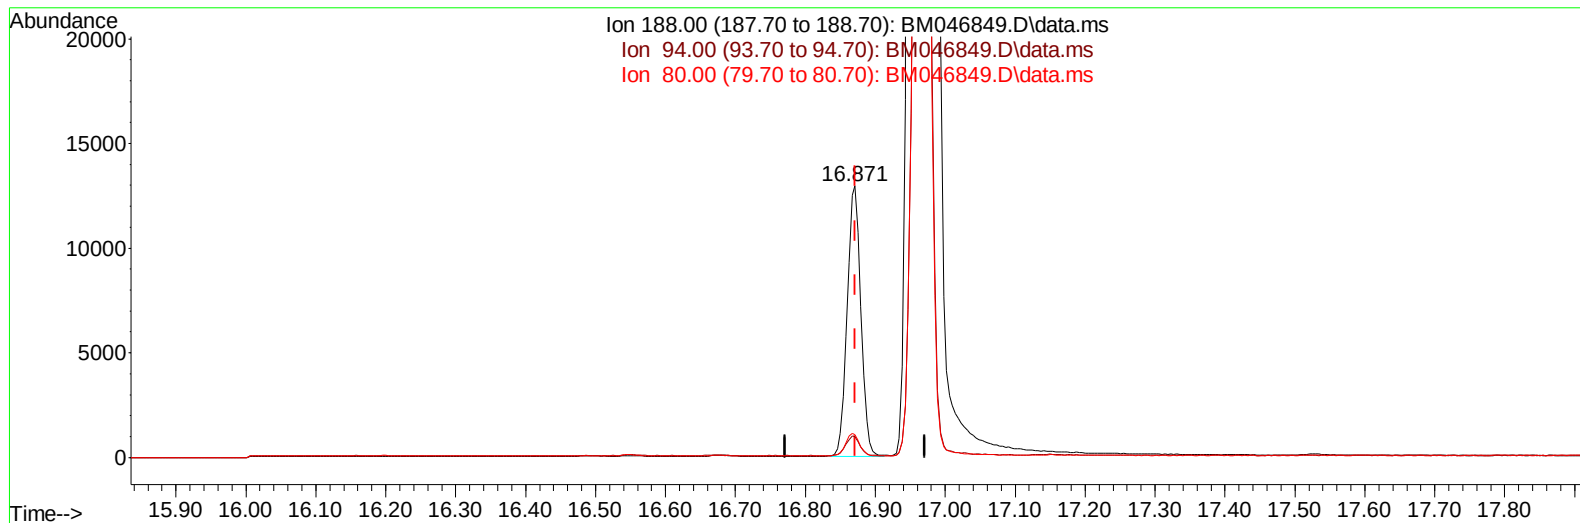

TIC: BM046849.D\data.ms

(13) Phenanthrene-d10 (I)

16.871min (-0.000) 0.40 ng/ul m

response 17597

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.60	7.75
80.00	6.30	8.33#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
Data File : BM046849.D
Acq On : 27 Jul 2024 03:06
Operator : MA/JU
Sample : PB162152BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Manual IntegrationsAPPROVED

Quant Time: Jul 27 03:38:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 08/05/2024

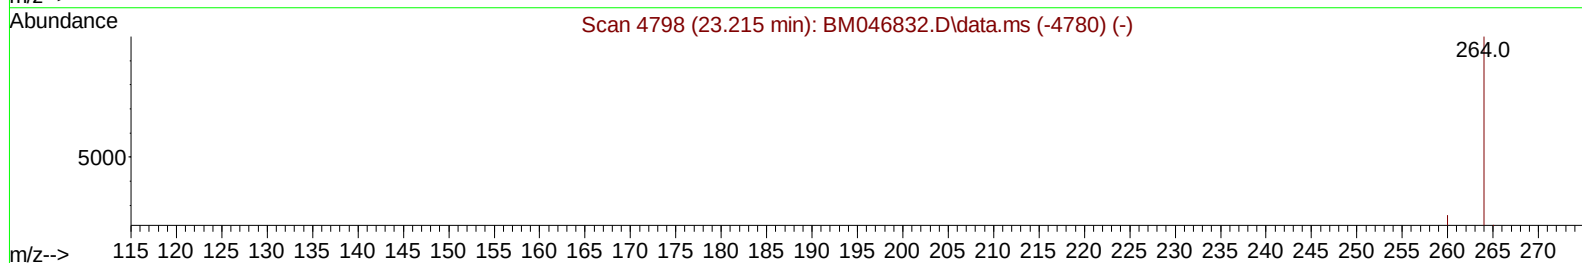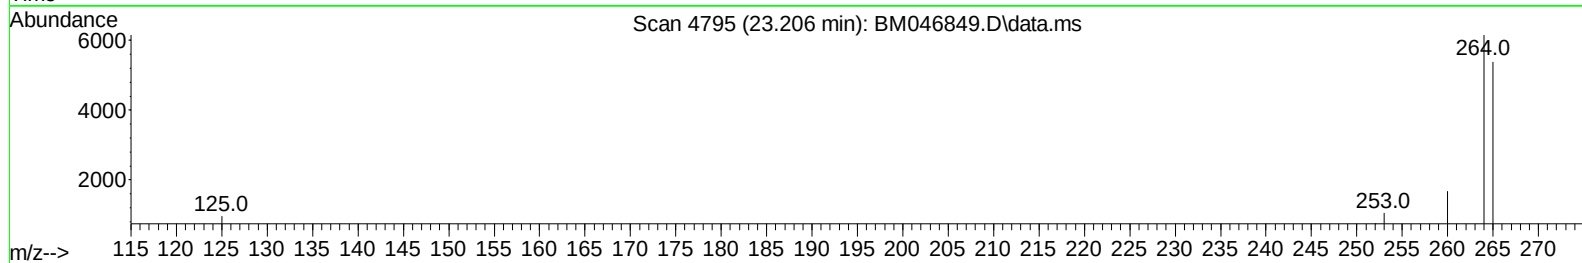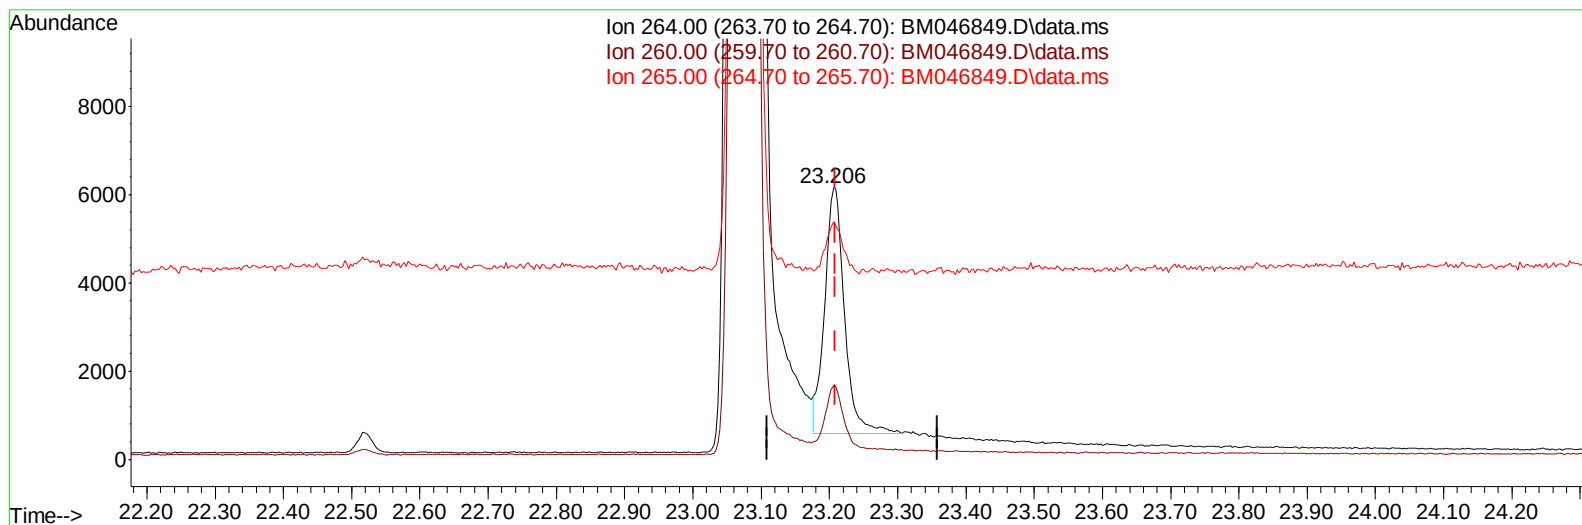

TIC: BM046849.D\data.ms

(23) Perylene-d12 (I)

23.206min (-0.003) 0.40 ng/u1

response 11226

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	27.23
265.00	89.90	87.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
Data File : BM046849.D
Acq On : 27 Jul 2024 03:06
Operator : MA/JU
Sample : PB162152BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Manual IntegrationsAPPROVED

Quant Time: Jul 27 03:38:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 08/05/2024

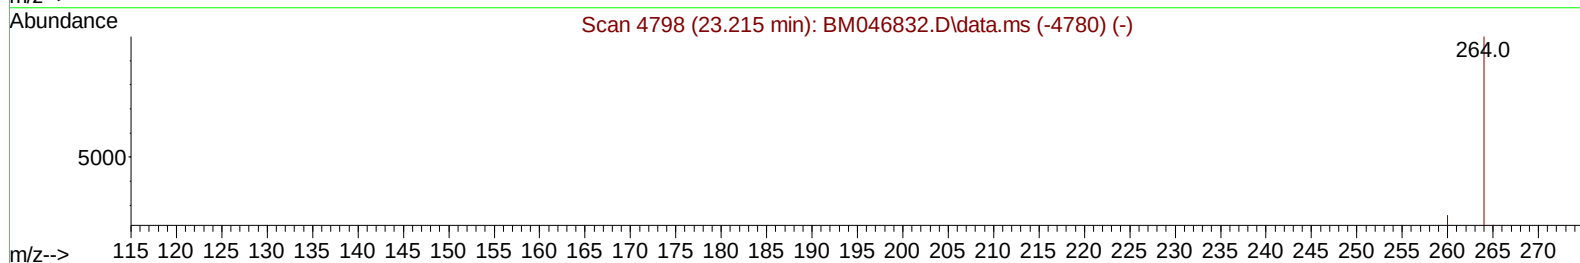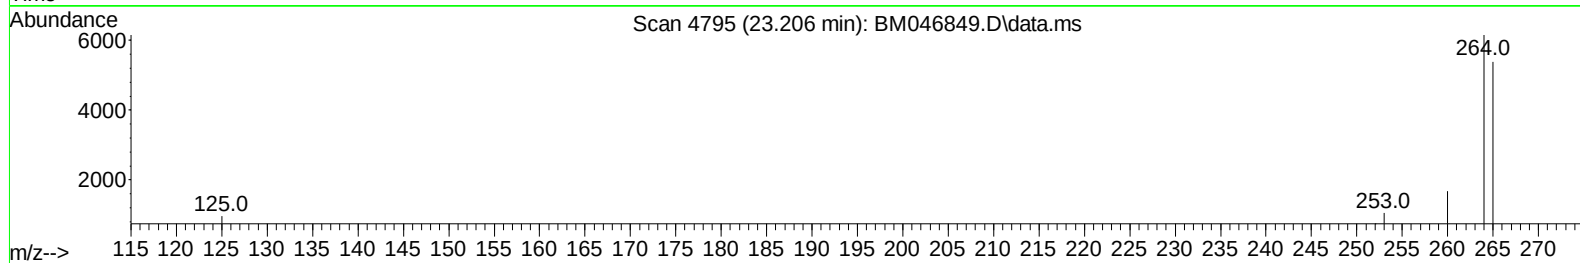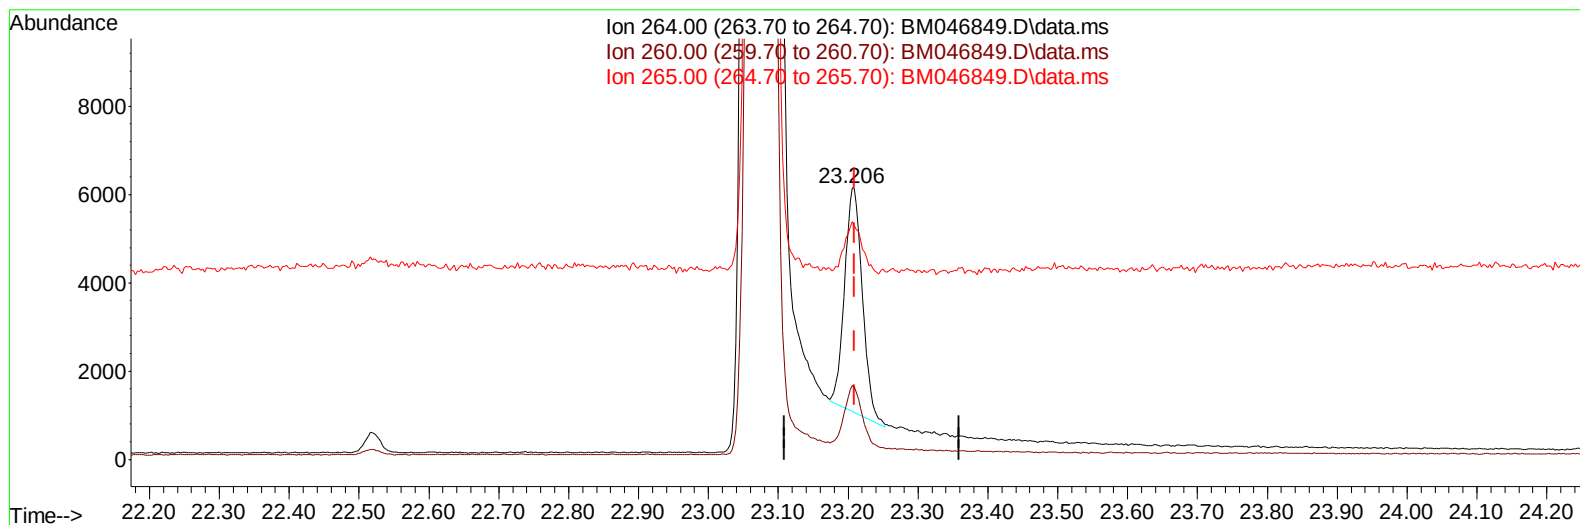

TIC: BM046849.D\data.ms

(23) Perylene-d12 (I)

23.206min (-0.003) 0.40 ng/ul m

response 8911

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	27.23
265.00	89.90	87.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
 Data File : BM046849.D
 Acq On : 27 Jul 2024 03:06
 Operator : MA/JU
 Sample : PB162152BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK152

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/27/2024
 Supervised By :mohammad ahmed 08/05/2024

Quant Time: Jul 27 03:38:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 24 15:10:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.468	152	3211	0.400	ng/ul	0.00
4) Naphthalene-d8	10.221	136	9342	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.113	164	5969	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.871	188	17597m	0.400	ng/ul	0.00
17) Chrysene-d12	21.081	240	9380	0.400	ng/ul	# 0.00
23) Perylene-d12	23.206	264	8911m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.096	96	13618	6.057	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.822	152	4951	0.333	ng/ul	0.00
18) Fluoranthene-d10	18.909	212	12087	0.396	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
Data File : BM046849.D
Acq On : 27 Jul 2024 03:06
Operator : MA/JU
Sample : PB162152BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK152

Manual IntegrationsAPPROVED

Quant Time: Jul 27 03:38:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 08/05/2024

