




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
Data File : BM046876.D
Acq On : 27 Jul 2024 20:08
Operator : MA/JU
Sample : P3300-23
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1GD2

Manual IntegrationsAPPROVED

Quant Time: Jul 28 23:32:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :mohammad ahmed 08/05/2024

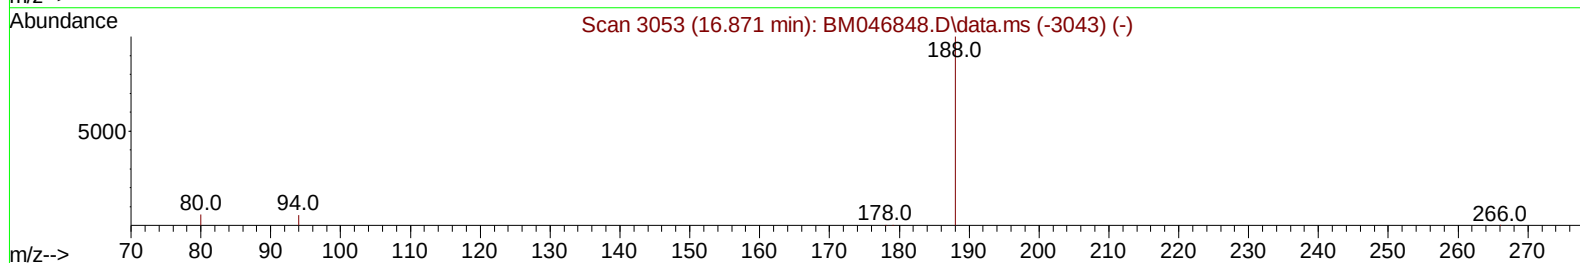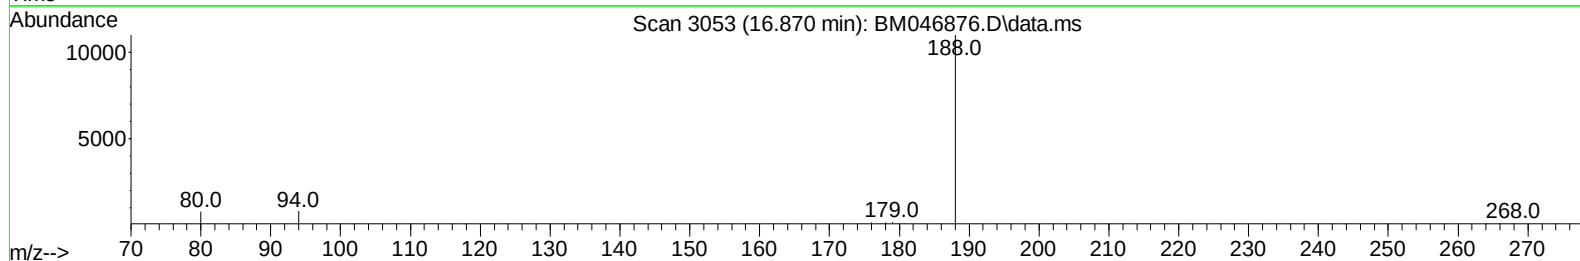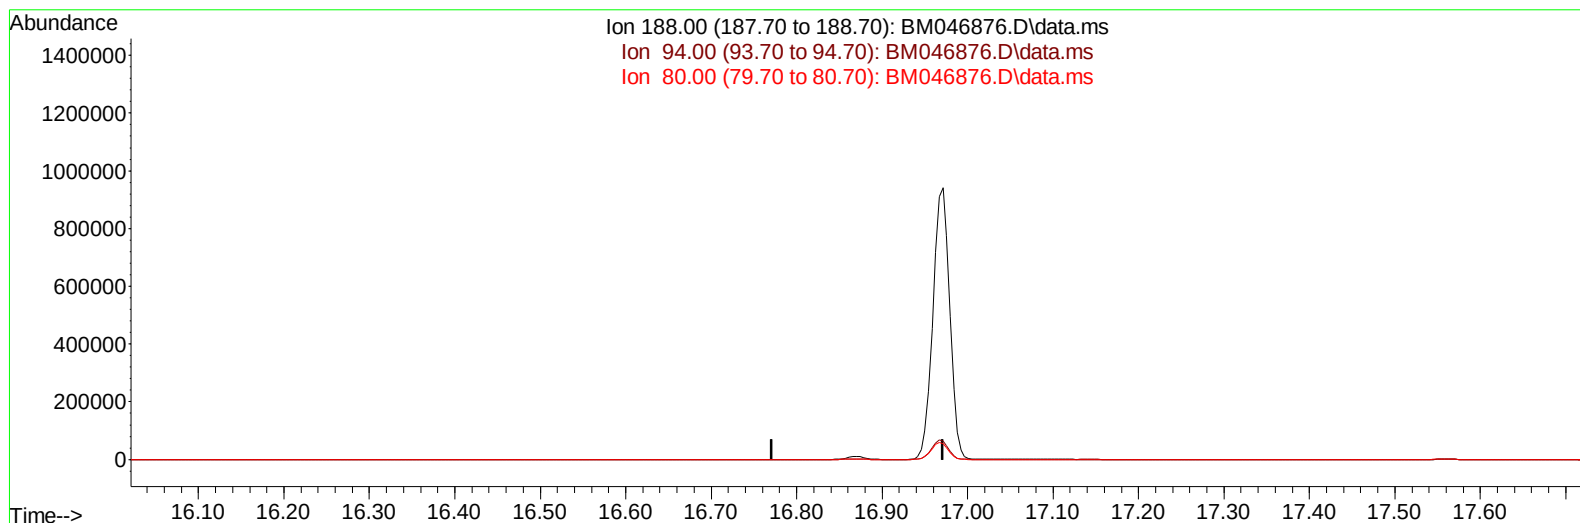

TIC: BM046876.D\data.ms

(13) Phenanthrene-d10 (I)

16.871min (-16.871) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.60	0.00#
80.00	6.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
Data File : BM046876.D
Acq On : 27 Jul 2024 20:08
Operator : MA/JU
Sample : P3300-23
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1GD2

Manual IntegrationsAPPROVED

Quant Time: Jul 28 23:32:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :mohammad ahmed 08/05/2024

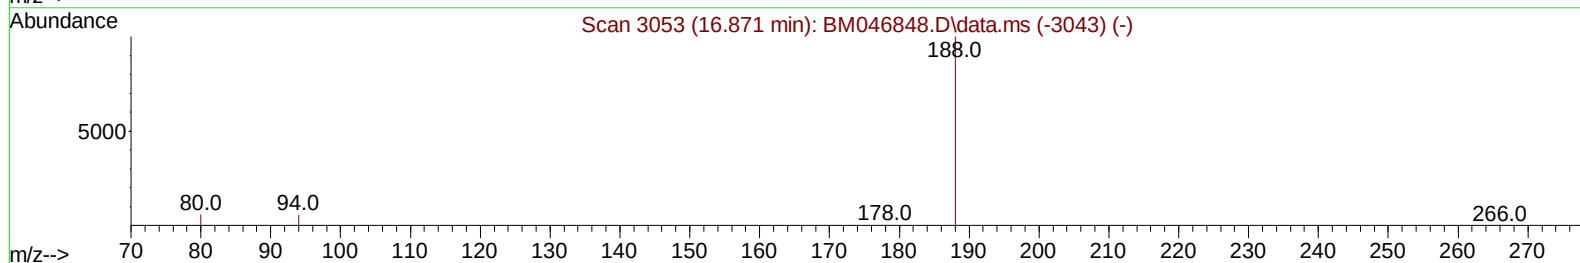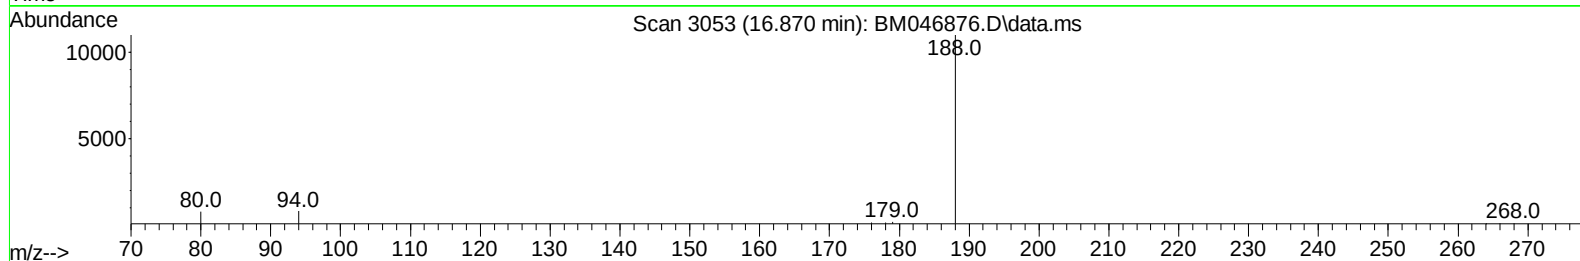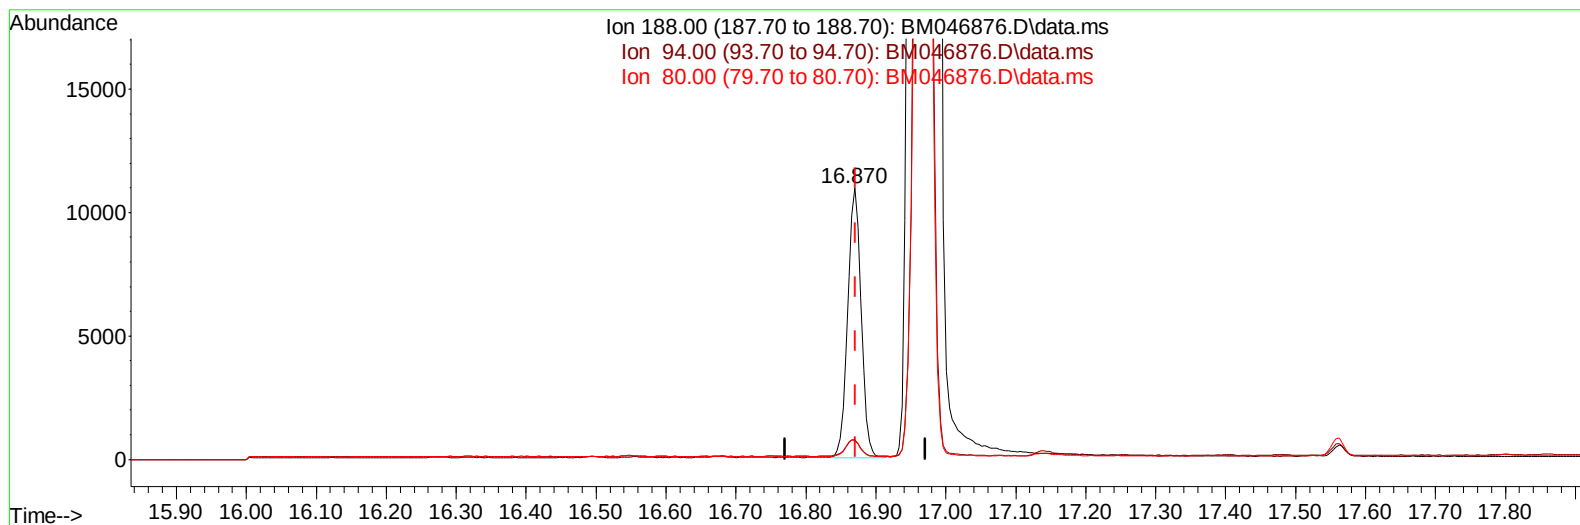

TIC: BM046876.D\data.ms

(13) Phenanthrene-d10 (I)

16.870min (-0.001) 0.40 ng/ul m

response 14600

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.60	7.21
80.00	6.30	7.06
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
Data File : BM046876.D
Acq On : 27 Jul 2024 20:08
Operator : MA/JU
Sample : P3300-23
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1GD2

Manual IntegrationsAPPROVED

Quant Time: Jul 28 23:32:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :mohammad ahmed 08/05/2024

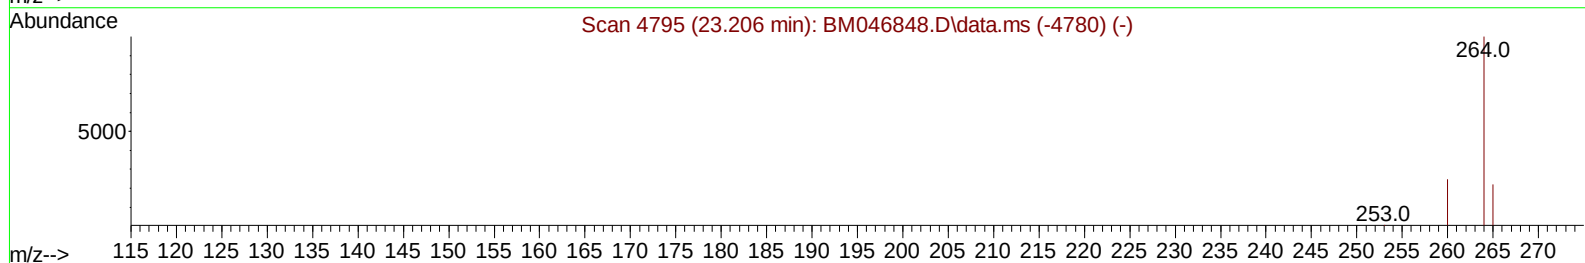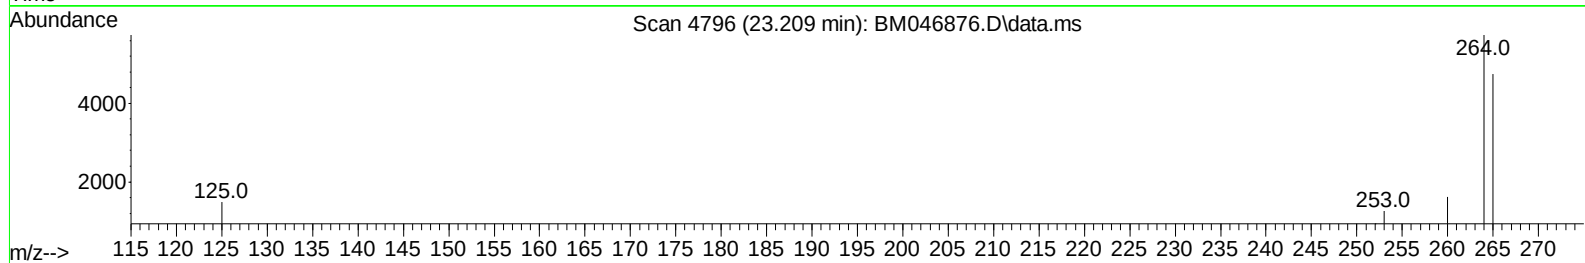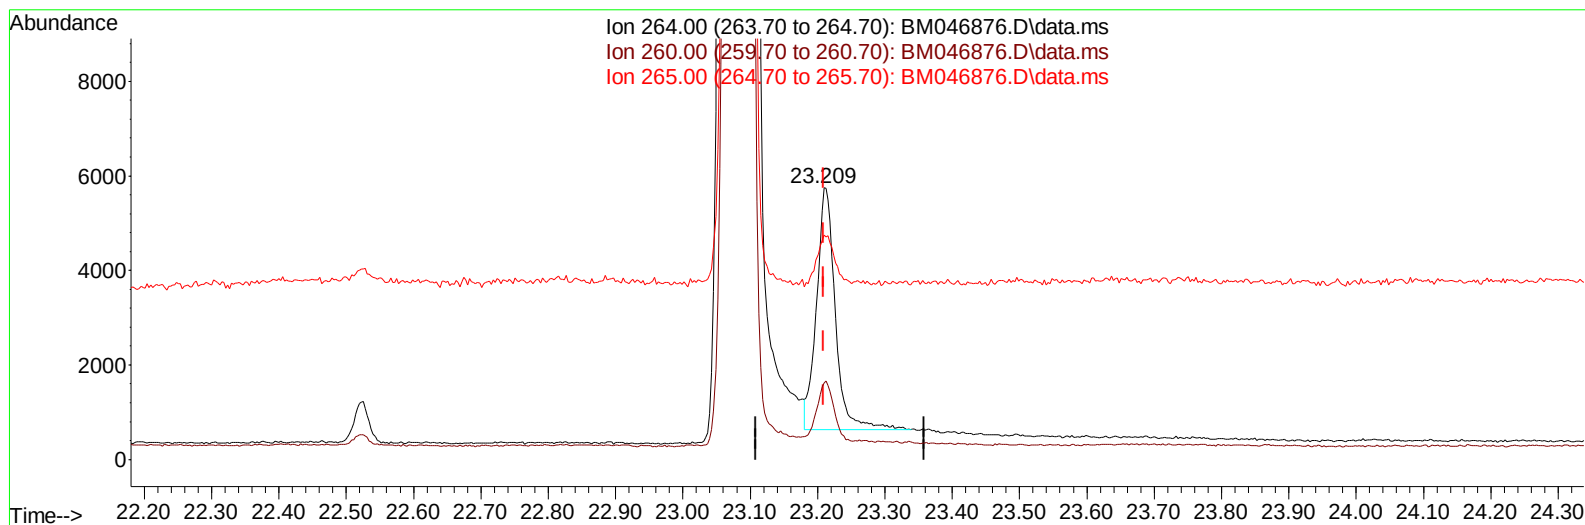

TIC: BM046876.D\data.ms

(23) Perylene-d12 (I)

23.209min (+ 0.001) 0.40 ng/u1

response 9983

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	28.27
265.00	89.90	82.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
Data File : BM046876.D
Acq On : 27 Jul 2024 20:08
Operator : MA/JU
Sample : P3300-23
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1GD2

Manual IntegrationsAPPROVED

Quant Time: Jul 28 23:32:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :mohammad ahmed 08/05/2024

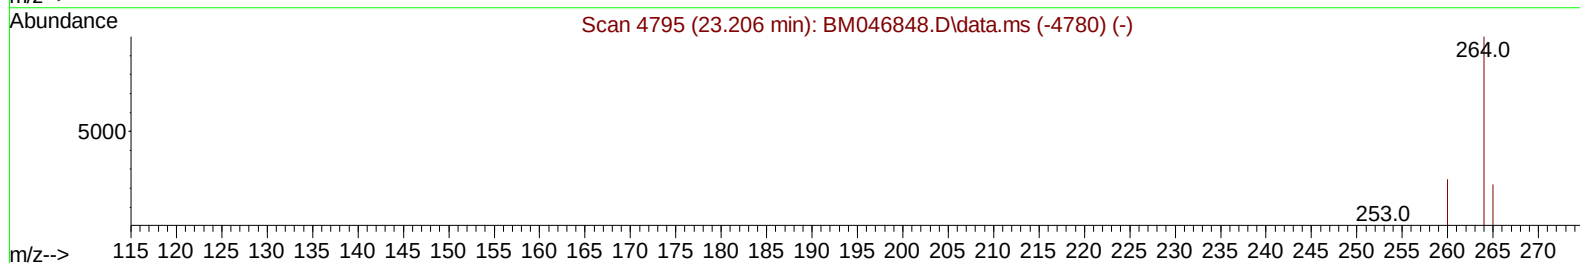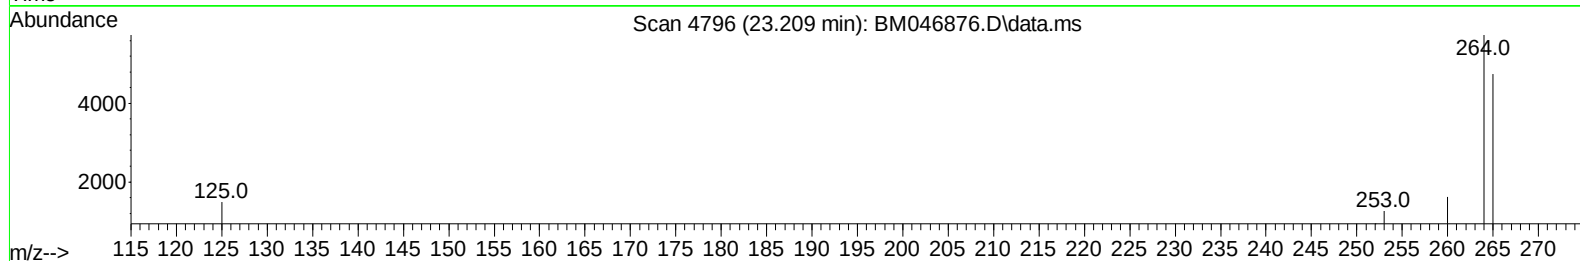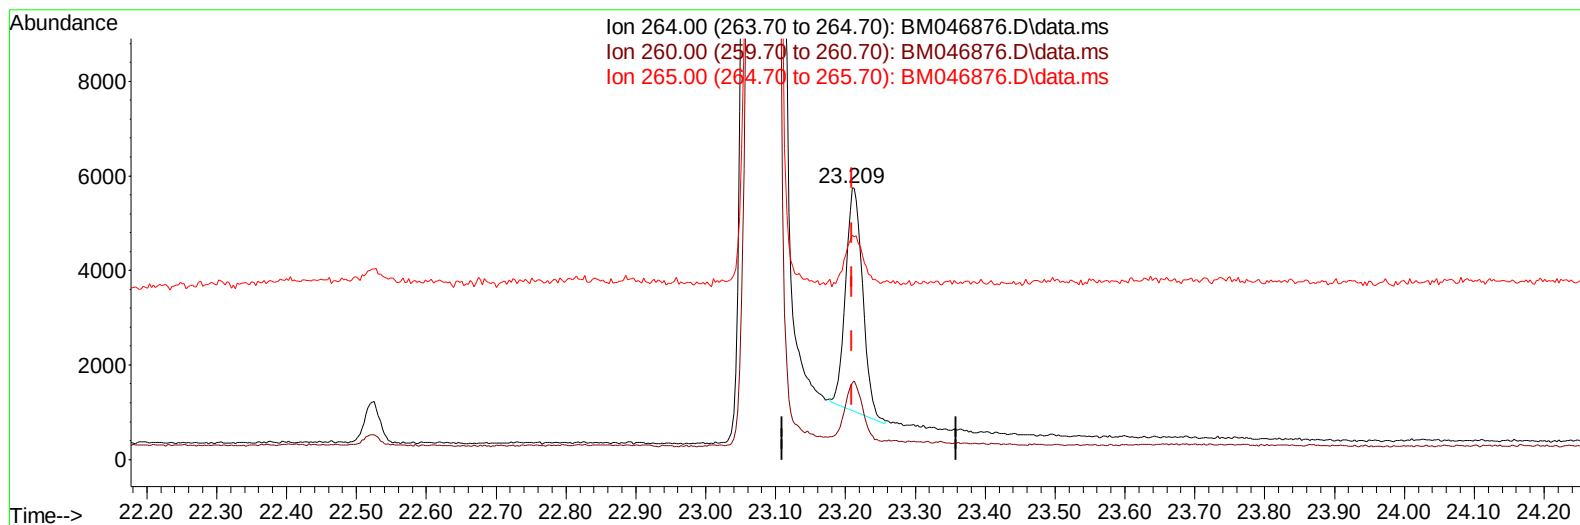

TIC: BM046876.D\data.ms

(23) Perylene-d12 (I)

23.209min (+ 0.001) 0.40 ng/ul m

response 7991

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.10	28.27
265.00	89.90	82.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
 Data File : BM046876.D
 Acq On : 27 Jul 2024 20:08
 Operator : MA/JU
 Sample : P3300-23
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1GD2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/29/2024
 Supervised By :mohammad ahmed 08/05/2024

Quant Time: Jul 28 23:32:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 24 15:10:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.464	152	4382	0.400	ng/ul	0.00
4) Naphthalene-d8	10.220	136	12884	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.112	164	7936	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.870	188	14600m	0.400	ng/ul	0.00
17) Chrysene-d12	21.082	240	7682	0.400	ng/ul	# 0.00
23) Perylene-d12	23.209	264	7991m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.092	96	13070	4.260	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.821	152	8535	0.417	ng/ul	0.00
18) Fluoranthene-d10	18.908	212	12631	0.505	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.270	128	2271	0.070	ng/ul#	93
7) 2-Methylnaphthalene	11.898	142	497	0.022	ng/ul	94
19) Fluoranthene	18.940	202	791	0.023	ng/ul#	56

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
Data File : BM046876.D
Acq On : 27 Jul 2024 20:08
Operator : MA/JU
Sample : P3300-23
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1GD2

Manual IntegrationsAPPROVED

Quant Time: Jul 28 23:32:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :mohammad ahmed 08/05/2024

