

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
 Data File : BM046835.D
 Acq On : 26 Jul 2024 17:55
 Operator : MA/JU
 Sample : P3325-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B32

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/27/2024
 Supervised By :mohammad ahmed 08/05/2024

Quant Time: Jul 26 18:25:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 24 15:10:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.468	152	2694	0.400	ng/ul	0.00
4) Naphthalene-d8	10.226	136	7449	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.112	164	4685	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.870	188	9795m	0.400	ng/ul	0.00
17) Chrysene-d12	21.082	240	6211	0.400	ng/ul	0.00
23) Perylene-d12	23.206	264	6087m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.096	96	9079	4.813	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.826	152	4668	0.394	ng/ul	0.00
18) Fluoranthene-d10	18.908	212	9725	0.481	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.130	88	3297	1.528	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
Data File : BM046835.D
Acq On : 26 Jul 2024 17:55
Operator : MA/JU
Sample : P3325-04
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0B32

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/27/2024
Supervised By :mohammad ahmed 08/05/2024


Quant Time: Jul 26 18:25:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

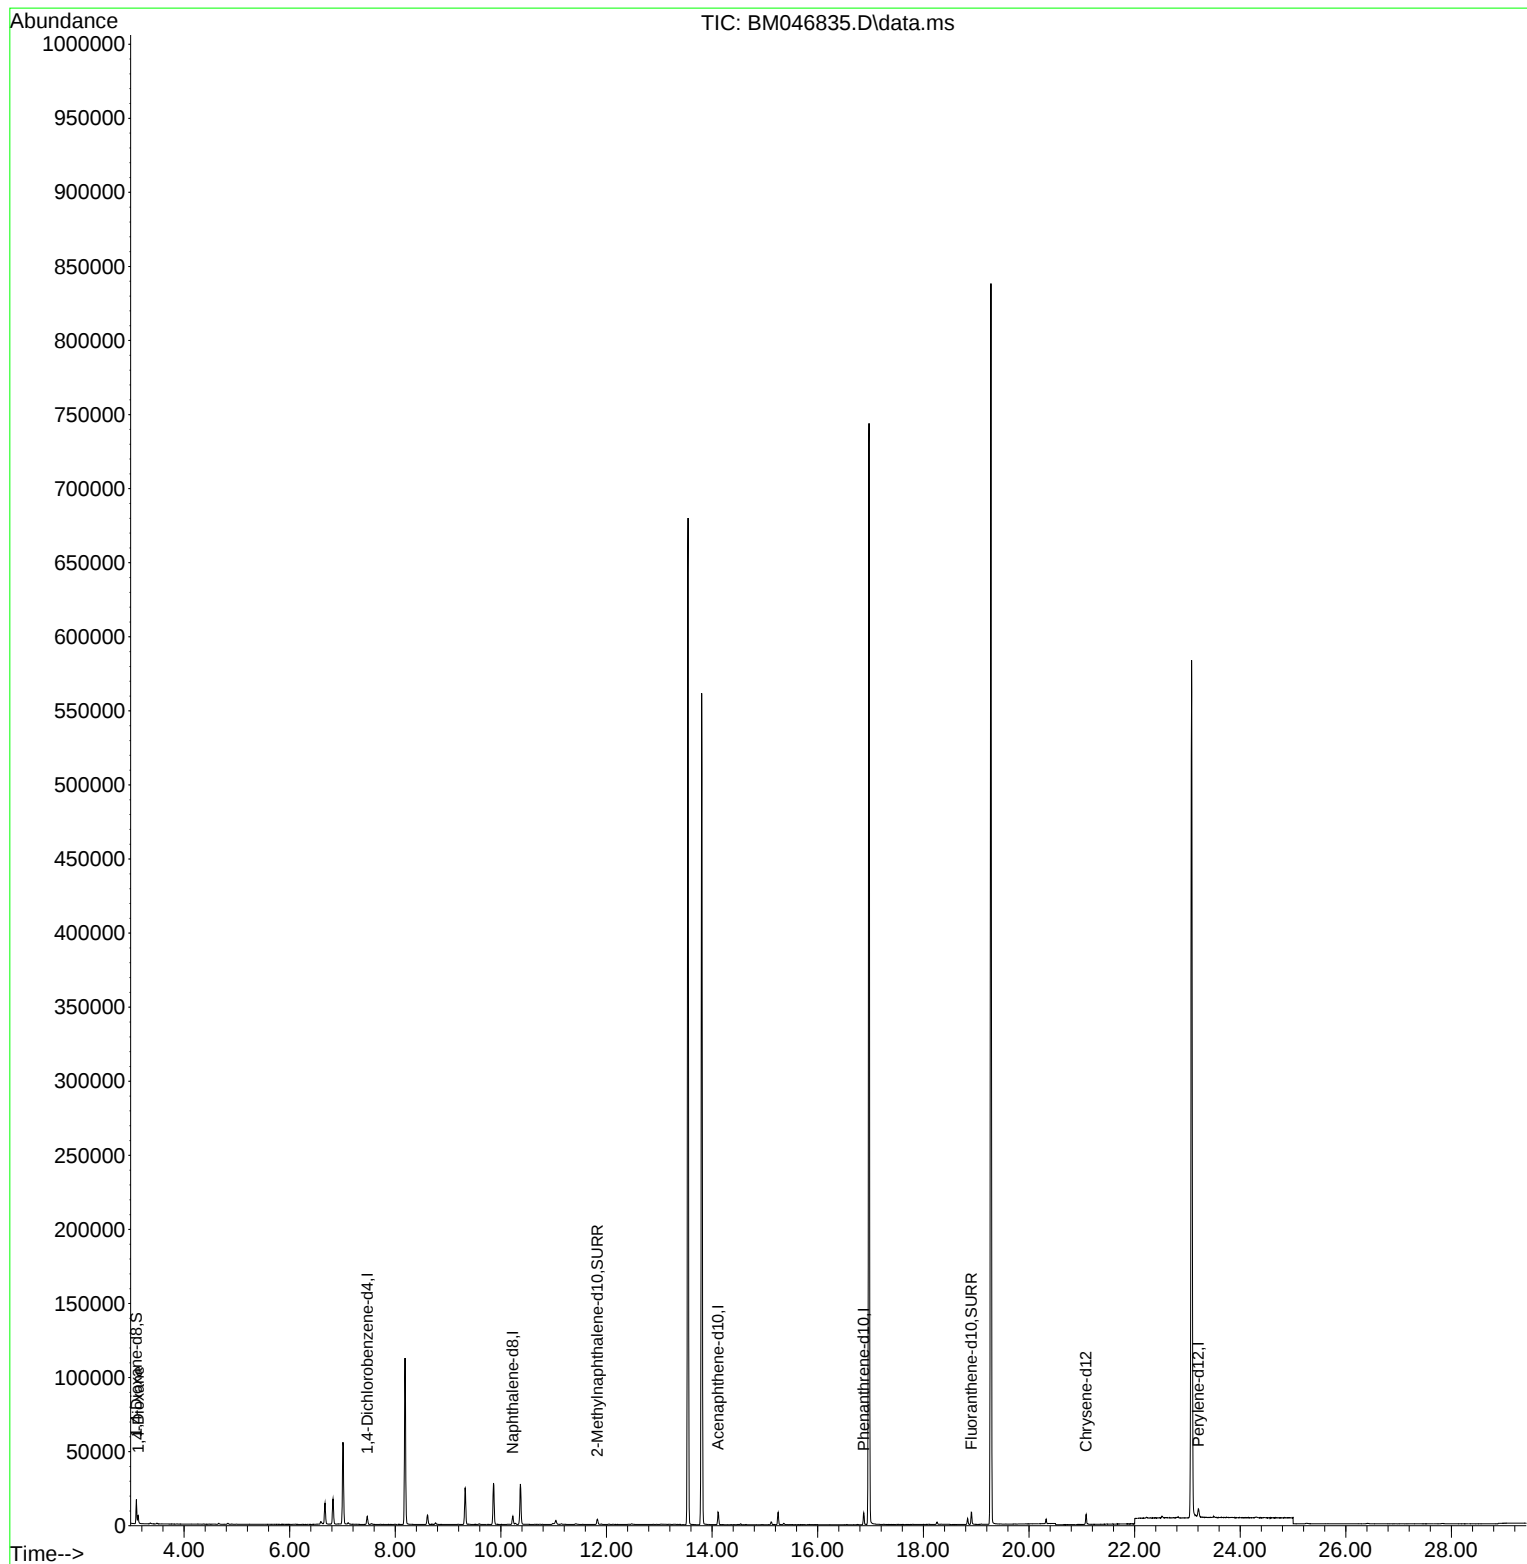

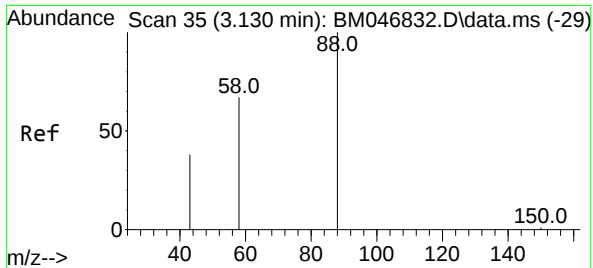

#2
 1,4-Dioxane
 Concen: 1.528 ng/ul
 RT: 3.130 min Scan# 31
 Delta R.T. -0.009 min
 Lab File: BM046835.D
 Acq: 26 Jul 2024 17:55

Instrument :
 BNA_M
 ClientSampleId :
 C0B32

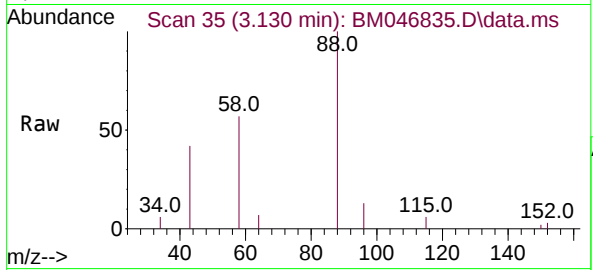

Tgt Ion: 88 Resp: 329

Ion	Ratio	Lower	Upper
88	100		
43	41.8	42.1	63.1
58	56.7	38.3	57.5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/27/2024
 Supervised By :mohammad ahmed 08/05/2024

