

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
 Data File : BM046862.D
 Acq On : 27 Jul 2024 11:01
 Operator : MA/JU
 Sample : P3329-19
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7E85

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/29/2024
 Supervised By :mohammad ahmed 08/05/2024

Quant Time: Jul 28 23:29:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 24 15:10:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.464	152	4024	0.400	ng/ul	0.00
4) Naphthalene-d8	10.220	136	11781	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.108	164	7485	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.866	188	14570m	0.400	ng/ul	0.00
17) Chrysene-d12	21.079	240	7083	0.400	ng/ul	# 0.00
23) Perylene-d12	23.204	264	6790m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.092	96	13189	4.681	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.821	152	6826	0.365	ng/ul	0.00
18) Fluoranthene-d10	18.908	212	12048	0.522	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.270	128	2078	0.070	ng/ul#	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072624\
Data File : BM046862.D
Acq On : 27 Jul 2024 11:01
Operator : MA/JU
Sample : P3329-19
Misc :
ALS Vial : 43 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F7E85

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :mohammad ahmed 08/05/2024


Quant Time: Jul 28 23:29:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

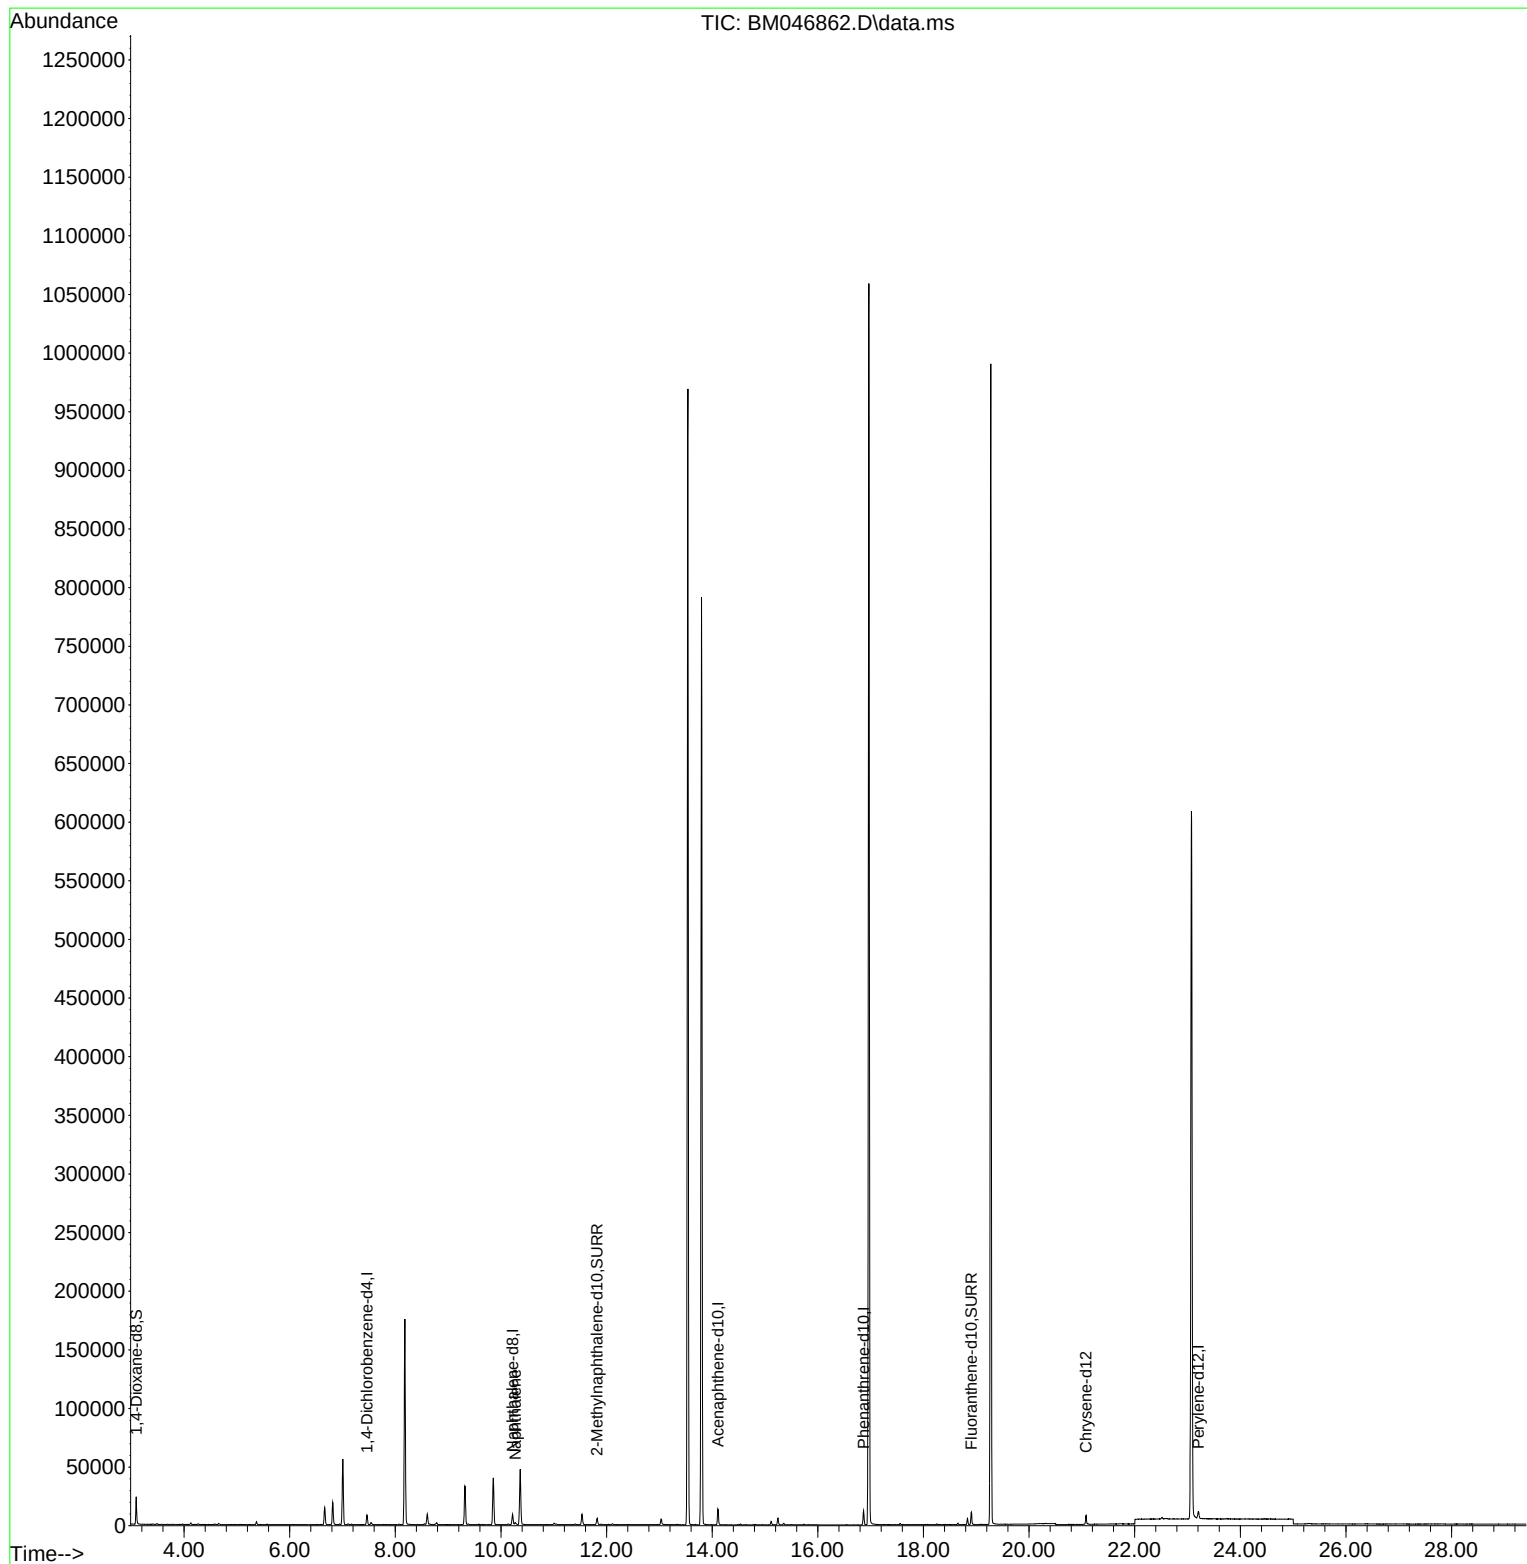

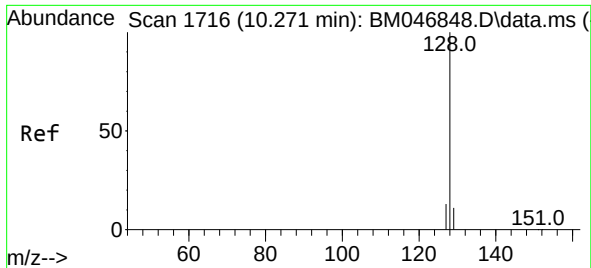

#5
Naphthalene
Concen: 0.070 ng/ul
RT: 10.270 min Scan# 11
Delta R.T. -0.007 min
Lab File: BM046862.D
Acq: 27 Jul 2024 11:01

Instrument :
BNA_M
ClientSampleId :
F7E85

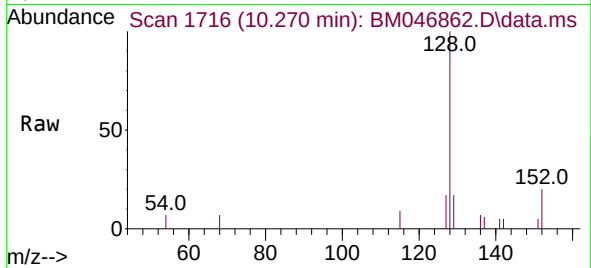

Tgt Ion:128 Resp: 2078
Ion Ratio Lower Upper
128 100
129 16.9 10.1 15.1
127 17.3 11.5 17.3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :mohammad ahmed 08/05/2024

